

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071918\
 Data File : VU025519.D
 Acq On : 19 Jul 2018 14:10
 Operator : MD/SY
 Sample : VIBLK45
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK45

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071718WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.680	27	28	29	rBV	223	73	0.01%	0.001%
2	0.741	44	47	49	rVB2	194	96	0.01%	0.001%
3	0.789	60	62	64	rBV	303	168	0.01%	0.003%
4	0.831	69	75	77	rBV3	298	279	0.02%	0.004%
5	0.870	86	87	90	rBV2	195	87	0.01%	0.001%
6	0.886	90	92	93	rBV	104	43	0.00%	0.001%
7	0.912	93	100	101	rBV2	267	235	0.02%	0.004%
8	0.931	104	106	108	rVV2	139	65	0.01%	0.001%
9	0.963	113	116	119	rBV	237	170	0.01%	0.003%
10	0.976	119	120	121	rBV	129	35	0.00%	0.001%
11	0.992	122	125	127	rVB2	197	109	0.01%	0.002%
12	1.008	128	130	132	rVB2	177	55	0.00%	0.001%
13	1.024	132	135	137	rBV2	275	207	0.02%	0.003%
14	1.092	147	156	177	rBV	1127871	1264707	100.00%	19.741%
15	1.404	247	253	263	rBV	59130	59172	4.68%	0.924%
16	1.687	334	341	357	rVB	53862	67695	5.35%	1.057%
17	2.278	516	525	538	rVB	115064	174532	13.80%	2.724%
18	2.651	639	641	643	rBV	352	177	0.01%	0.003%
19	2.709	651	659	667	rBV4	1381	1736	0.14%	0.027%
20	2.979	739	743	744	rBV3	736	513	0.04%	0.008%
21	3.037	759	761	763	rBV	221	108	0.01%	0.002%
22	3.063	767	769	773	rBV2	288	205	0.02%	0.003%
23	3.082	773	775	782	rVB	476	357	0.03%	0.006%
24	3.124	783	788	790	rBV3	324	297	0.02%	0.005%
25	3.198	808	811	813	rBV	194	116	0.01%	0.002%
26	3.217	813	817	819	rBV	308	257	0.02%	0.004%
27	3.413	875	878	879	rBV2	231	155	0.01%	0.002%
28	3.500	903	905	906	rBV	291	122	0.01%	0.002%
29	3.561	922	924	928	rVB2	514	298	0.02%	0.005%
30	3.587	928	932	935	rBV3	380	319	0.03%	0.005%
31	3.632	943	946	948	rVB3	200	102	0.01%	0.002%
32	3.686	959	963	967	rBV3	380	370	0.03%	0.006%
33	3.719	970	973	975	rBV2	213	137	0.01%	0.002%
34	3.735	976	978	983	rVB2	364	317	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U071918\
 Data File : VU025519.D
 Acq On : 19 Jul 2018 14:10
 Operator : MD/SY
 Sample : VIBLK45
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK45

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071718WMA.M
 Title : VOC Analysis

35	3.773	986	990	992	rBV	255	225	0.002%	0.004%
36	3.873	1019	1021	1022	rBV	204	81	0.001%	0.001%
37	3.931	1037	1039	1042	rBV2	179	131	0.001%	0.002%
38	3.998	1059	1060	1063	rVB	339	124	0.001%	0.002%
39	4.014	1063	1065	1068	rBV2	327	219	0.002%	0.003%
40	4.066	1077	1081	1084	rBV	297	237	0.002%	0.004%
41	4.121	1092	1098	1099	rBV	456	359	0.003%	0.006%
42	4.175	1100	1115	1147	rVV2	55068	166171	13.14%	2.594%
43	4.458	1200	1203	1204	rBV2	381	240	0.002%	0.004%
44	4.651	1246	1263	1281	rBV	114751	267141	21.12%	4.170%
45	4.918	1343	1346	1352	rVB2	353	316	0.002%	0.005%
46	4.957	1352	1358	1362	rBV	418	428	0.003%	0.007%
47	4.979	1362	1365	1366	rBV	425	185	0.001%	0.003%
48	5.146	1413	1417	1420	rVB2	280	186	0.001%	0.003%
49	5.166	1421	1423	1424	rBV	258	80	0.001%	0.001%
50	5.217	1436	1439	1442	rBV2	353	277	0.002%	0.004%
51	5.346	1455	1479	1500	rBV2	201809	616126	48.72%	9.617%
52	5.545	1539	1541	1545	rVB	226	159	0.001%	0.002%
53	5.661	1574	1577	1579	rVB2	309	137	0.001%	0.002%
54	5.683	1581	1584	1588	rBV2	563	567	0.004%	0.009%
55	5.764	1606	1609	1610	rBV	230	122	0.001%	0.002%
56	5.796	1617	1619	1620	rBV	202	78	0.001%	0.001%
57	5.889	1634	1648	1672	rBV	254563	500927	39.61%	7.819%
58	6.146	1724	1728	1731	rBV3	541	520	0.004%	0.008%
59	6.182	1735	1739	1740	rBV2	1448	942	0.007%	0.015%
60	6.252	1758	1761	1764	rBV3	175	126	0.001%	0.002%
61	6.333	1772	1786	1805	rBV	147728	296103	23.41%	4.622%
62	6.448	1819	1822	1823	rBV2	776	325	0.003%	0.005%
63	6.500	1833	1838	1840	rBV2	328	276	0.002%	0.004%
64	6.625	1870	1877	1880	rBV3	365	393	0.003%	0.006%
65	6.754	1911	1917	1919	rBV2	349	392	0.003%	0.006%
66	6.789	1926	1928	1932	rBV2	436	306	0.002%	0.005%
67	6.841	1941	1944	1945	rBV	885	478	0.004%	0.007%
68	6.889	1956	1959	1963	rVB2	316	248	0.002%	0.004%
69	6.950	1975	1978	1980	rBV2	331	197	0.002%	0.003%
70	6.998	1990	1993	1995	rBV2	236	142	0.001%	0.002%
71	7.014	1995	1998	1999	rBV	133	65	0.001%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071918\
 Data File : VU025519.D
 Acq On : 19 Jul 2018 14:10
 Operator : MD/SY
 Sample : VIBLK45
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK45

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071718WMA.M
 Title : VOC Analysis

72	7.091	2019	2022	2028	rBV	273	292	0.02%	0.005%
73	7.230	2052	2065	2088	rBV	81811	146516	11.58%	2.287%
74	7.567	2157	2170	2185	rBV	268960	456004	36.06%	7.118%
75	7.760	2228	2230	2231	rBV	329	125	0.01%	0.002%
76	7.854	2248	2259	2279	rVB2	59141	99449	7.86%	1.552%
77	7.963	2291	2293	2295	rBV2	308	204	0.02%	0.003%
78	8.037	2313	2316	2318	rBV2	327	149	0.01%	0.002%
79	8.181	2348	2361	2368	rBV3	5678	12450	0.98%	0.194%
80	8.310	2392	2401	2425	rVB	174886	301650	23.85%	4.708%
81	8.503	2458	2461	2465	rBV2	259	258	0.02%	0.004%
82	8.583	2484	2486	2490	rVB	394	179	0.01%	0.003%
83	8.609	2490	2494	2496	rBV2	489	419	0.03%	0.007%
84	8.783	2545	2548	2550	rBV2	336	198	0.02%	0.003%
85	8.844	2565	2567	2570	rBV3	297	244	0.02%	0.004%
86	8.976	2606	2608	2610	rBV	215	115	0.01%	0.002%
87	9.091	2632	2644	2664	rBV	348252	582377	46.05%	9.090%
88	9.345	2721	2723	2726	rVB2	338	146	0.01%	0.002%
89	9.490	2766	2768	2771	rVB2	339	137	0.01%	0.002%
90	9.866	2882	2885	2886	rBV	242	141	0.01%	0.002%
91	10.021	2929	2933	2934	rBV	320	236	0.02%	0.004%
92	10.162	2973	2977	2987	rVB4	931	1184	0.09%	0.018%
93	10.204	2987	2990	2991	rBV	409	247	0.02%	0.004%
94	10.435	3050	3062	3078	rBV	212575	345502	27.32%	5.393%
95	10.615	3110	3118	3133	rVB5	4729	9542	0.75%	0.149%
96	10.673	3133	3136	3137	rBV	351	189	0.01%	0.003%
97	11.355	3345	3348	3352	rBV	483	494	0.04%	0.008%
98	11.487	3377	3389	3406	rBV	343432	543274	42.96%	8.480%
99	11.863	3494	3506	3524	rBV	290684	476592	37.68%	7.439%


Sum of corrected areas: 6406656

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU071918\
Data File : VU025519.D
Acq On : 19 Jul 2018 14:10
Operator : MD/SY
Sample : VIBLK45
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK45

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071718WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

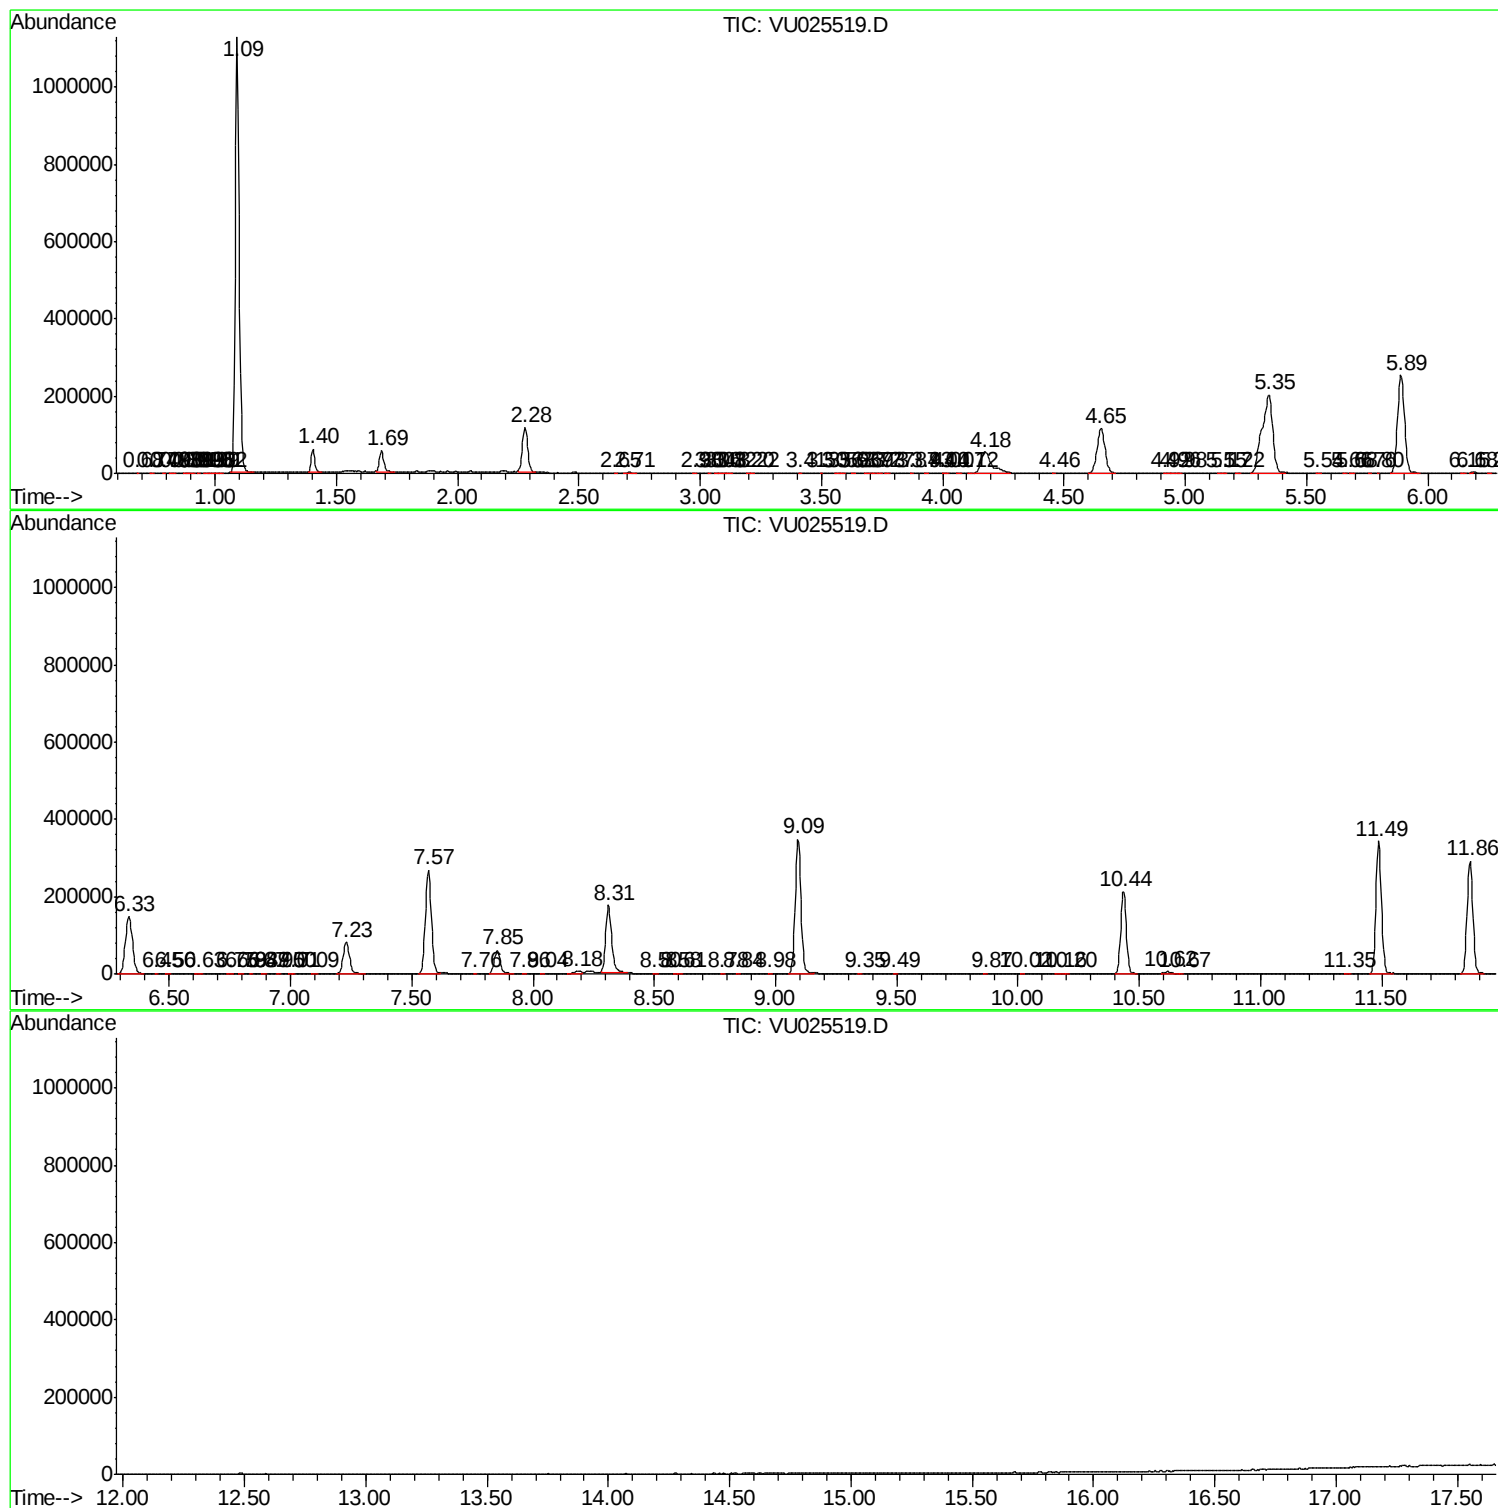

Data_Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU071918\
Data_File : VU025519.D
Acq_On : 19 Jul 2018 14:100
Operator : MD/SYY
Sample : VIBLK455
Misc : 5.0mL/MSVOA_U/WATER
ALS_Vial : 9 Sample_Multiplier: 11

Instrument :
MSVOA_U
ClientSampleId :
VIBLK45

Quant_Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071718WMA.MM
Quant_Title : VOC_Analysis

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
