

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071918\
 Data File : VU025521.D
 Acq On : 19 Jul 2018 14:56
 Operator : MD/SY
 Sample : J4065-13
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JHT42

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071718WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.609	3	6	8	rBV	231	121	0.01%	0.002%
2	0.625	8	11	19	rVB3	637	639	0.08%	0.009%
3	0.661	19	22	23	rBV2	221	136	0.02%	0.002%
4	0.683	27	29	32	rVV2	305	188	0.02%	0.003%
5	0.757	50	52	54	rBV	306	142	0.02%	0.002%
6	0.770	54	56	58	rBV	245	107	0.01%	0.002%
7	0.792	61	63	65	rVB	246	106	0.01%	0.002%
8	0.876	82	89	90	rBV2	189	141	0.02%	0.002%
9	0.886	90	92	96	rBV	322	229	0.03%	0.003%
10	0.934	103	107	109	rBV2	216	145	0.02%	0.002%
11	0.982	119	122	124	rBV2	273	186	0.02%	0.003%
12	1.092	135	156	174	rBV	145881	177696	21.35%	2.545%
13	1.403	246	253	262	rBV	74013	77103	9.26%	1.104%
14	1.686	334	341	354	rVB	68510	86386	10.38%	1.237%
15	2.278	516	525	536	rVB	148347	221214	26.58%	3.168%
16	2.661	641	644	645	rBV2	606	301	0.04%	0.004%
17	2.895	714	717	720	rBV3	354	228	0.03%	0.003%
18	3.050	763	765	771	rBV3	280	299	0.04%	0.004%
19	3.124	785	788	791	rBV2	271	189	0.02%	0.003%
20	3.207	812	814	816	rBV3	355	202	0.02%	0.003%
21	3.342	852	856	859	rBV3	416	430	0.05%	0.006%
22	3.407	874	876	880	rVB	558	326	0.04%	0.005%
23	3.429	881	883	884	rBV	360	144	0.02%	0.002%
24	3.497	902	904	905	rBV	351	154	0.02%	0.002%
25	3.805	998	1000	1003	rBV2	247	105	0.01%	0.002%
26	3.873	1017	1021	1023	rBV2	280	209	0.03%	0.003%
27	3.924	1035	1037	1039	rVB	218	110	0.01%	0.002%
28	3.940	1039	1042	1045	rBV2	461	304	0.04%	0.004%
29	3.956	1045	1047	1048	rBV	326	143	0.02%	0.002%
30	4.175	1097	1115	1152	rBV	75568	212404	25.52%	3.042%
31	4.429	1192	1194	1196	rVB2	472	157	0.02%	0.002%
32	4.503	1215	1217	1219	rVB	322	114	0.01%	0.002%
33	4.513	1219	1220	1223	rVB2	245	95	0.01%	0.001%
34	4.654	1248	1264	1284	rBV	142942	332054	39.90%	4.756%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071918\
 Data File : VU025521.D
 Acq On : 19 Jul 2018 14:56
 Operator : MD/SY
 Sample : J4065-13
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JHT42

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071718WMA.M
 Title : VOC Analysis

35	4.757	1294	1296	1299	rBV2	437	236	0.03%	0.003%
36	4.834	1317	1320	1322	rBV	290	190	0.02%	0.003%
37	4.918	1344	1346	1349	rVB2	518	234	0.03%	0.003%
38	4.934	1349	1351	1355	rBV2	205	94	0.01%	0.001%
39	4.950	1355	1356	1357	rBV	361	98	0.01%	0.001%
40	5.069	1391	1393	1396	rVB2	238	137	0.02%	0.002%
41	5.104	1396	1404	1405	rBV	364	369	0.04%	0.005%
42	5.255	1447	1451	1453	rVB	351	242	0.03%	0.003%
43	5.345	1453	1479	1507	rBV2	259878	785310	94.36%	11.247%
44	5.538	1532	1539	1544	rBV2	518	685	0.08%	0.010%
45	5.644	1570	1572	1576	rBV3	295	256	0.03%	0.004%
46	5.667	1576	1579	1586	rVV4	638	604	0.07%	0.009%
47	5.699	1586	1589	1592	rVB2	300	165	0.02%	0.002%
48	5.741	1598	1602	1605	rBV2	399	390	0.05%	0.006%
49	5.776	1610	1613	1615	rVB2	228	117	0.01%	0.002%
50	5.799	1618	1620	1623	rBV3	342	244	0.03%	0.003%
51	5.889	1634	1648	1672	rBV	366687	720888	86.62%	10.325%
52	6.062	1701	1702	1705	rVB2	281	108	0.01%	0.002%
53	6.095	1709	1712	1716	rVB2	467	288	0.03%	0.004%
54	6.143	1724	1727	1728	rBV2	160	96	0.01%	0.001%
55	6.265	1762	1765	1766	rBV	308	170	0.02%	0.002%
56	6.336	1772	1787	1804	rBV	188186	374598	45.01%	5.365%
57	6.496	1835	1837	1840	rBV2	344	177	0.02%	0.003%
58	6.609	1869	1872	1873	rBV	240	147	0.02%	0.002%
59	6.670	1890	1891	1893	rBV2	231	106	0.01%	0.002%
60	6.709	1900	1903	1904	rBV	347	152	0.02%	0.002%
61	6.734	1908	1911	1914	rVV2	315	250	0.03%	0.004%
62	6.847	1938	1946	1949	rBV4	1626	2238	0.27%	0.032%
63	6.940	1971	1975	1977	rBV2	203	136	0.02%	0.002%
64	6.969	1982	1984	1989	rVB2	338	203	0.02%	0.003%
65	7.001	1991	1994	1995	rBV2	283	151	0.02%	0.002%
66	7.123	2030	2032	2035	rBV	243	129	0.02%	0.002%
67	7.136	2035	2036	2041	rBV2	287	239	0.03%	0.003%
68	7.230	2048	2065	2088	rBV2	104392	188597	22.66%	2.701%
69	7.313	2088	2091	2095	rBV2	726	521	0.06%	0.007%
70	7.461	2131	2137	2140	rBV4	1158	1233	0.15%	0.018%
71	7.567	2153	2170	2189	rBV	331629	578388	69.50%	8.284%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071918\
 Data File : VU025521.D
 Acq On : 19 Jul 2018 14:56
 Operator : MD/SY
 Sample : J4065-13
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JHT42

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071718WMA.M
 Title : VOC Analysis

72	7.850	2247	2258	2279	rBV	71977	124509	14.96%	1.783%
73	8.027	2310	2313	2315	rBV	484	260	0.03%	0.004%
74	8.127	2341	2344	2346	rBV3	406	284	0.03%	0.004%
75	8.184	2350	2362	2372	rBV	19737	42330	5.09%	0.606%
76	8.310	2391	2401	2429	rVB	231091	398915	47.93%	5.713%
77	8.487	2450	2456	2458	rBV4	516	423	0.05%	0.006%
78	8.545	2466	2474	2478	rBV3	738	1133	0.14%	0.016%
79	8.641	2501	2504	2507	rBV3	465	273	0.03%	0.004%
80	8.702	2519	2523	2526	rBV3	343	315	0.04%	0.005%
81	8.885	2578	2580	2586	rVB2	366	300	0.04%	0.004%
82	8.921	2586	2591	2598	rBV4	635	860	0.10%	0.012%
83	9.091	2631	2644	2662	rBV	504172	832206	100.00%	11.919%
84	9.307	2709	2711	2713	rBV3	279	147	0.02%	0.002%
85	9.377	2727	2733	2744	rBV4	1442	1888	0.23%	0.027%
86	9.586	2793	2798	2801	rBV2	582	549	0.07%	0.008%
87	9.918	2897	2901	2904	rBV3	336	311	0.04%	0.004%
88	9.966	2912	2916	2919	rBV2	271	221	0.03%	0.003%
89	10.065	2945	2947	2951	rBV	457	332	0.04%	0.005%
90	10.265	3007	3009	3012	rVB	654	315	0.04%	0.005%
91	10.297	3012	3019	3021	rBV2	351	419	0.05%	0.006%
92	10.435	3050	3062	3085	rBV	275003	444921	53.46%	6.372%
93	10.612	3108	3117	3127	rBV3	10214	17748	2.13%	0.254%
94	10.786	3169	3171	3173	rBV	327	198	0.02%	0.003%
95	11.065	3255	3258	3261	rBV2	452	272	0.03%	0.004%
96	11.078	3261	3262	3265	rBV2	312	136	0.02%	0.002%
97	11.487	3376	3389	3405	rBV	471669	755666	90.80%	10.823%
98	11.770	3475	3477	3480	rBV2	457	260	0.03%	0.004%
99	11.863	3494	3506	3526	rVB	362828	585900	70.40%	8.391%
100	12.786	3791	3793	3796	rBV2	601	307	0.04%	0.004%


Sum of corrected areas: 6982091

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU071918\
Data File : VU025521.D
Acq On : 19 Jul 2018 14:56
Operator : MD/SY
Sample : J4065-13
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
JHT42

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071718WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

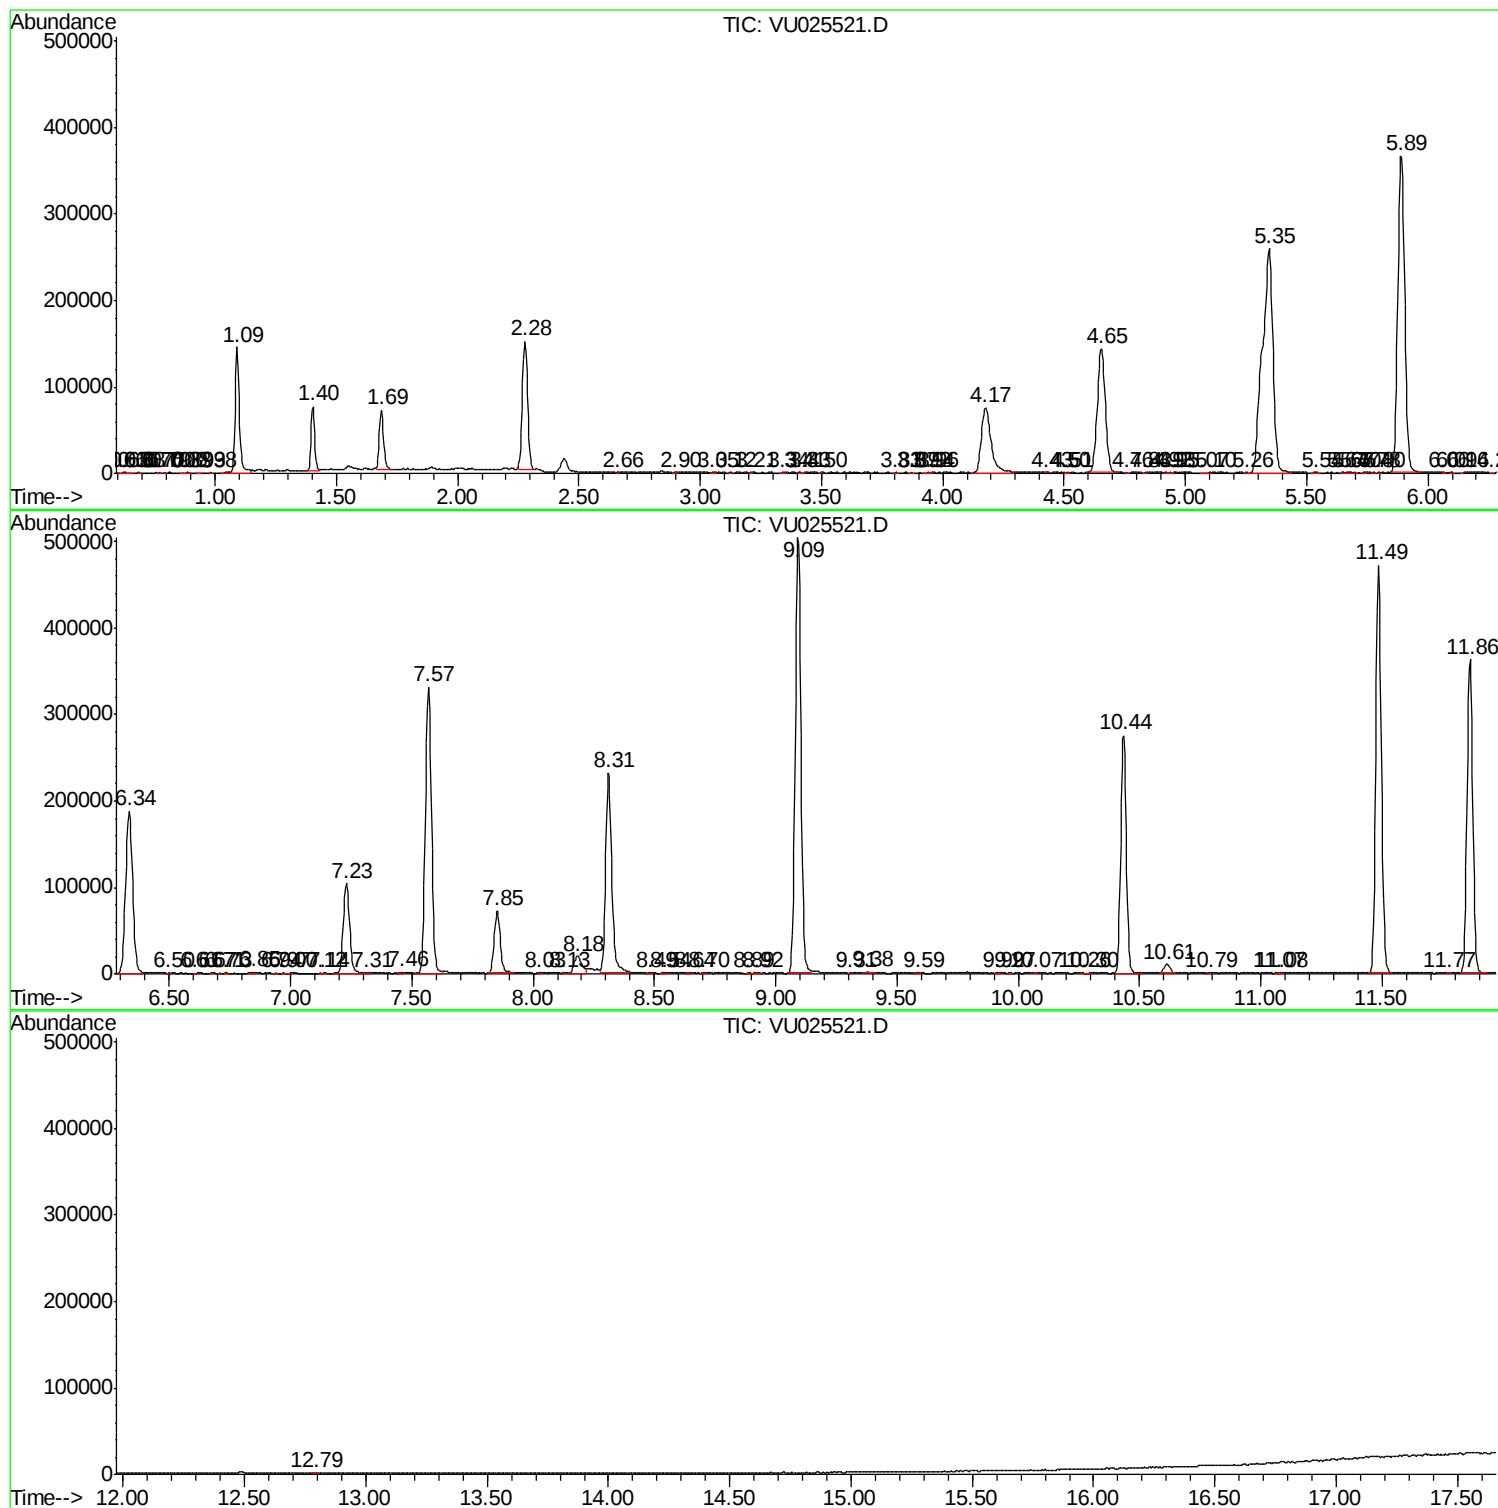

Data_Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU071918\
Data_File : VU025521.D
Acq_On : 19 Jul 2018 14:566
Operator : MD/SYY
Sample : J4065-133
Misc : 5.0mL/MSVOA_U/WATER
ALS_Vial : 11 Sample Multiplier: 11

Instrument :
MSVOA_U
ClientSampleId :
JHT42

Quant_Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071718WMA.MM
Quant_Title : VOC_Analysis

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
