


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071918\
 Data File : VU025511.D
 Acq On : 19 Jul 2018 08:58
 Operator : MD/SY
 Sample : BFB45
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB45

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071718WMA.M
 Title : VOC Analysis
 Last Update : Mon Jul 23 11:32:28 2018

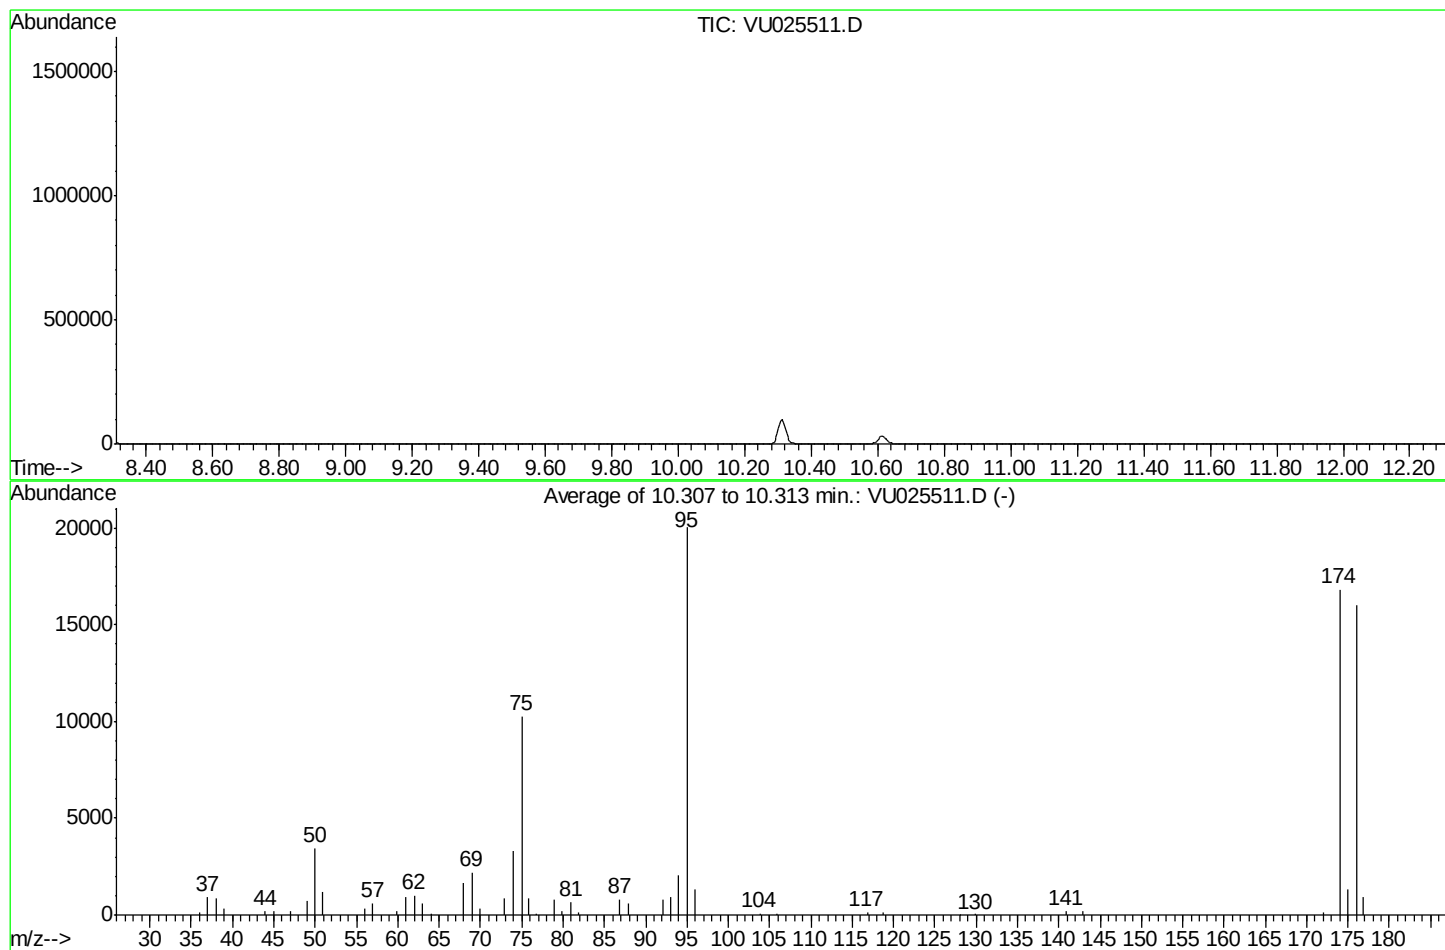

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	3462	PASS
75	95	30	80	51.3	10286	PASS
95	95	100	100	100.0	20034	PASS
96	95	5	9	6.5	1309	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.0	16823	PASS
175	174	5	9	7.9	1336	PASS
176	174	95	101	95.2	16009	PASS
177	176	5	9	5.9	941	PASS

Scan 3011 (10.272 min): VU025511.D
BFB45

m/z	Abundance
44.00	280.0
207.00	360.0
207.90	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
36.00	161.0
37.00	948.0
38.00	848.0
39.00	309.0
44.00	501.0
44.90	140.0
47.00	196.0
49.00	745.0
50.00	3497.0
51.00	1160.0
56.00	324.0
57.00	668.0
59.90	159.0
61.00	995.0
62.00	999.0
63.00	584.0
68.00	1699.0
69.00	2244.0
69.90	250.0
73.00	894.0
74.00	3357.0
75.00	9692.0
75.90	899.0
76.80	140.0
78.90	798.0
79.90	156.0
81.00	643.0
81.90	107.0
86.90	793.0
87.90	617.0
92.00	761.0
93.00	888.0
94.00	2086.0
95.00	19512.0
96.00	1248.0
105.90	110.0
116.90	125.0
118.80	130.0
140.90	234.0
142.90	218.0
172.00	129.0
174.00	15605.0
175.00	1270.0
176.00	15298.0
176.90	914.0
207.00	282.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
36.00	134.0
37.00	959.0
38.00	834.0
39.00	334.0
44.00	502.0
45.00	202.0
47.00	208.0
49.00	727.0
50.00	3527.0
51.00	1203.0
56.00	326.0
57.00	654.0
59.90	209.0
61.00	973.0
62.00	1042.0
63.00	631.0
64.00	124.0
68.00	1636.0
69.00	2308.0
69.90	314.0
73.00	888.0
74.00	3352.0
75.00	10688.0
75.90	861.0
76.80	117.0
78.90	827.0
79.90	176.0
81.00	717.0
81.90	116.0
86.90	833.0
87.90	614.0
92.00	892.0
93.00	967.0
94.00	2101.0
95.00	20632.0
96.00	1314.0
103.80	125.0
116.80	140.0
118.80	123.0
128.10	103.0
140.90	226.0
142.90	192.0
172.00	149.0
174.00	17392.0
175.00	1354.0
176.00	16496.0
176.90	969.0
207.00	250.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
35.90	117.0
37.00	923.0
38.00	886.0
39.00	355.0
43.90	457.0
45.00	245.0
47.00	160.0
49.00	669.0
50.00	3363.0
50.90	1123.0
55.90	292.0
57.00	515.0
59.90	249.0
61.00	905.0
62.00	1037.0
63.00	618.0
64.00	112.0
68.00	1640.0
69.00	2095.0
69.90	336.0
72.90	806.0
74.00	3196.0
75.00	10478.0
75.90	753.0
78.90	738.0
79.90	177.0
81.00	721.0
81.90	126.0
86.90	803.0
87.90	608.0
92.10	812.0
93.00	916.0
94.00	2054.0
95.00	19960.0
96.00	1366.0
103.90	144.0
116.80	146.0
118.80	100.0
129.90	127.0
140.90	195.0
143.00	172.0
172.00	127.0
174.00	17472.0
175.00	1384.0
176.00	16235.0
176.90	940.0
207.00	245.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45