

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071919\
 Data File : VU033337.D
 Acq On : 19 Jul 2019 15:14
 Operator : JC/SP
 Sample : K3831-02MS
 Misc : 14.82g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GAMR0MS

Quant Time: Aug 02 06:49:57 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 19 22:54:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	281312	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	292420	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.47	152	164550	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	83544	39.23	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	78.46%
7) Chloroethane-d5	1.63	69	102329	56.25	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	112.50%
11) 1,1-Dichloroethene-d2	2.23	63	226265	58.58	ug/L	-0.03
Spiked Amount	50.000	Range	60 - 125	Recovery	=	117.16%
21) 2-Butanone-d5	4.16	46	157571	116.78	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	116.78%
24) Chloroform-d	4.62	84	175327	49.13	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.26%
26) 1,2-Dichloroethane-d4	5.28	65	119715	52.30	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.60%
32) Benzene-d6	5.31	84	365036	50.89	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.78%
36) 1,2-Dichloropropane-d6	6.31	67	117398	51.09	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.18%
41) Toluene-d8	7.55	98	361881	53.50	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.00%
43) trans-1,3-Dichloropropene-	7.83	79	65078	57.75	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	115.50%
47) 2-Hexanone-d5	8.31	63	133003	128.39	ug/L	0.01
Spiked Amount	100.000	Range	45 - 130	Recovery	=	128.39%
57) 1,1,2,2-Tetrachloroethane-	10.42	84	199835	57.46	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	114.92%
64) 1,2-Dichlorobenzene-d4	11.85	152	158862	54.14	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	108.28%

Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
12) 1,1-Dichloroethene	2.24	96	99137	52.798	ug/L	94
15) Methyl Acetate	2.61	43	7611	3.457	ug/L	99
29) Cyclohexane	4.95	56	82806	25.988	ug/L #	78
33) Benzene	5.36	78	393665	46.163	ug/L	100
34) Trichloroethene	6.16	95	102939	46.156	ug/L	99
35) Methylcyclohexane	6.39	83	288845	84.546	ug/L	91
42) Toluene	7.62	91	439856	47.842	ug/L	99
51) Chlorobenzene	9.10	112	286857	47.802	ug/L	99
52) Ethylbenzene	9.23	91	250711	25.484	ug/L	99
53) m,p-Xylene	9.36	106	182504	48.977	ug/L	99
56) Isopropylbenzene	10.15	105	145669	15.299	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU071919\
Data File : VU033337.D
Acq On : 19 Jul 2019 15:14
Operator : JC/SP
Sample : K3831-02MS
Misc : 14.82g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GAMR0MS

Quant Time: Aug 02 06:49:57 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 19 22:54:17 2019
Response via : Initial Calibration




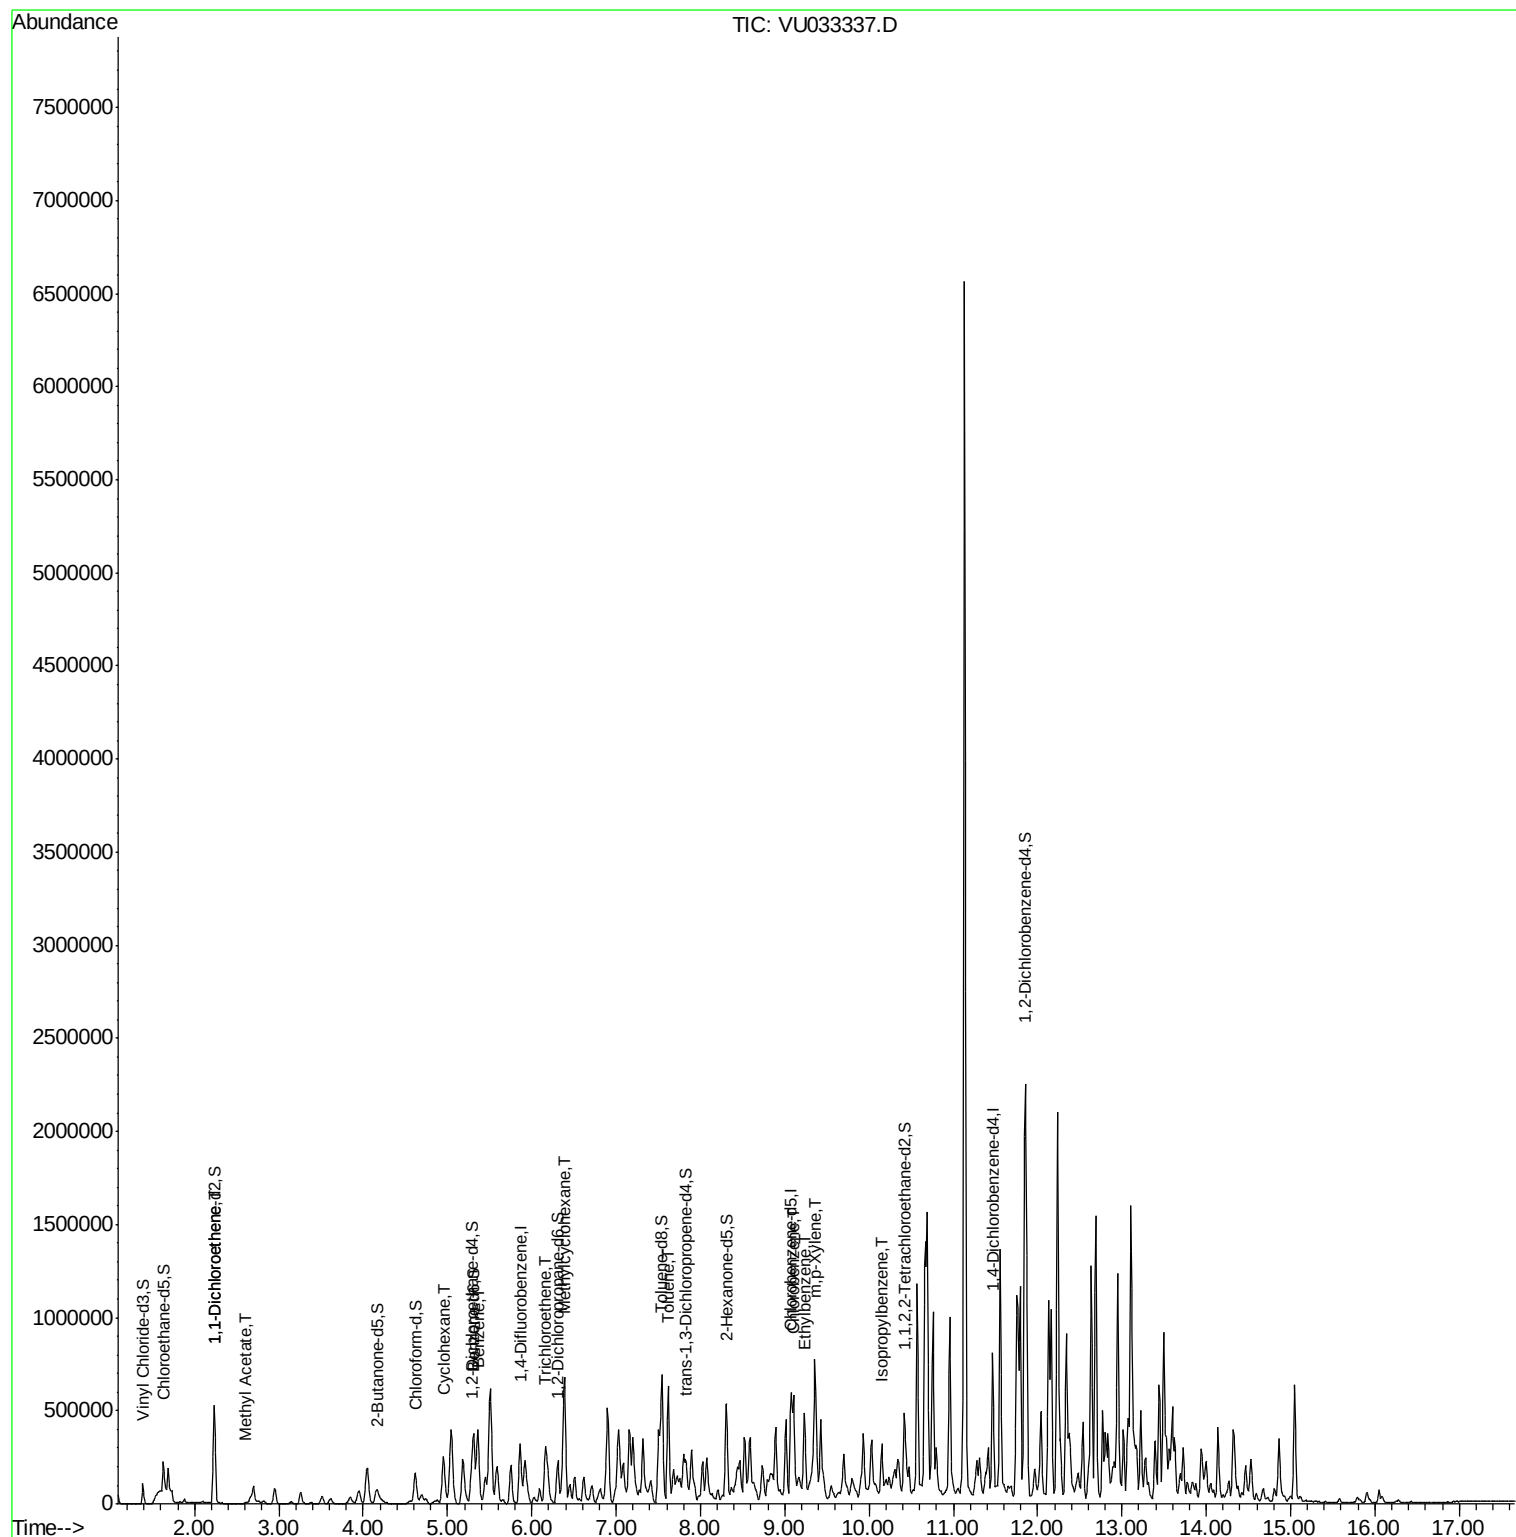


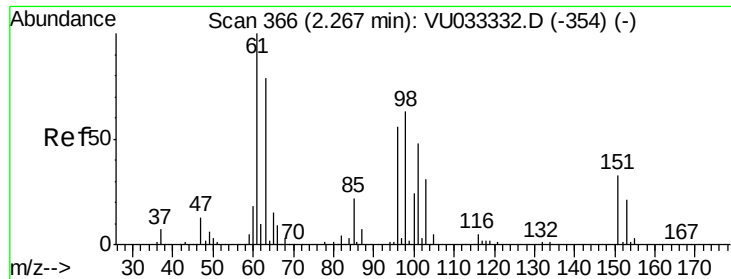

#12
 1,1-Dichloroethene
 Concen: 52.798 ug/L
 RT: 2.24 min Scan# 357
 Delta R.T. -0.03 min
 Lab File: VU033337.D
 Acq: 19 Jul 2019 15:14




Instrument :
 MSVOA_U
 ClientSampleId :
 GAMR0MS


Tot Ion	Ratio	Lower	Upper
96	100		
61	187.0	126.1	234.1
63	146.8	96.8	179.8

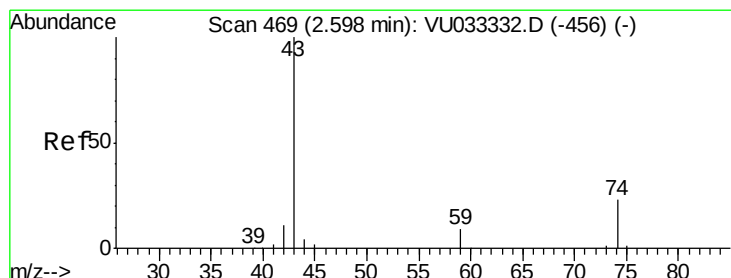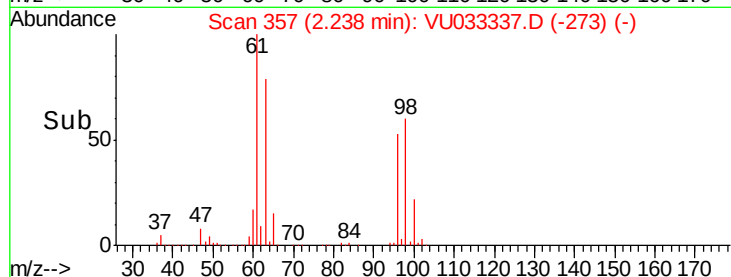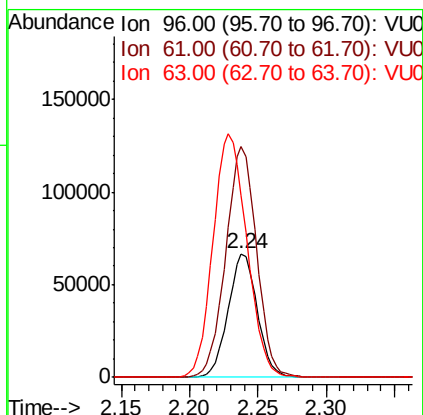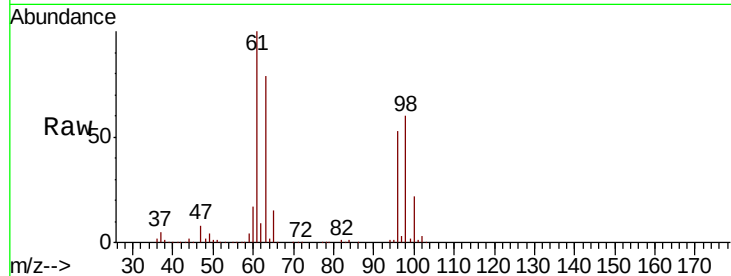

#15
 Methyl Acetate
 Concen: 3.457 ug/L
 RT: 2.61 min Scan# 472
 Delta R.T. 0.01 min
 Lab File: VU033337.D
 Acq: 19 Jul 2019 15:14

Tgt Ion	Ratio	Lower	Upper
43	100		
74	25.4	19.9	29.9

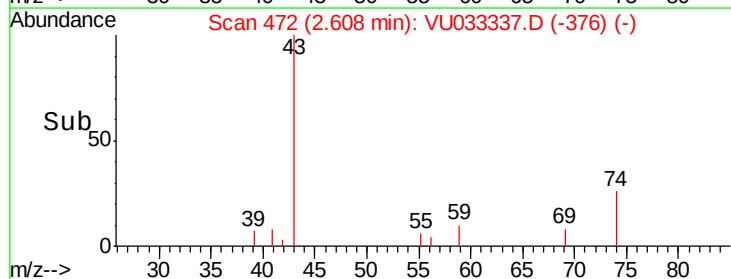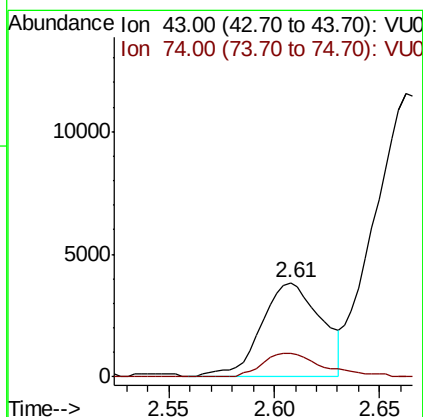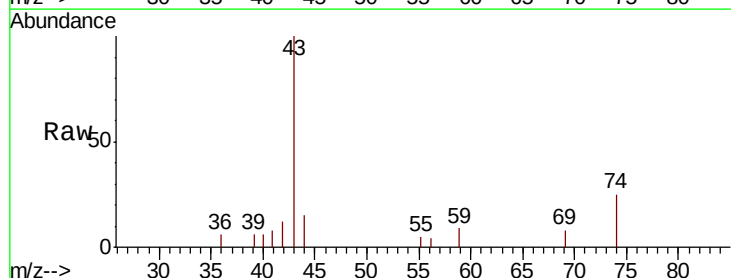


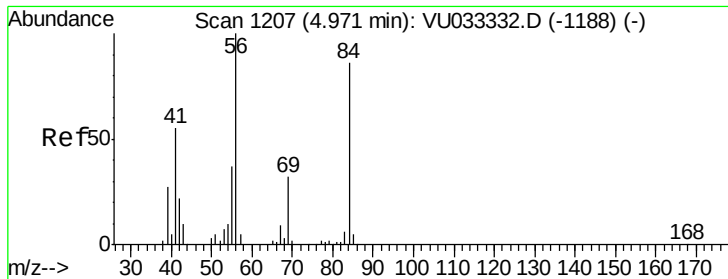




#29
Cyclohexane
Concen: 25.988 ug/L
RT: 4.95 min Scan# 1202
Delta R.T. -0.02 min
Lab File: VU033337.D
Acq: 19 Jul 2019 15:14

Instrument :
MSVOA_U
ClientSampleId :
GAMR0MS

Tot Ion: 56 Resp: 82806
Ion Ratio Lower Upper
56 100
69 21.1 24.7 37.1#
84 65.4 70.2 105.2#

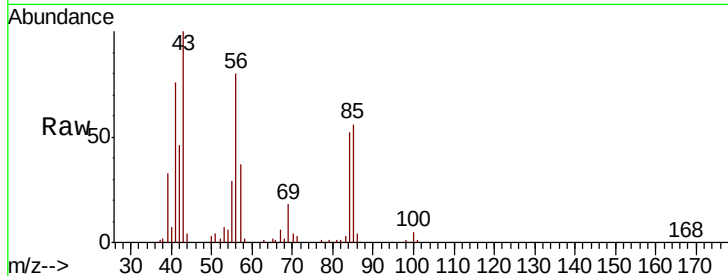


Abundance Ion 56.00 (55.70 to 56.70): VU0
Ion 69.00 (68.70 to 69.70): VU0
Ion 84.00 (83.70 to 84.70): VU0

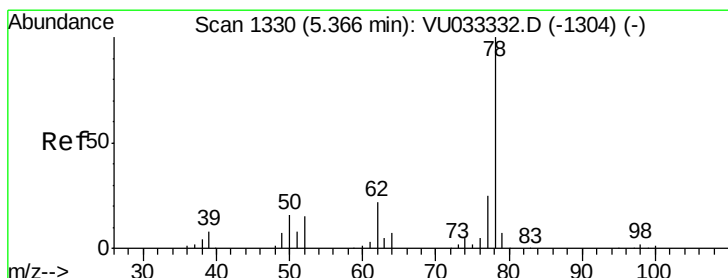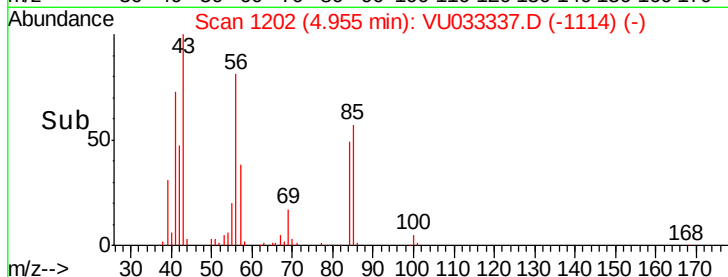
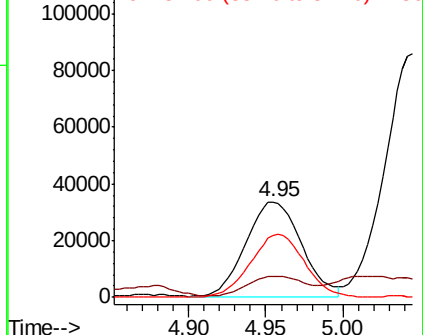



#33
Benzene
Concen: 46.163 ug/L
RT: 5.36 min Scan# 1328
Delta R.T. -0.01 min
Lab File: VU033337.D
Acq: 19 Jul 2019 15:14

Tgt Ion: 78 Resp: 393665

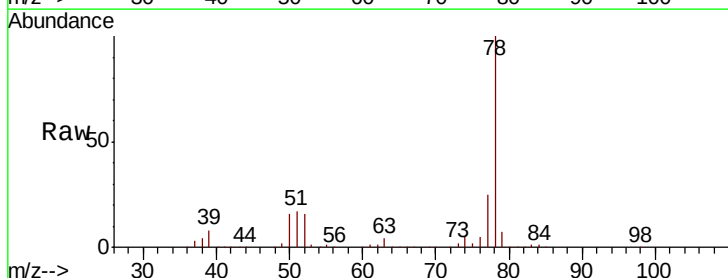

Abundance Ion 78.00 (77.70 to 78.70): VU0

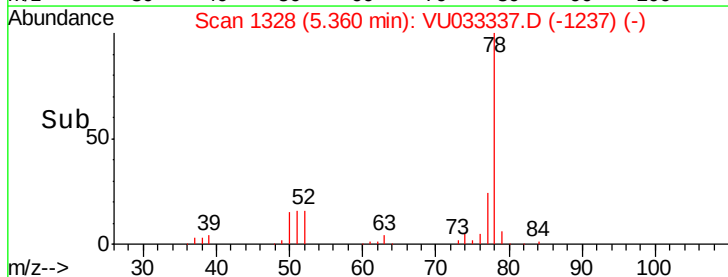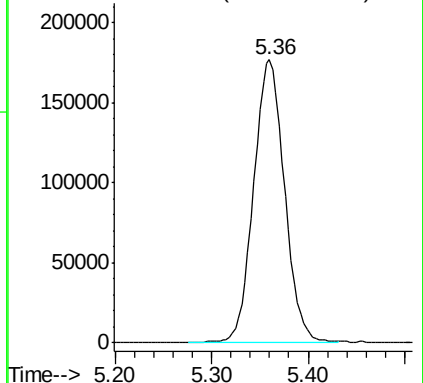

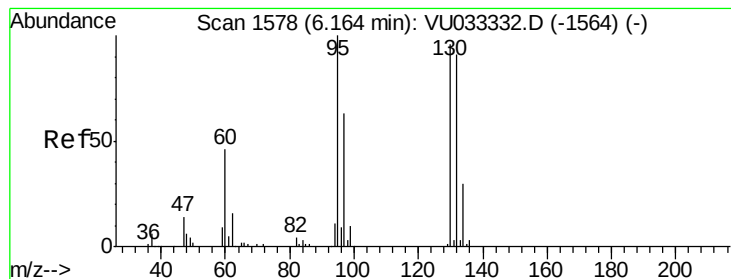

#34

Trichloroethene

Concen: 46.156 ug/L

RT: 6.16 min Scan# 1577

Delta R.T. -0.00 min

Lab File: VU033337.D

Acq: 19 Jul 2019 15:14

Instrument :

MSVOA_U

ClientSampleId :

GAMR0MS

Tot Ion: 95 Resp: 102939


Ion Ratio Lower Upper

95 100

97 64.5 43.8 81.4

132 93.4 65.5 121.6

130 97.9 69.7 129.5



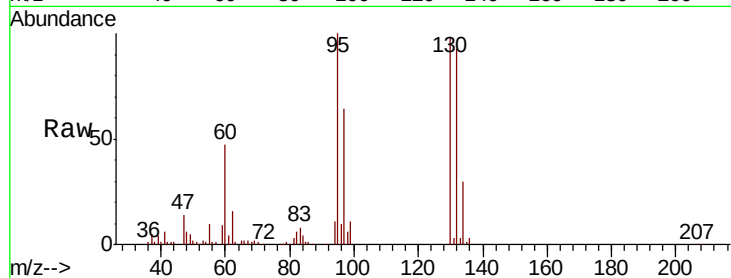


Abundance Ion 95.00 (94.70 to 95.70): VU033332.D (-1564) (-)

Ion 97.00 (96.70 to 97.70): VU033332.D (-1564) (-)

Ion 132.00 (131.70 to 132.70): VU033332.D (-1564) (-)

Ion 130.00 (129.70 to 130.70): VU033332.D (-1564) (-)

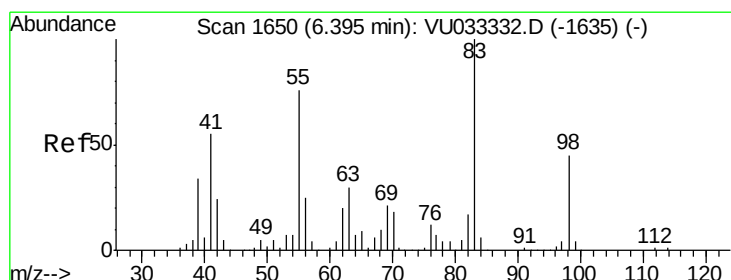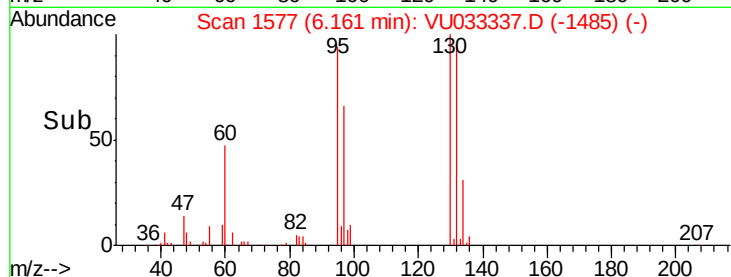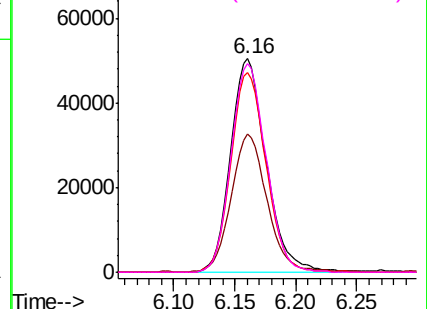

#35

Methylcyclohexane

Concen: 84.546 ug/L

RT: 6.39 min Scan# 1648

Delta R.T. -0.01 min

Lab File: VU033337.D

Acq: 19 Jul 2019 15:14


Tgt Ion: 83 Resp: 288845

Ion Ratio Lower Upper

83 100

55 86.1 60.5 90.7



98 43.5 37.4 56.0

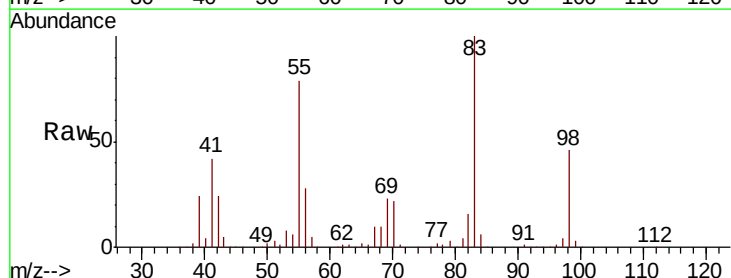


Abundance Ion 83.00 (82.70 to 83.70): VU033332.D (-1635) (-)

Ion 55.00 (54.70 to 55.70): VU033332.D (-1635) (-)

Ion 98.00 (97.70 to 98.70): VU033332.D (-1635) (-)

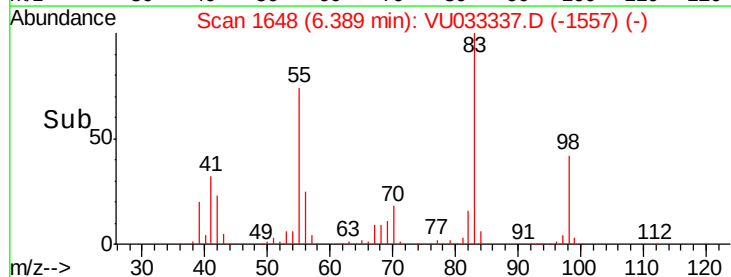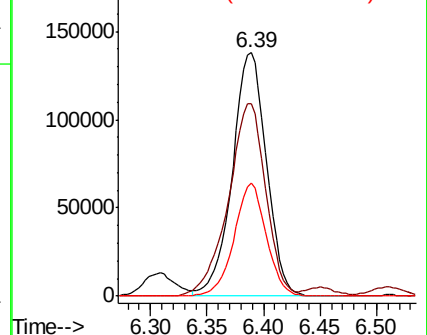

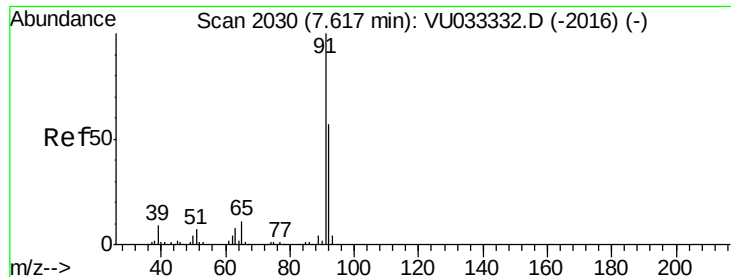

#42

Toluene

Concen: 47.842 ug/L

RT: 7.62 min Scan# 2030

Delta R.T. 0.00 min

Lab File: VU033337.D

Acq: 19 Jul 2019 15:14

Instrument :

MSVOA_U

ClientSampled :





GAMR0MS

Tot Ion: 91 Resp: 439856

Ion Ratio Lower Upper

91 100

92 56.3 39.8 74.0

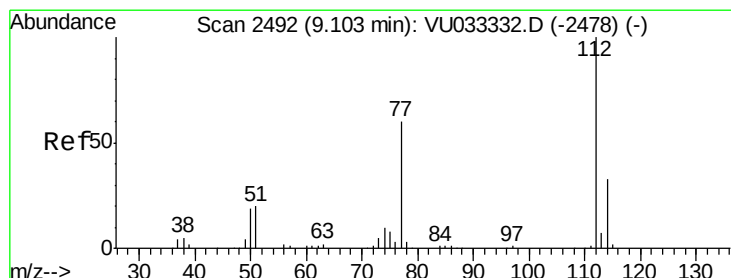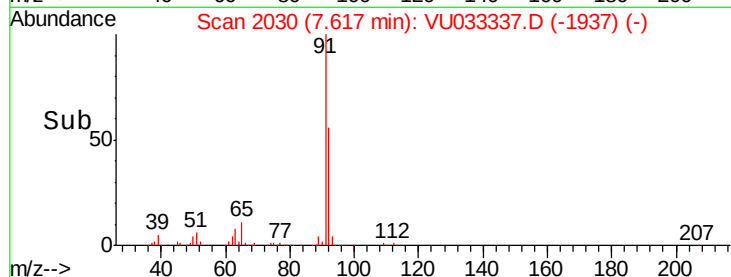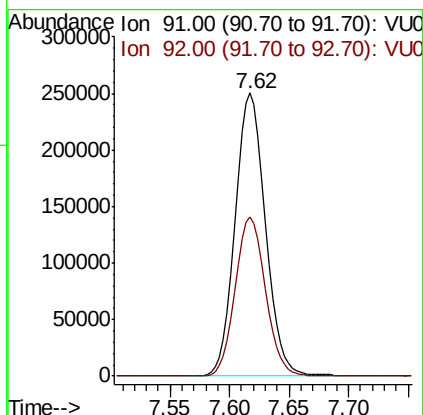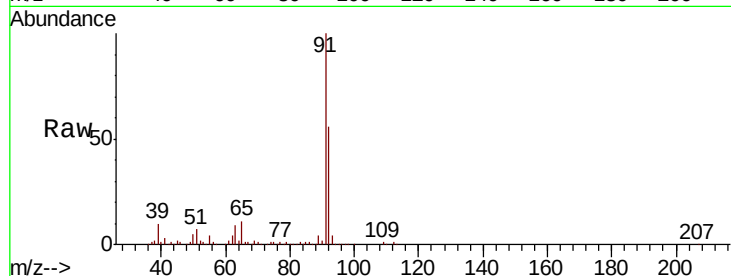

#51

Chlorobenzene

Concen: 47.802 ug/L

RT: 9.10 min Scan# 2492

Delta R.T. 0.00 min

Lab File: VU033337.D

Acq: 19 Jul 2019 15:14




Tgt Ion: 112 Resp: 286857


Ion Ratio Lower Upper

112 100

114 30.8 22.3 41.3

77 59.3 47.2 70.8

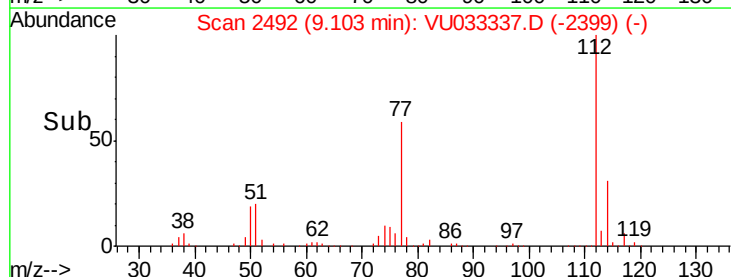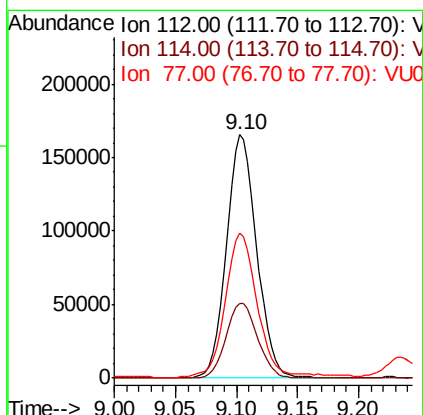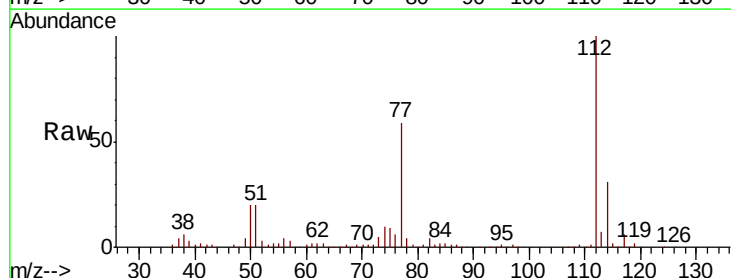

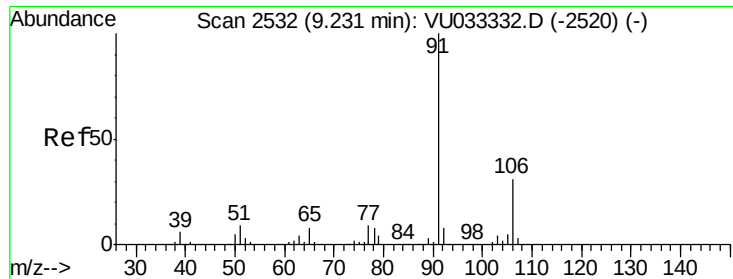

#52

Ethylbenzene

Concen: 25.484 ug/L

RT: 9.23 min Scan# 2533

Delta R.T. 0.00 min

Lab File: VU033337.D

Acq: 19 Jul 2019 15:14

Instrument :

MSVOA_U

ClientSampleId :





GAMR0MS

Tot Ion: 91 Resp: 250711

Ion Ratio Lower Upper

91 100

106 30.9 22.2 41.2

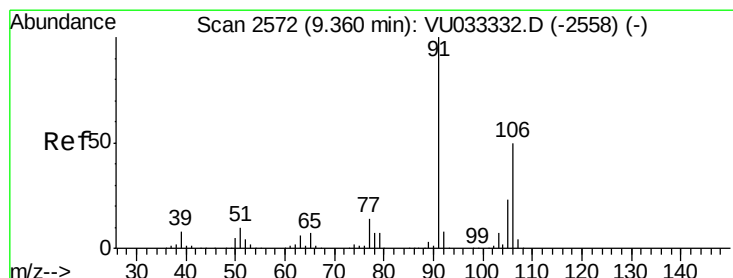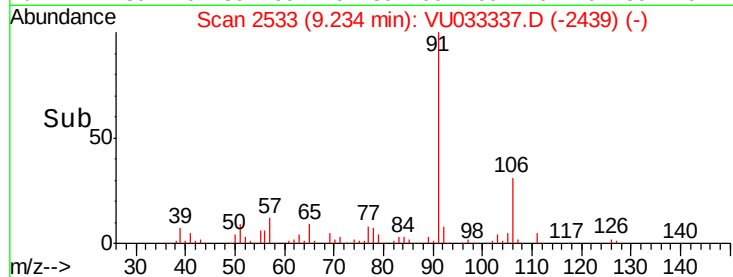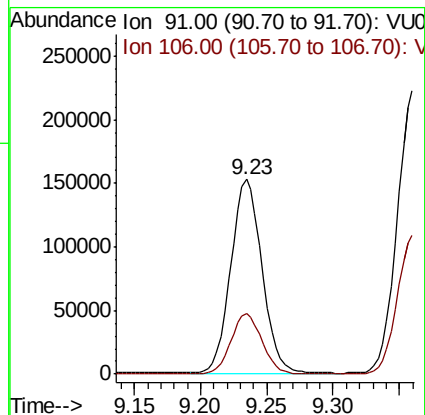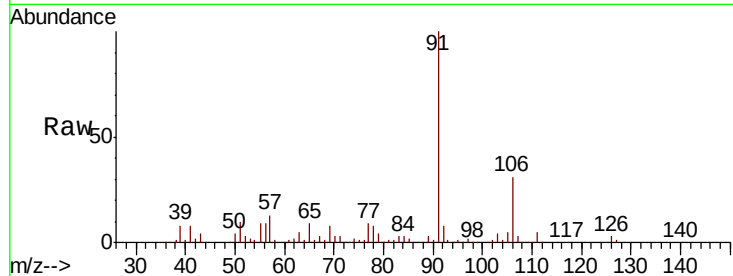

#53

m,p-Xylene

Concen: 48.977 ug/L

RT: 9.36 min Scan# 2572

Delta R.T. 0.00 min

Lab File: VU033337.D




Acq: 19 Jul 2019 15:14


Tgt Ion: 106 Resp: 182504

Ion Ratio Lower Upper

106 100

91 203.4 141.3 262.3

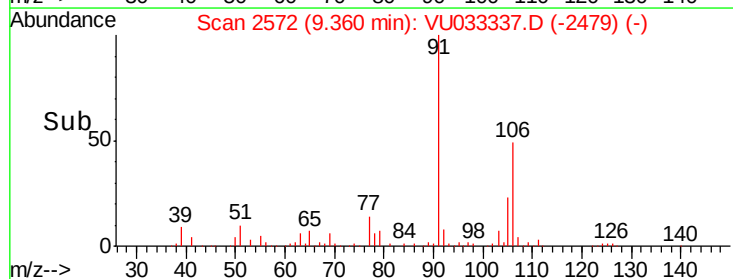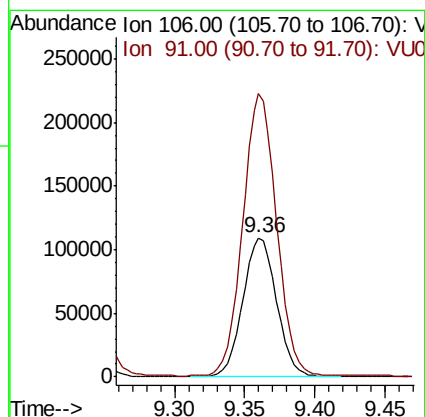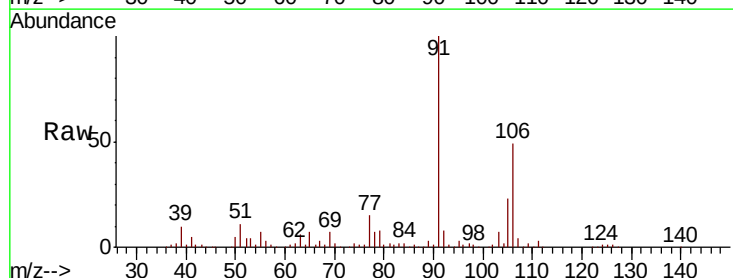

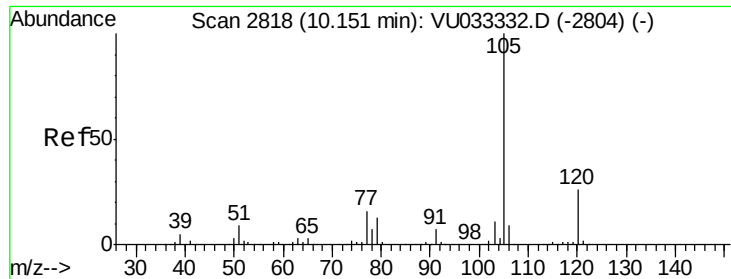

#56

Isopropylbenzene

Concen: 15.299 ug/L

RT: 10.15 min Scan# 2818

Delta R.T. 0.00 min

Lab File: VU033337.D

Acq: 19 Jul 2019 15:14

Instrument :

MSVOA_U

ClientSampleId :

GAMR0MS


Tot Ion:105 Resp: 145669

Ion Ratio Lower Upper

105 100

120 26.3 21.2 31.8

77 16.7 12.9 19.3

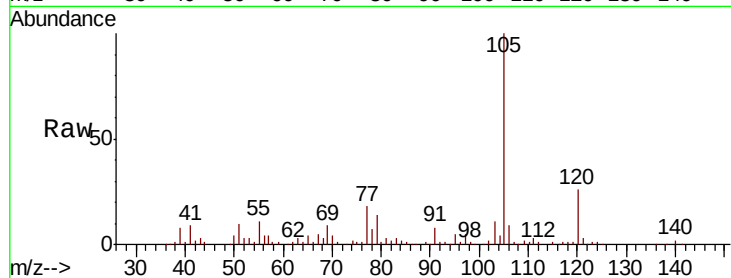

Abundance

Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

Ion 77.00 (76.70 to 77.70): VU0

