

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071919\
 Data File : VU033339.D
 Acq On : 19 Jul 2019 16:04
 Operator : JC/SP
 Sample : K3920-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A42M5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.177	23	27	35	rVB3	2539	2753	0.19%	0.023%
2	1.392	85	94	108	rBV2	294600	314404	21.59%	2.630%
3	1.540	134	140	149	rVB2	19572	24101	1.66%	0.202%
4	1.669	172	180	198	rBV	156783	204640	14.05%	1.712%
5	2.257	353	363	376	rBV2	308213	506784	34.81%	4.239%
6	2.354	391	393	398	rVB2	846	598	0.04%	0.005%
7	2.434	409	418	424	rBV3	2427	4026	0.28%	0.034%
8	2.685	488	496	508	rBV6	2107	4320	0.30%	0.036%
9	2.817	524	537	548	rVV4	1996	4661	0.32%	0.039%
10	2.977	572	587	602	rBV2	17018	38416	2.64%	0.321%
11	3.427	710	727	741	rBV2	22656	50266	3.45%	0.420%
12	4.061	921	924	927	rBV3	432	391	0.03%	0.003%
13	4.148	938	951	956	rBV	112675	220476	15.14%	1.844%
14	4.620	1082	1098	1120	rBV	204268	485307	33.33%	4.059%
15	4.890	1166	1182	1199	rVV2	28661	70215	4.82%	0.587%
16	4.955	1199	1202	1204	rVV3	741	520	0.04%	0.004%
17	4.971	1205	1207	1213	rVB3	1234	967	0.07%	0.008%
18	5.054	1225	1233	1242	rVB5	1305	2024	0.14%	0.017%
19	5.193	1271	1276	1278	rBV2	570	376	0.03%	0.003%
20	5.318	1288	1315	1342	rBV2	415768	1244287	85.46%	10.407%
21	5.450	1352	1356	1358	rBV3	577	459	0.03%	0.004%
22	5.585	1395	1398	1403	rBV4	481	393	0.03%	0.003%
23	5.768	1453	1455	1459	rVB5	762	422	0.03%	0.004%
24	5.865	1471	1485	1502	rBV	377346	738005	50.69%	6.173%
25	6.164	1563	1578	1605	rBV	758639	1456041	100.00%	12.178%
26	6.308	1609	1623	1642	rVV	275019	549077	37.71%	4.592%
27	6.524	1685	1690	1692	rVB2	586	423	0.03%	0.004%
28	6.595	1706	1712	1714	rBV5	1418	1486	0.10%	0.012%
29	6.842	1784	1789	1790	rBV4	830	558	0.04%	0.005%
30	6.903	1803	1808	1810	rBV3	1129	1059	0.07%	0.009%
31	7.032	1844	1848	1856	rVB4	606	832	0.06%	0.007%
32	7.164	1879	1889	1891	rBV4	917	1172	0.08%	0.010%
33	7.209	1891	1903	1932	rVV	159752	288253	19.80%	2.411%
34	7.328	1934	1940	1944	rVB6	818	947	0.07%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U071919\
 Data File : VU033339.D
 Acq On : 19 Jul 2019 16:04
 Operator : JC/SP
 Sample : K3920-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A42M5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
 Title : VOC Analysis

35	7.373	1949	1954	1957	rBV2	656	741	0.05%	0.006%
36	7.546	1992	2008	2027	rBV	567189	989351	67.95%	8.275%
37	7.739	2059	2068	2077	rBV8	3770	7144	0.49%	0.060%
38	7.832	2081	2097	2114	rBV	109174	194490	13.36%	1.627%
39	7.974	2139	2141	2146	rVB2	577	393	0.03%	0.003%
40	8.160	2192	2199	2208	rVV4	2593	4306	0.30%	0.036%
41	8.209	2208	2214	2223	rVB4	4271	5780	0.40%	0.048%
42	8.295	2229	2241	2279	rBV	345236	639966	43.95%	5.353%
43	8.556	2320	2322	2326	rVB2	583	427	0.03%	0.004%
44	8.582	2326	2330	2331	rBV2	1084	795	0.05%	0.007%
45	8.630	2342	2345	2351	rVB2	407	370	0.03%	0.003%
46	8.726	2373	2375	2379	rVB3	463	343	0.02%	0.003%
47	8.803	2387	2399	2403	rVV4	1317	1870	0.13%	0.016%
48	8.845	2406	2412	2419	rVV4	1468	2437	0.17%	0.020%
49	8.893	2419	2427	2438	rVV4	8676	15107	1.04%	0.126%
50	9.016	2455	2465	2471	rBV3	8451	13590	0.93%	0.114%
51	9.074	2471	2483	2509	rVV2	564030	1072604	73.67%	8.971%
52	9.238	2527	2534	2542	rVB4	3172	4469	0.31%	0.037%
53	9.311	2552	2557	2558	rBV2	482	406	0.03%	0.003%
54	9.331	2561	2563	2566	rVV5	838	537	0.04%	0.004%
55	9.363	2566	2573	2580	rVV4	2024	3359	0.23%	0.028%
56	9.427	2584	2593	2612	rVB3	12363	22936	1.58%	0.192%
57	9.562	2630	2635	2641	rBV2	442	599	0.04%	0.005%
58	9.639	2650	2659	2662	rBV4	894	1498	0.10%	0.013%
59	9.701	2669	2678	2688	rBV4	4936	8110	0.56%	0.068%
60	9.742	2688	2691	2694	rBV3	628	613	0.04%	0.005%
61	9.768	2696	2699	2702	rBV4	684	442	0.03%	0.004%
62	9.800	2702	2709	2720	rBV5	4344	7327	0.50%	0.061%
63	9.897	2731	2739	2741	rBV3	1719	1938	0.13%	0.016%
64	9.935	2742	2751	2762	rVB2	15446	25568	1.76%	0.214%
65	9.993	2762	2769	2770	rBV3	1676	1690	0.12%	0.014%
66	10.028	2774	2780	2789	rVV6	4333	7879	0.54%	0.066%
67	10.074	2789	2794	2807	rVB5	3327	5853	0.40%	0.049%
68	10.125	2807	2810	2811	rBV2	767	470	0.03%	0.004%
69	10.147	2813	2817	2824	rVB7	1889	2469	0.17%	0.021%
70	10.241	2838	2846	2853	rBV5	5634	8981	0.62%	0.075%
71	10.414	2889	2900	2917	rBV	396167	657329	45.14%	5.498%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071919\
 Data File : VU033339.D
 Acq On : 19 Jul 2019 16:04
 Operator : JC/SP
 Sample : K3920-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A42M5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
 Title : VOC Analysis

72	10.672	2971	2980	2982	rBV7	2611	3432	0.24%	0.029%
73	10.736	2993	3000	3011	rBV7	4884	9911	0.68%	0.083%
74	10.800	3012	3020	3037	rVB2	25769	42273	2.90%	0.354%
75	10.887	3042	3047	3054	rBV6	1875	2317	0.16%	0.019%
76	10.996	3074	3081	3087	rBV8	4643	6744	0.46%	0.056%
77	11.054	3096	3099	3106	rVB4	3083	3127	0.21%	0.026%
78	11.099	3107	3113	3119	rVV3	12363	16982	1.17%	0.142%
79	11.135	3119	3124	3134	rVB2	13619	18170	1.25%	0.152%
80	11.254	3155	3161	3169	rBV7	4260	7184	0.49%	0.060%
81	11.469	3217	3228	3241	rBV	570438	906109	62.23%	7.579%
82	11.556	3250	3255	3262	rBV5	7845	9637	0.66%	0.081%
83	11.845	3334	3345	3365	rVB	577648	926095	63.60%	7.746%
84	12.601	3571	3580	3585	rBV7	5658	10276	0.71%	0.086%
85	12.691	3603	3608	3616	rBV4	4757	6517	0.45%	0.055%
86	12.816	3641	3647	3652	rBV8	2633	4109	0.28%	0.034%
87	13.022	3706	3711	3718	rVB6	2571	3175	0.22%	0.027%
88	13.067	3722	3725	3726	rBV2	1197	681	0.05%	0.006%
89	13.112	3735	3739	3745	rVB5	4299	4481	0.31%	0.037%
90	13.273	3783	3789	3792	rBV6	1896	2433	0.17%	0.020%
91	13.395	3821	3827	3833	rBV7	1628	2446	0.17%	0.020%
92	13.446	3838	3843	3849	rVV6	2236	2401	0.16%	0.020%
93	13.498	3853	3859	3866	rBV7	3144	4235	0.29%	0.035%
94	13.929	3990	3993	3994	rBV3	727	462	0.03%	0.004%
95	14.109	4047	4049	4051	rBV3	675	398	0.03%	0.003%
96	14.321	4111	4115	4116	rBV3	1554	1005	0.07%	0.008%
97	14.466	4157	4160	4161	rBV3	1010	522	0.04%	0.004%
98	14.803	4261	4265	4269	rBV6	1104	1355	0.09%	0.011%
99	14.877	4278	4288	4292	rBV6	4242	6769	0.46%	0.057%
100	15.057	4336	4344	4361	rVB3	12854	22083	1.52%	0.185%


Sum of corrected areas: 11956175

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU071919\
Data File : VU033339.D
Acq On : 19 Jul 2019 16:04
Operator : JC/SP
Sample : K3920-01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A42M5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

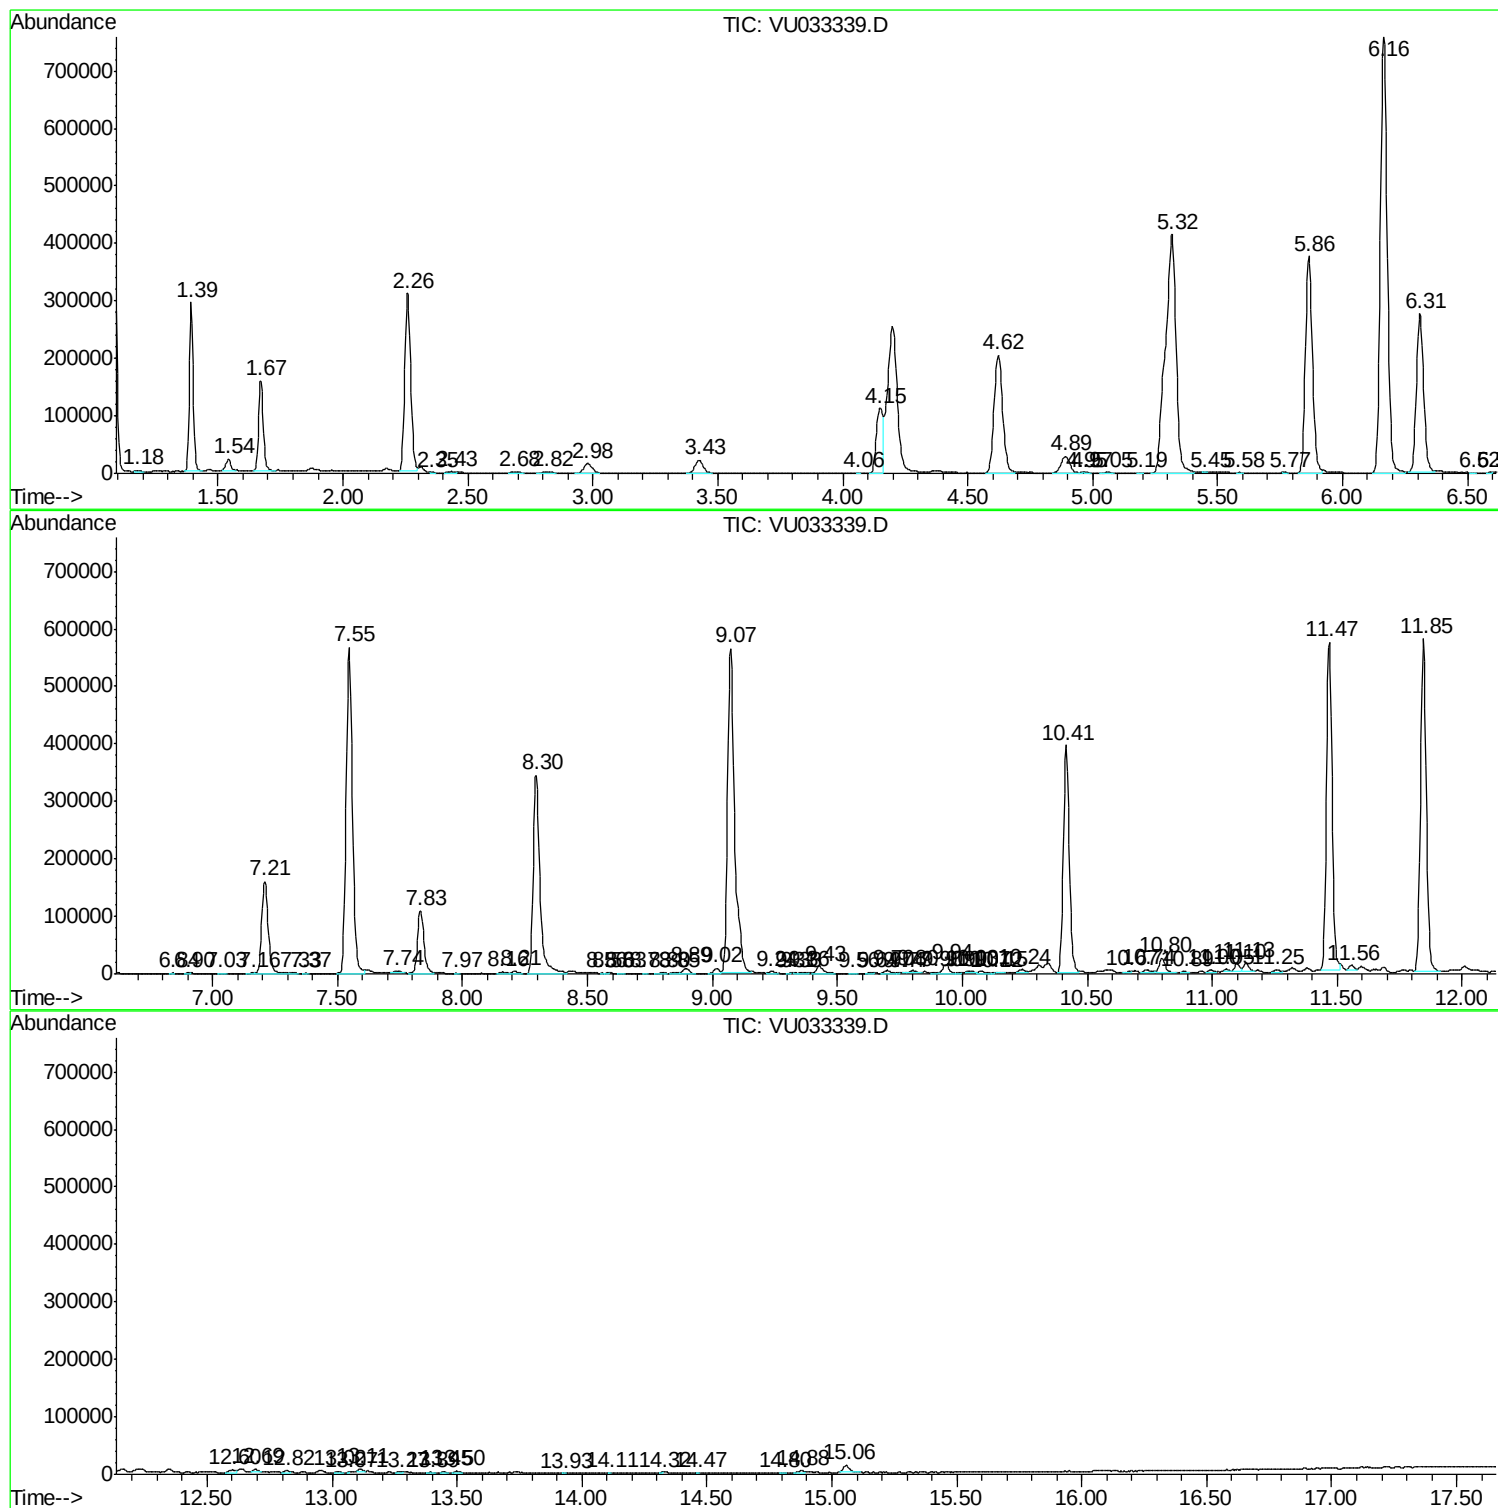

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU071919\
Data File : VU033339.D
Acq On : 19 Jul 2019 16:04
Operator : JC/SP
Sample : K3920-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A42M5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU071919\
Data File : VU033339.D
Acq On : 19 Jul 2019 16:04
Operator : JC/SP
Sample : K3920-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A42M5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc