

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071919\
 Data File : VU033340.D
 Acq On : 19 Jul 2019 16:25
 Operator : JC/SP
 Sample : K3920-02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A42M6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.177	23	27	36	rBV4	2857	2951	0.25%	0.028%
2	1.393	86	94	107	rBV2	218458	240933	20.20%	2.260%
3	1.541	135	140	151	rVB2	15971	18932	1.59%	0.178%
4	1.669	172	180	199	rVB	148010	190040	15.93%	1.783%
5	2.261	353	364	376	rBV2	334006	580911	48.69%	5.450%
6	2.431	407	417	425	rBV4	2686	5300	0.44%	0.050%
7	2.528	445	447	454	rBV3	365	298	0.02%	0.003%
8	2.685	491	496	501	rVB3	882	992	0.08%	0.009%
9	2.724	506	508	513	rVB	424	288	0.02%	0.003%
10	2.814	526	536	550	rVB3	2020	4039	0.34%	0.038%
11	2.917	564	568	572	rBV2	342	301	0.03%	0.003%
12	2.981	572	588	604	rBV	56484	125656	10.53%	1.179%
13	3.425	709	726	754	rBV	73989	165097	13.84%	1.549%
14	3.817	844	848	855	rVB2	357	310	0.03%	0.003%
15	3.981	895	899	906	rVB4	289	373	0.03%	0.003%
16	4.068	920	926	928	rBV3	313	312	0.03%	0.003%
17	4.151	939	952	957	rBV	105612	219834	18.43%	2.062%
18	4.367	1011	1019	1041	rVB3	5770	14929	1.25%	0.140%
19	4.531	1067	1070	1072	rBV2	396	292	0.02%	0.003%
20	4.621	1081	1098	1122	rBV	194831	463026	38.81%	4.344%
21	4.891	1164	1182	1201	rBV	136315	334834	28.07%	3.141%
22	4.974	1206	1208	1217	rVB5	959	801	0.07%	0.008%
23	5.068	1230	1237	1239	rBV	386	462	0.04%	0.004%
24	5.180	1268	1272	1275	rBV3	331	328	0.03%	0.003%
25	5.315	1290	1314	1349	rBV2	397073	1192984	100.00%	11.192%
26	5.508	1371	1374	1377	rVV4	454	337	0.03%	0.003%
27	5.727	1438	1442	1447	rBV2	429	400	0.03%	0.004%
28	5.865	1471	1485	1505	rBV	369856	729388	61.14%	6.842%
29	5.997	1524	1526	1533	rVB3	661	489	0.04%	0.005%
30	6.164	1565	1578	1603	rBV	179581	347870	29.16%	3.263%
31	6.309	1609	1623	1645	rBV	260727	524538	43.97%	4.921%
32	6.598	1704	1713	1731	rVB3	4458	9723	0.82%	0.091%
33	7.209	1890	1903	1933	rBV	148234	273819	22.95%	2.569%
34	7.396	1959	1961	1967	rVB3	542	507	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U071919\
 Data File : VU033340.D
 Acq On : 19 Jul 2019 16:25
 Operator : JC/SP
 Sample : K3920-02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A42M6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
 Title : VOC Analysis

35	7.425	1967	1970	1974	rVB2	508	444	0.04%	0.004%
36	7.547	1993	2008	2028	rBV	531971	937385	78.57%	8.794%
37	7.736	2056	2067	2084	rBV3	19865	37868	3.17%	0.355%
38	7.830	2086	2096	2116	rBV	101742	179280	15.03%	1.682%
39	7.958	2134	2136	2143	rVB5	520	450	0.04%	0.004%
40	8.016	2148	2154	2158	rBV3	630	491	0.04%	0.005%
41	8.045	2158	2163	2164	rBV4	866	605	0.05%	0.006%
42	8.161	2190	2199	2207	rBV4	2807	4633	0.39%	0.043%
43	8.216	2211	2216	2221	rVB2	573	694	0.06%	0.007%
44	8.293	2228	2240	2283	rBV	319161	605789	50.78%	5.683%
45	8.617	2334	2341	2345	rBV3	267	366	0.03%	0.003%
46	8.894	2423	2427	2433	rVB4	940	1037	0.09%	0.010%
47	9.007	2459	2462	2463	rBV	742	392	0.03%	0.004%
48	9.071	2470	2482	2516	rBV	559414	960854	80.54%	9.014%
49	9.232	2528	2532	2536	rBV6	767	725	0.06%	0.007%
50	9.289	2542	2550	2555	rBV4	1083	1175	0.10%	0.011%
51	9.354	2566	2570	2571	rBV3	509	334	0.03%	0.003%
52	9.428	2580	2593	2602	rBV5	1818	2807	0.24%	0.026%
53	9.592	2638	2644	2647	rBV2	316	284	0.02%	0.003%
54	9.701	2673	2678	2681	rBV4	902	849	0.07%	0.008%
55	9.736	2686	2689	2691	rBV2	538	292	0.02%	0.003%
56	9.801	2703	2709	2716	rBV6	1112	1681	0.14%	0.016%
57	9.936	2743	2751	2758	rVB5	3160	4589	0.38%	0.043%
58	10.003	2767	2772	2775	rVB3	321	312	0.03%	0.003%
59	10.026	2775	2779	2786	rBV3	797	919	0.08%	0.009%
60	10.074	2792	2794	2799	rVB2	598	375	0.03%	0.004%
61	10.235	2838	2844	2852	rBV3	1350	1924	0.16%	0.018%
62	10.305	2852	2866	2871	rBV7	3927	7431	0.62%	0.070%
63	10.415	2888	2900	2918	rBV	380178	612350	51.33%	5.745%
64	10.518	2928	2932	2934	rBV2	636	447	0.04%	0.004%
65	10.588	2948	2954	2965	rVB4	2991	5704	0.48%	0.054%
66	10.637	2965	2969	2974	rBV3	439	480	0.04%	0.005%
67	10.669	2975	2979	2982	rBV4	456	360	0.03%	0.003%
68	10.688	2982	2985	2988	rBV4	502	369	0.03%	0.003%
69	10.727	2993	2997	3000	rBV3	417	380	0.03%	0.004%
70	10.743	3000	3002	3007	rBV2	694	502	0.04%	0.005%
71	10.797	3011	3019	3033	rBV4	6942	11392	0.95%	0.107%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071919\
 Data File : VU033340.D
 Acq On : 19 Jul 2019 16:25
 Operator : JC/SP
 Sample : K3920-02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A42M6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
 Title : VOC Analysis

72	10.884	3040	3046	3048	rBV4	736	707	0.06%	0.007%
73	10.939	3061	3063	3065	rBV	475	300	0.03%	0.003%
74	10.994	3074	3080	3088	rBV5	2065	3213	0.27%	0.030%
75	11.055	3093	3099	3105	rBV7	2328	3225	0.27%	0.030%
76	11.100	3106	3113	3119	rBV5	5706	7331	0.61%	0.069%
77	11.257	3156	3162	3168	rBV3	1692	2347	0.20%	0.022%
78	11.293	3170	3173	3175	rBV2	691	536	0.04%	0.005%
79	11.318	3175	3181	3189	rVB5	3101	4960	0.42%	0.047%
80	11.367	3190	3196	3198	rBV5	2018	1986	0.17%	0.019%
81	11.466	3215	3227	3249	rBV	555043	904779	75.84%	8.488%
82	11.685	3289	3295	3307	rVB7	3875	6361	0.53%	0.060%
83	11.846	3332	3345	3366	rBV	526771	866853	72.66%	8.132%
84	11.994	3388	3391	3392	rBV3	1025	653	0.05%	0.006%
85	12.013	3392	3397	3403	rVB6	3088	4134	0.35%	0.039%
86	12.103	3422	3425	3431	rBV3	784	739	0.06%	0.007%
87	12.212	3453	3459	3461	rBV5	2067	2294	0.19%	0.022%
88	12.338	3494	3498	3499	rBV	1908	1215	0.10%	0.011%
89	12.405	3515	3519	3522	rBV3	803	859	0.07%	0.008%
90	12.601	3570	3580	3585	rBV6	2582	4161	0.35%	0.039%
91	12.688	3603	3607	3614	rVB5	1744	1681	0.14%	0.016%
92	12.817	3645	3647	3650	rBV3	790	538	0.05%	0.005%
93	12.932	3679	3683	3685	rBV3	389	361	0.03%	0.003%
94	12.955	3689	3690	3698	rVB5	743	598	0.05%	0.006%
95	13.096	3729	3734	3735	rBV3	622	525	0.04%	0.005%
96	13.235	3774	3777	3780	rBV3	563	352	0.03%	0.003%
97	13.318	3800	3803	3805	rBV	622	401	0.03%	0.004%
98	13.511	3860	3863	3864	rBV2	579	333	0.03%	0.003%
99	13.646	3900	3905	3907	rBV2	568	598	0.05%	0.006%
100	13.659	3907	3909	3912	rBV2	545	393	0.03%	0.004%


Sum of corrected areas: 10659696

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU071919\
Data File : VU033340.D
Acq On : 19 Jul 2019 16:25
Operator : JC/SP
Sample : K3920-02
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A42M6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

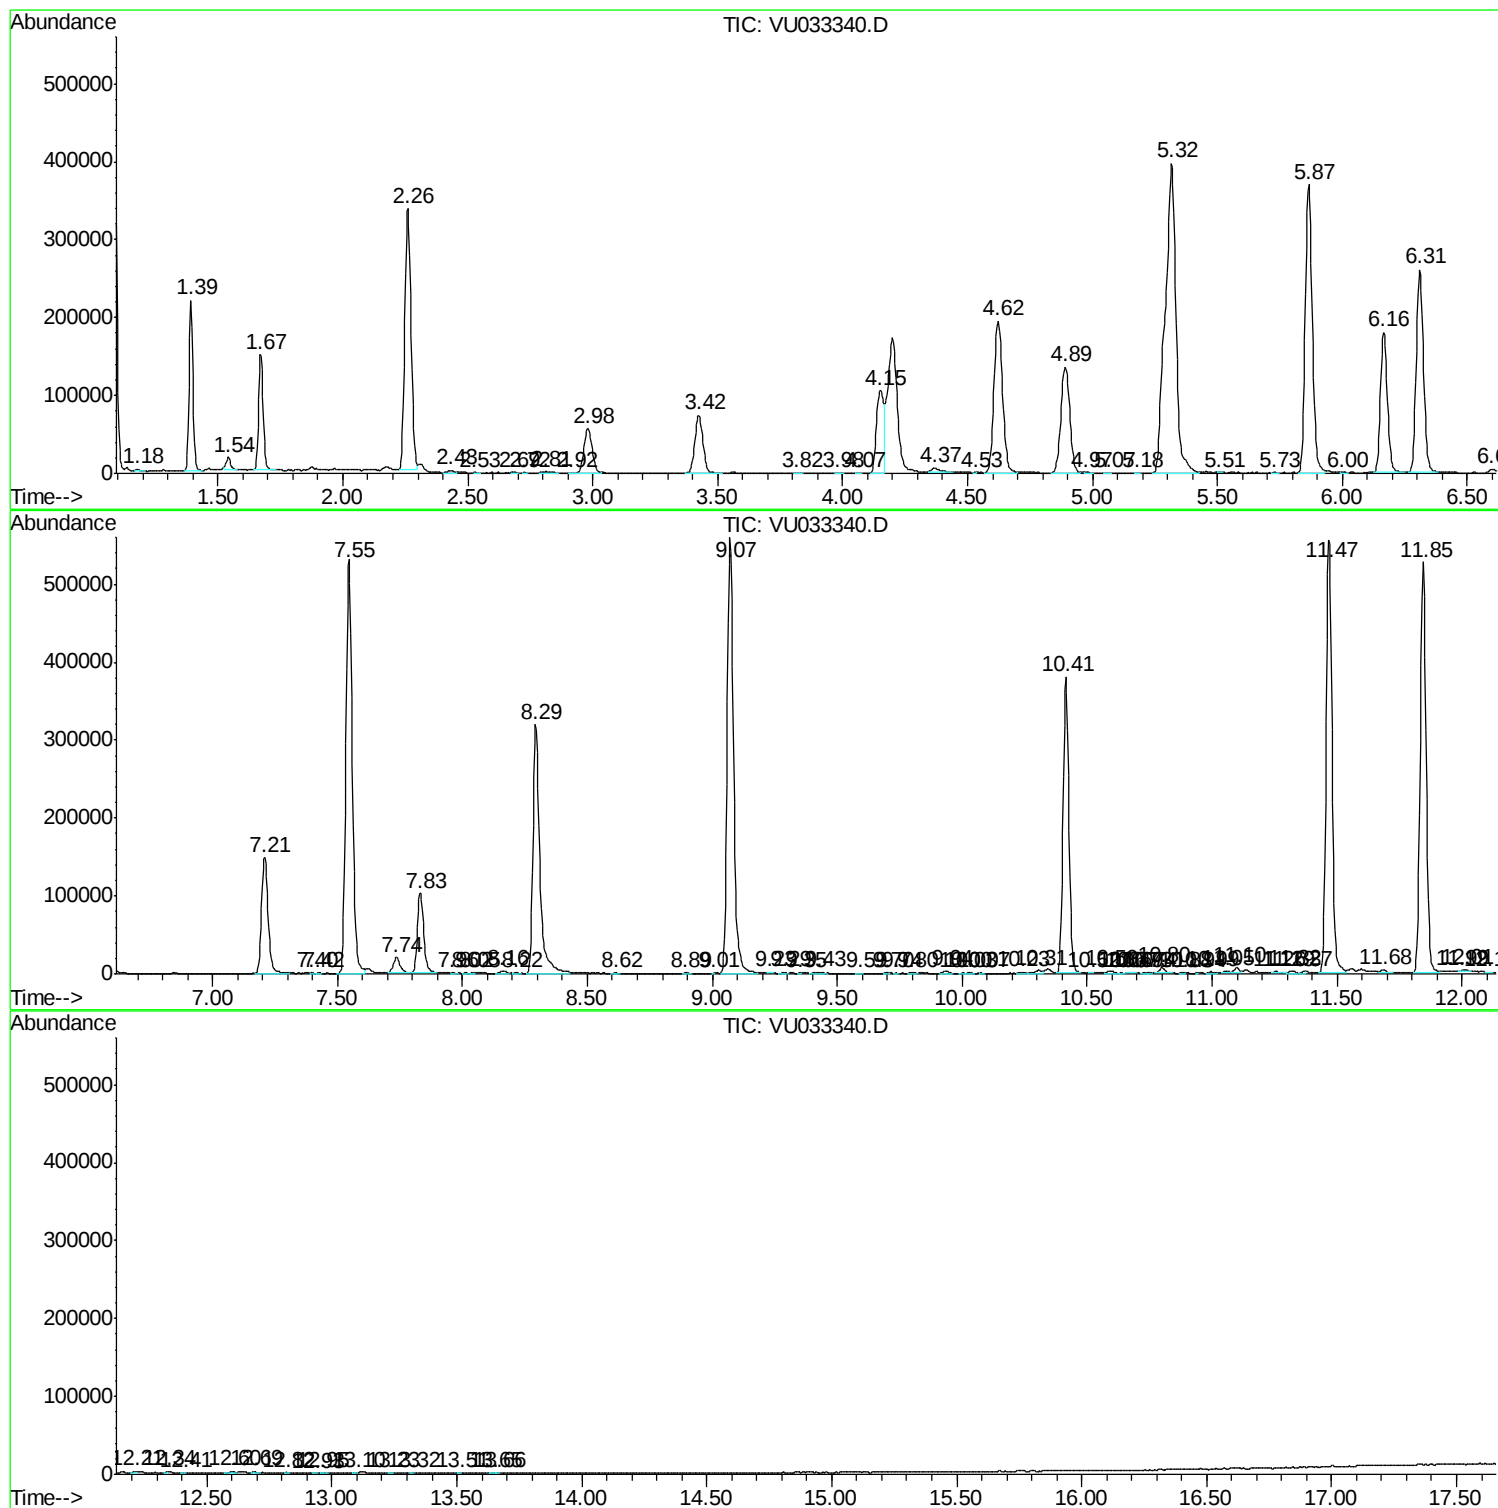

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU071919\
Data File : VU033340.D
Acq On : 19 Jul 2019 16:25
Operator : JC/SP
Sample : K3920-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A42M6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU071919\
Data File : VU033340.D
Acq On : 19 Jul 2019 16:25
Operator : JC/SP
Sample : K3920-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A42M6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc