

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071921\
 Data File : VU044356.D
 Acq On : 19 Jul 2021 10:16
 Operator : SY/MD
 Sample : VU0719WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0719WBL01

Quant Time: Jul 20 01:20:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Jul 16 14:36:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.121	96	53172	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.642	95	20522	0.956	ug/l	0.00
Spiked Amount 1.000			Recovery	=	96.000%	
68) 1,2-Dichlorobenzene-d4	12.201	152	19895	0.951	ug/l	0.00
Spiked Amount 1.000			Recovery	=	95.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071921\
Data File : VU044356.D
Acq On : 19 Jul 2021 10:16
Operator : SY/MD
Sample : VU0719WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0719WBL01

Quant Time: Jul 20 01:20:16 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Jul 16 14:36:39 2021
Response via : Initial Calibration

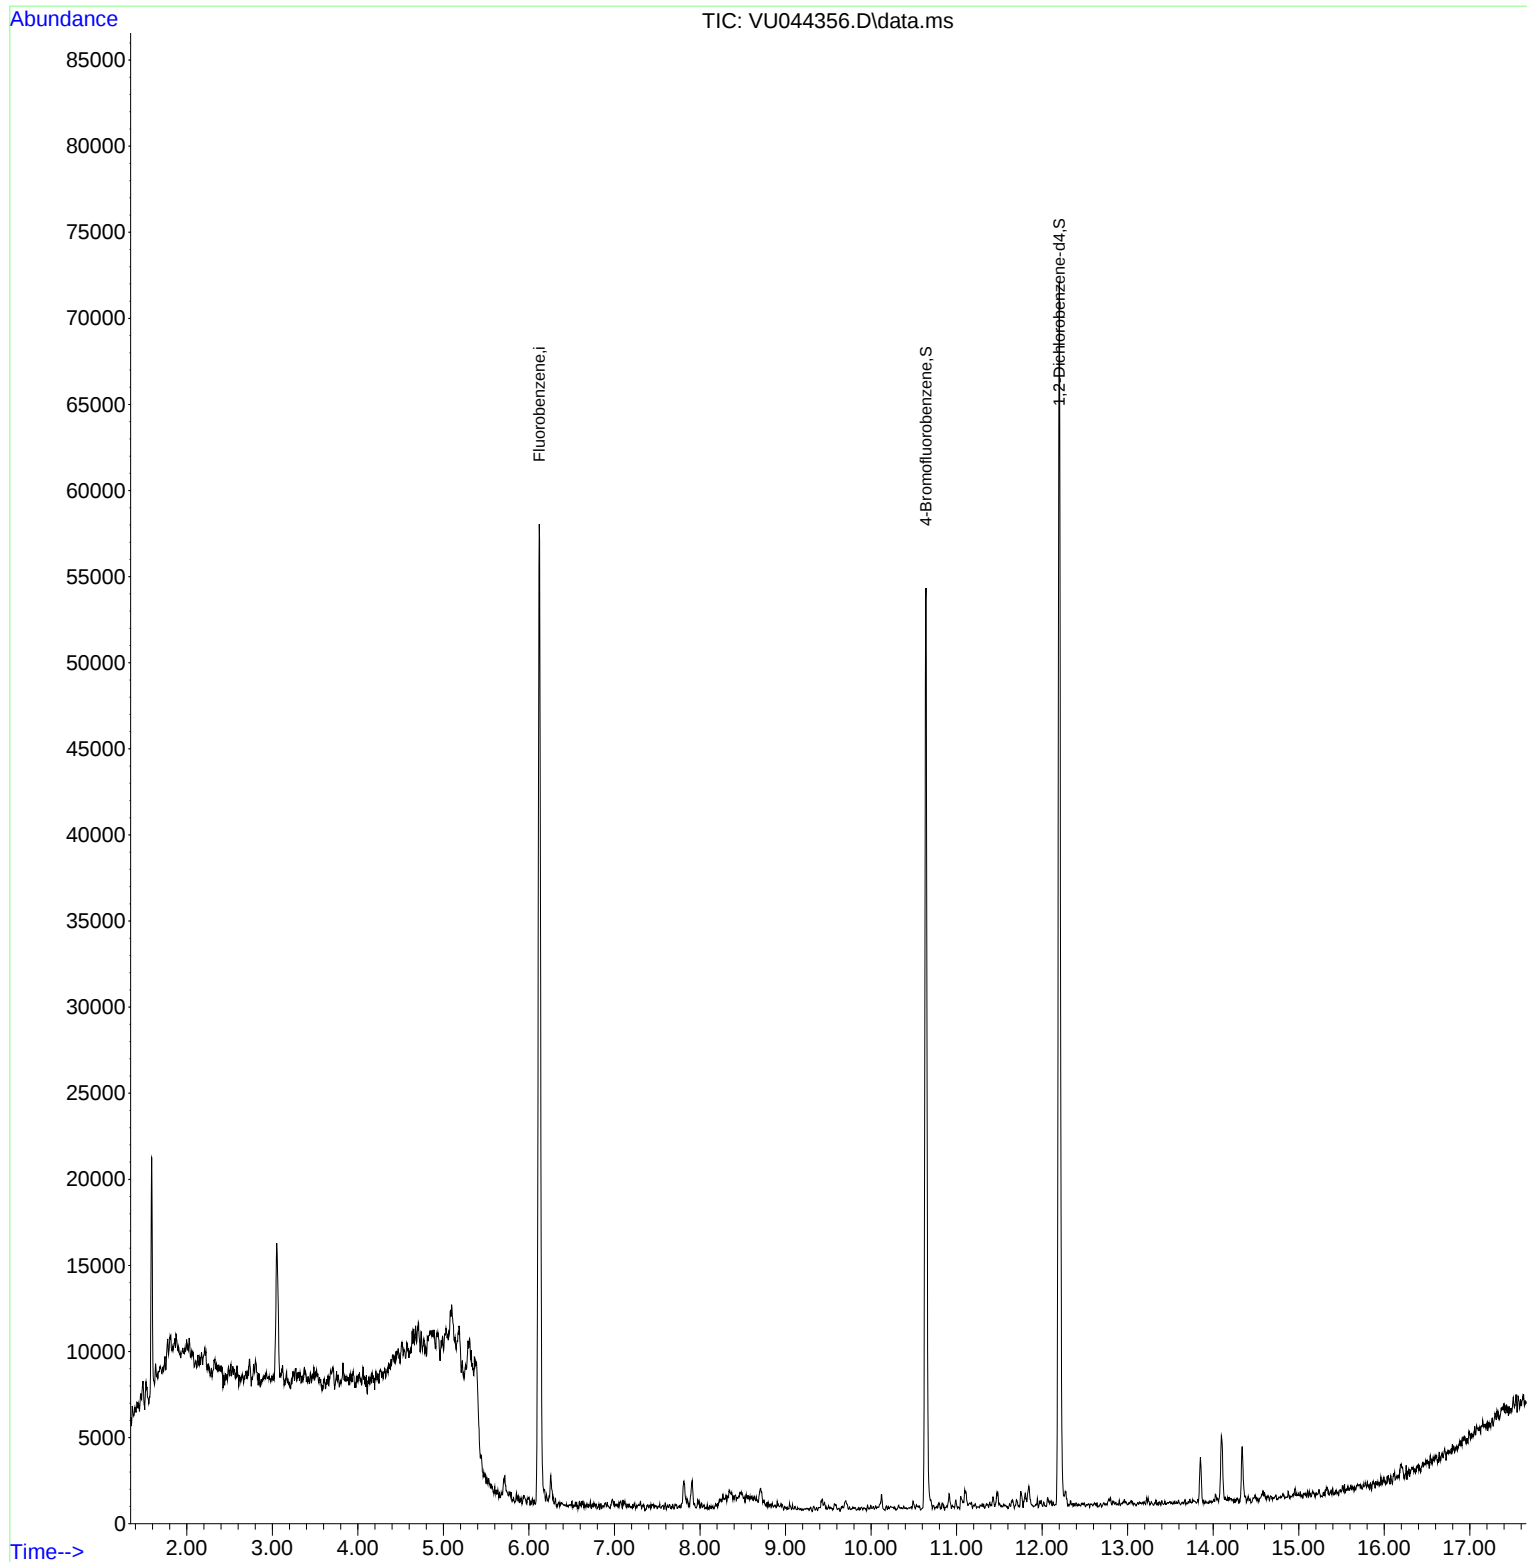




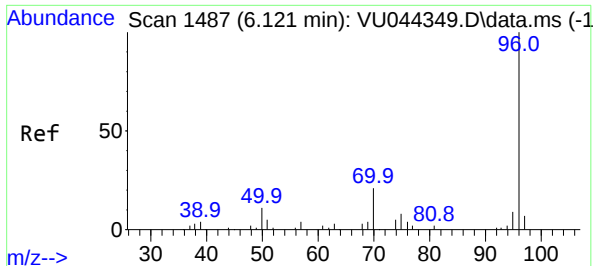


#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.121 min Scan# 1487
Delta R.T. 0.000 min
Lab File: VU044356.D
Acq: 19 Jul 2021 10:16

Instrument :
MSVOA_U
ClientSampleId :
VU0719WBL01

Tgt Ion: 96 Resp: 53172




Ion	Ratio	Lower	Upper
96	100		
70	21.1	16.2	24.2
95	9.2	7.3	10.9
97	6.7	0.0	0.0

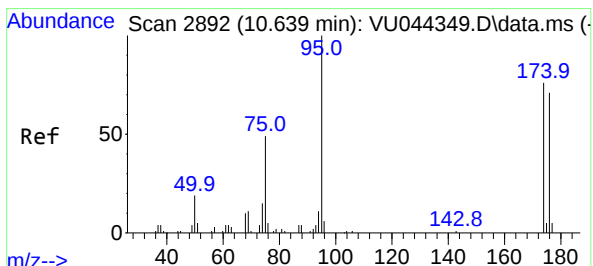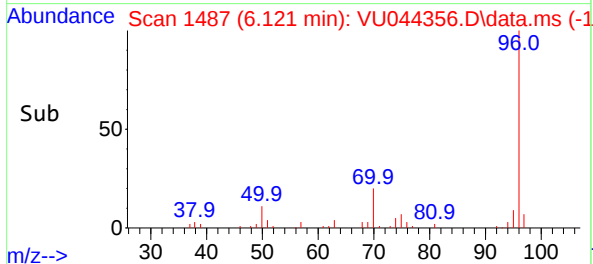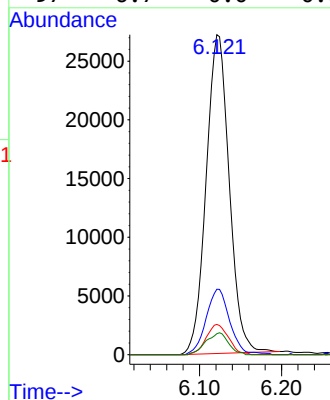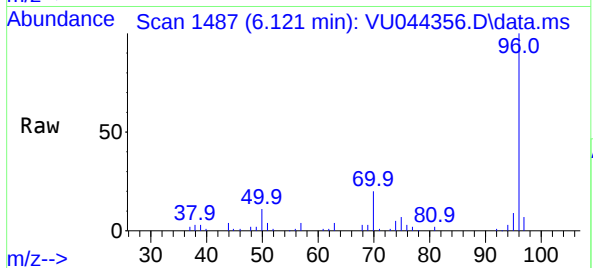


#57
4-Bromofluorobenzene
Concen: 0.956 ug/l
RT: 10.642 min Scan# 2893
Delta R.T. 0.003 min
Lab File: VU044356.D
Acq: 19 Jul 2021 10:16

Tgt Ion: 95 Resp: 20522


Ion	Ratio	Lower	Upper
95	100		
174	73.4	62.2	93.2
176	68.7	60.3	90.5

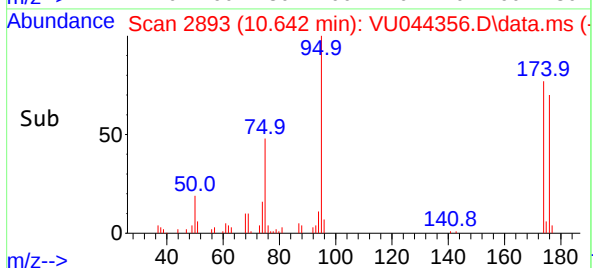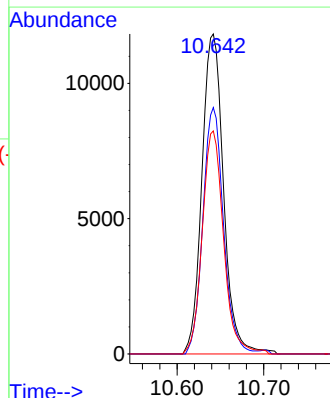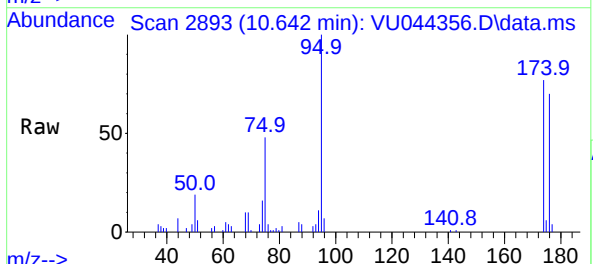

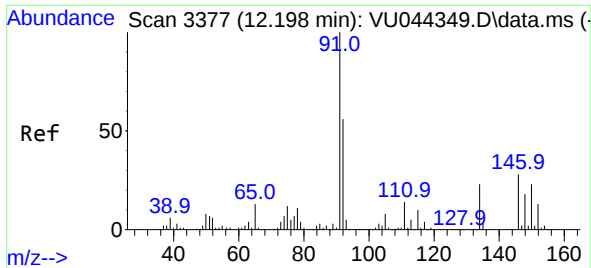

#68
1,2-Dichlorobenzene-d4
Concen: 0.951 ug/l
RT: 12.201 min Scan# 31
Delta R.T. 0.003 min
Lab File: VU044356.D
Acq: 19 Jul 2021 10:16

Instrument :
MSVOA_U
ClientSampleId :
VU0719WBL01

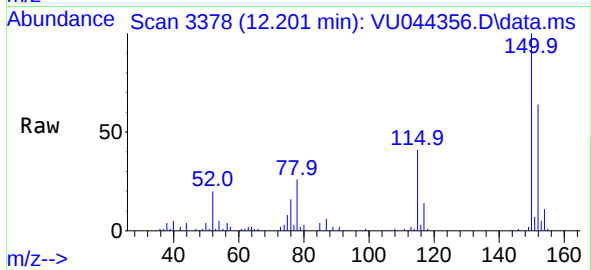

Tgt Ion	Ratio	Lower	Upper
152	100		
115	65.9	0.0	257.0
150	157.7	0.0	630.2

