

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071921\
 Data File : VU044356.D
 Acq On : 19 Jul 2021 10:16
 Operator : SY/MD
 Sample : VU0719WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0719WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU044356.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.050	528	532	544	rVB3	7809	12710	10.34%	3.526%
2	6.121	1473	1487	1503	rBV	56904	111533	90.75%	30.940%
3	6.256	1525	1529	1536	rVB4	1336	1469	1.20%	0.408%
4	7.812	2006	2013	2022	rBV3	1305	2000	1.63%	0.555%
5	7.909	2034	2043	2050	rBV3	1503	2345	1.91%	0.651%
6	10.124	2721	2732	2740	rVB6	875	1258	1.02%	0.349%
7	10.642	2881	2893	2909	rBV	53409	87663	71.33%	24.319%
8	11.751	3233	3238	3246	rVB2	960	1256	1.02%	0.348%
9	11.844	3260	3267	3278	rVB3	1111	1930	1.57%	0.535%
10	12.201	3366	3378	3394	rBV	71040	122903	100.00%	34.095%
11	13.851	3884	3891	3901	rVB4	2661	3737	3.04%	1.037%
12	14.095	3957	3967	3979	rBV2	3847	6792	5.53%	1.884%
13	14.339	4034	4043	4053	rBV4	3200	4881	3.97%	1.354%




Sum of corrected areas: 360477

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071921\
Data File : VU044356.D
Acq On : 19 Jul 2021 10:16
Operator : SY/MD
Sample : VU0719WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0719WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

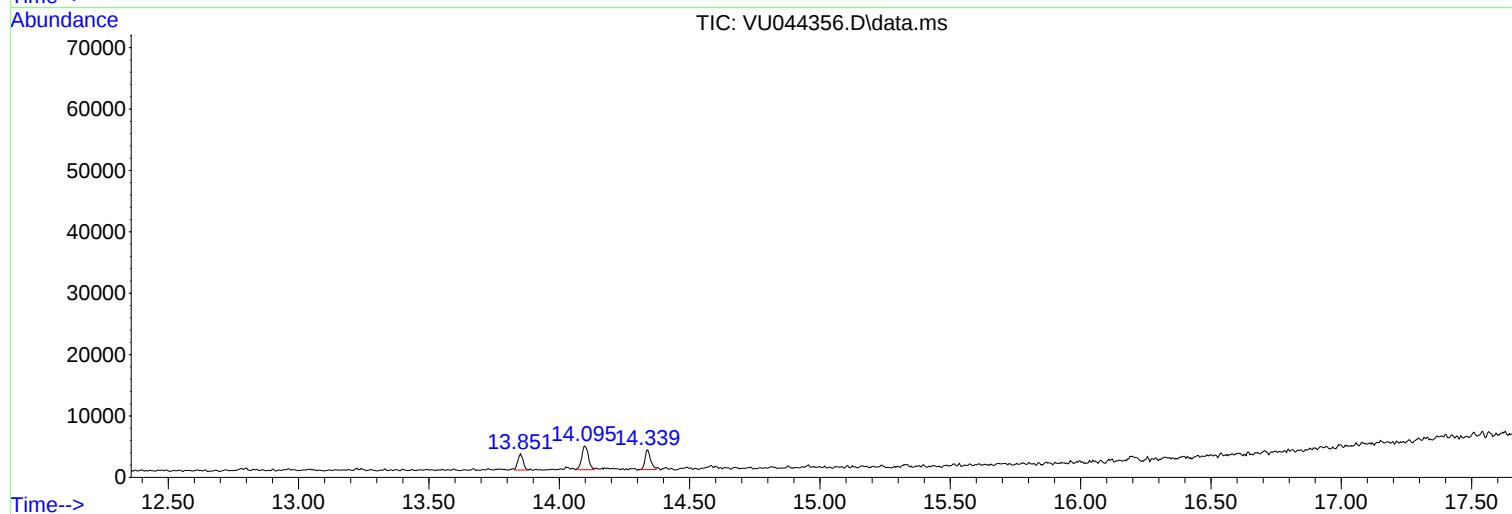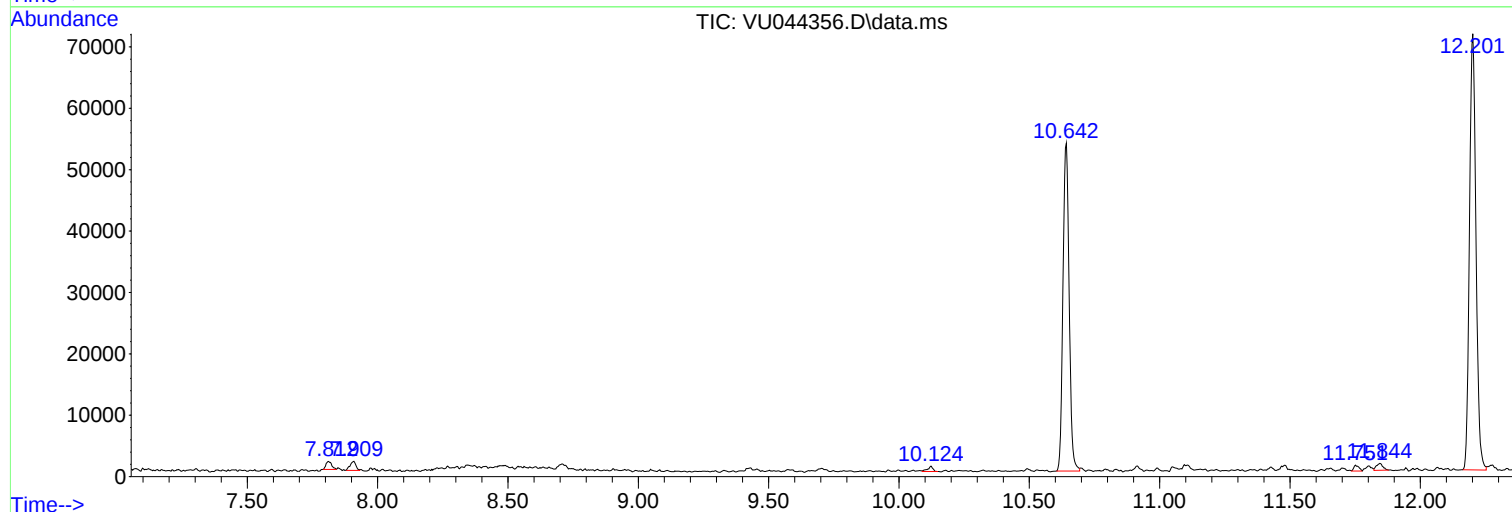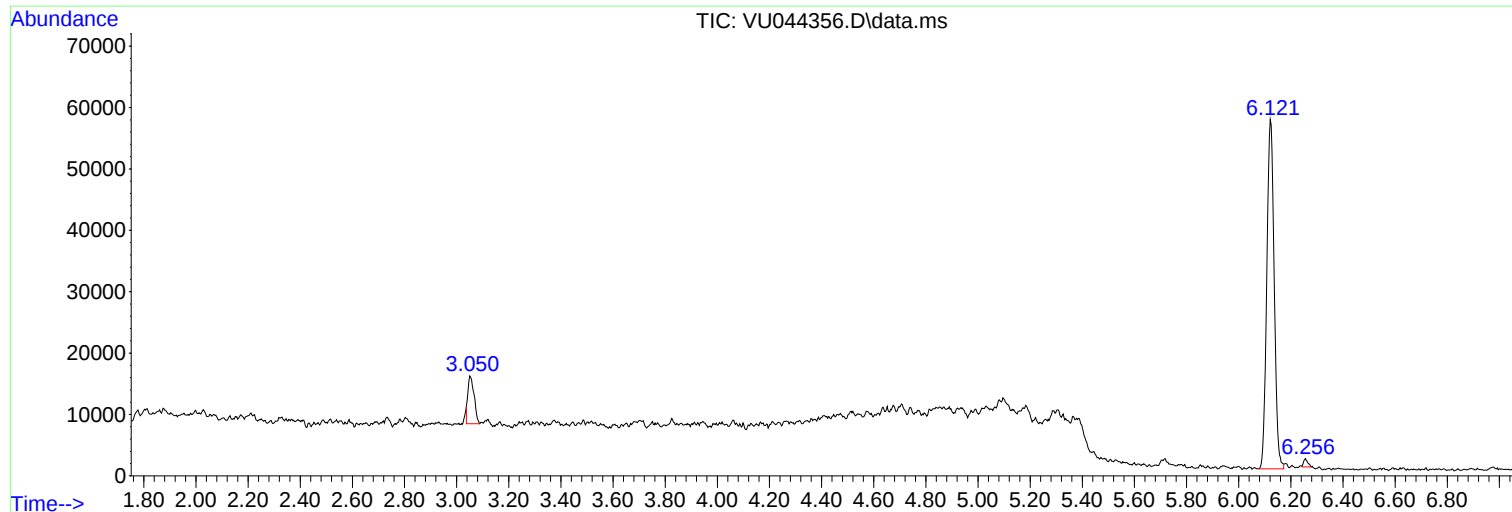

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071921\
Data File : VU044356.D
Acq On : 19 Jul 2021 10:16
Operator : SY/MD
Sample : VU0719WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0719WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071921\
Data File : VU044356.D
Acq On : 19 Jul 2021 10:16
Operator : SY/MD
Sample : VU0719WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0719WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------