

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071921\
Data File : VU044359.D
Acq On : 19 Jul 2021 11:50
Operator : SY/MD
Sample : M3035-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-THM-WS

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU044359.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.099	1152	1169	1209	rBV	1136610	2484969	100.00%	37.600%
2	6.121	1473	1487	1501	rBV	55903	107628	4.33%	1.629%
3	7.115	1780	1796	1829	rBV	969840	1824531	73.42%	27.607%
4	8.819	2312	2326	2359	rBV	813817	1444499	58.13%	21.857%
5	10.298	2773	2786	2810	rBV	316347	542190	21.82%	8.204%
6	10.639	2882	2892	2912	rBV	52568	87299	3.51%	1.321%
7	12.201	3366	3378	3395	rBV	70372	117760	4.74%	1.782%




Sum of corrected areas: 6608876

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071921\
Data File : VU044359.D
Acq On : 19 Jul 2021 11:50
Operator : SY/MD
Sample : M3035-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-THM-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

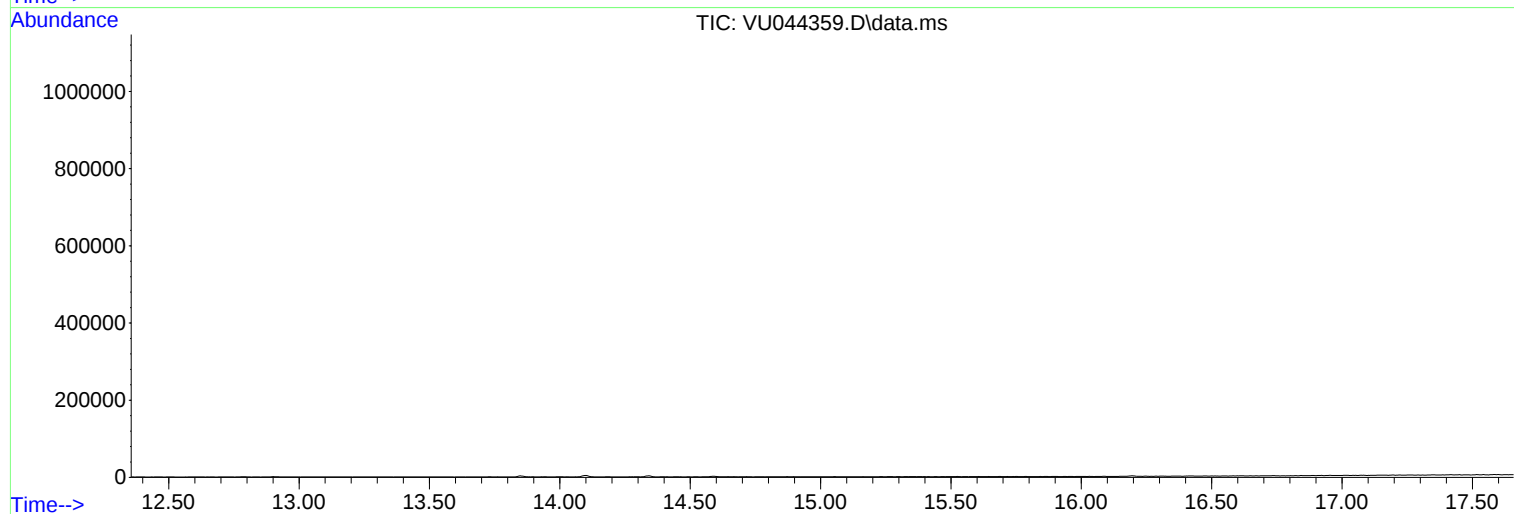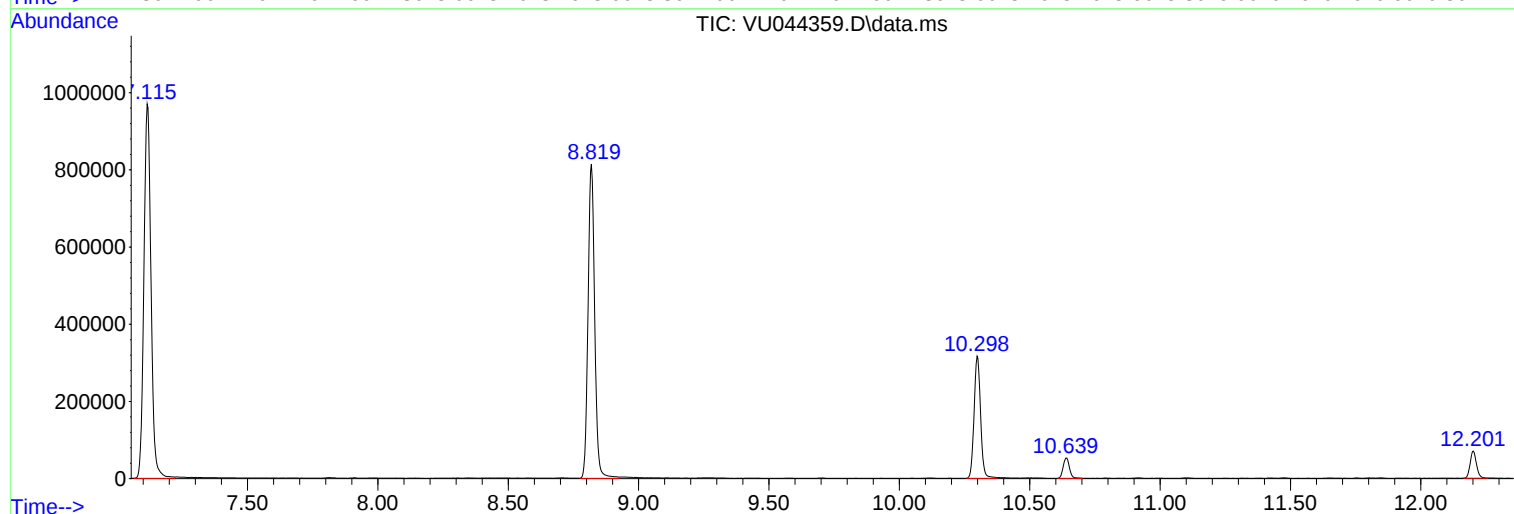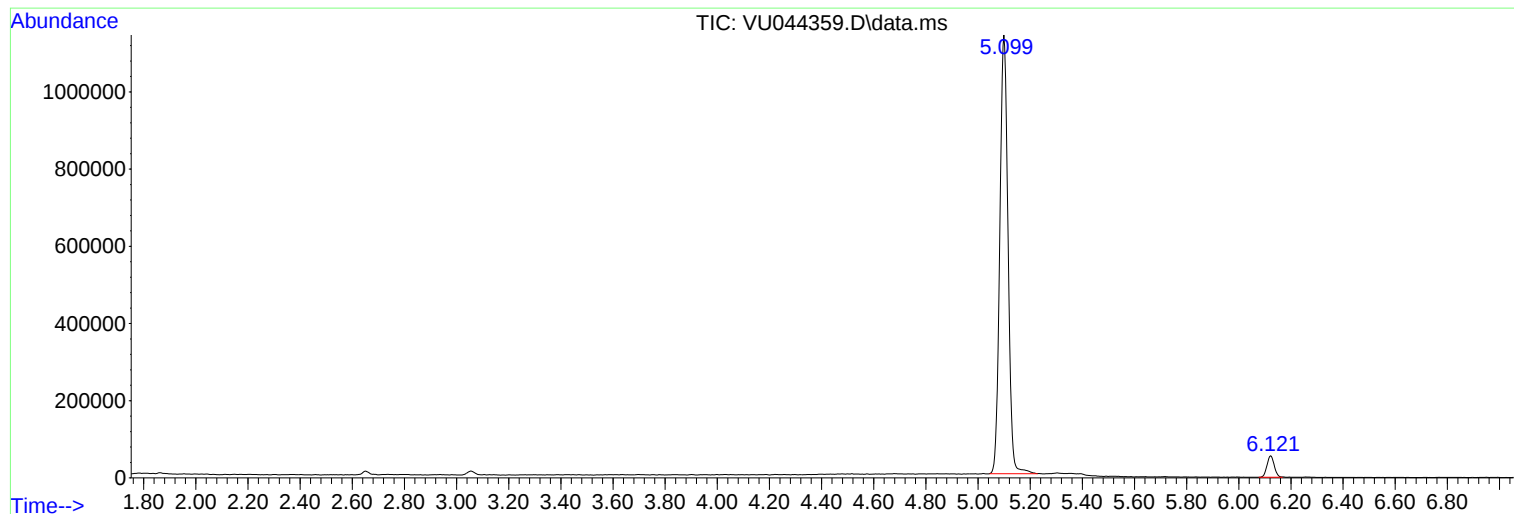

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071921\
Data File : VU044359.D
Acq On : 19 Jul 2021 11:50
Operator : SY/MD
Sample : M3035-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-THM-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071921\
Data File : VU044359.D
Acq On : 19 Jul 2021 11:50
Operator : SY/MD
Sample : M3035-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-THM-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc