

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071921\
 Data File : VU044361.D
 Acq On : 19 Jul 2021 14:28
 Operator : SY/MD
 Sample : M3035-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PT-UNRVOA-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU044361.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.938	176	186	204	rBV	361049	476031	14.33%	1.353%
2	3.054	521	533	552	rVB	108873	201305	6.06%	0.572%
3	3.379	615	634	654	rBV	1406955	3322907	100.00%	9.441%
4	3.880	773	790	809	rVB	309062	729471	21.95%	2.073%
5	4.674	1020	1037	1057	rVB	281326	687889	20.70%	1.954%
6	4.983	1119	1133	1151	rBV	186638	402059	12.10%	1.142%
7	5.530	1288	1303	1325	rBV	189740	384382	11.57%	1.092%
8	6.121	1473	1487	1502	rBV	55164	108118	3.25%	0.307%
9	6.928	1724	1738	1768	rBV	102559	197521	5.94%	0.561%
10	7.616	1938	1952	1977	rBV	295250	532935	16.04%	1.514%
11	8.221	2125	2140	2165	rBV	542572	944274	28.42%	2.683%
12	8.584	2234	2253	2276	rBV	565806	1016990	30.61%	2.890%
13	9.542	2536	2551	2575	rBV	861610	1448914	43.60%	4.117%
14	10.491	2833	2846	2873	rBV	386626	614661	18.50%	1.746%
15	10.639	2882	2892	2916	rVB	56838	91269	2.75%	0.259%
16	10.790	2922	2939	2946	rBV2	1125176	1864512	56.11%	5.298%
17	10.832	2946	2952	2965	rVV	441145	717613	21.60%	2.039%
18	10.912	2965	2977	2990	rVV	1170653	1767781	53.20%	5.023%
19	10.993	2990	3002	3016	rVB	1188731	1883397	56.68%	5.351%
20	11.099	3022	3035	3068	rVB2	1764103	3057172	92.00%	8.686%
21	11.427	3118	3137	3145	rBV	1463422	2309235	69.49%	6.561%
22	11.475	3145	3152	3178	rVB	770297	1168665	35.17%	3.321%
23	11.648	3191	3206	3226	rBV	791044	1206215	36.30%	3.427%
24	11.751	3226	3238	3246	rVV	628657	996080	29.98%	2.830%
25	11.800	3246	3253	3276	rVB	502826	760254	22.88%	2.160%
26	12.214	3363	3382	3412	rBV	1232690	1943302	58.48%	5.521%
27	14.028	3933	3946	3956	rBV	1008053	1547018	46.56%	4.396%
28	14.092	3956	3966	3988	rVB	1589888	2540146	76.44%	7.217%
29	14.336	4029	4042	4068	rBV	1403647	2275163	68.47%	6.464%




Sum of corrected areas: 35195279

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071921\
Data File : VU044361.D
Acq On : 19 Jul 2021 14:28
Operator : SY/MD
Sample : M3035-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

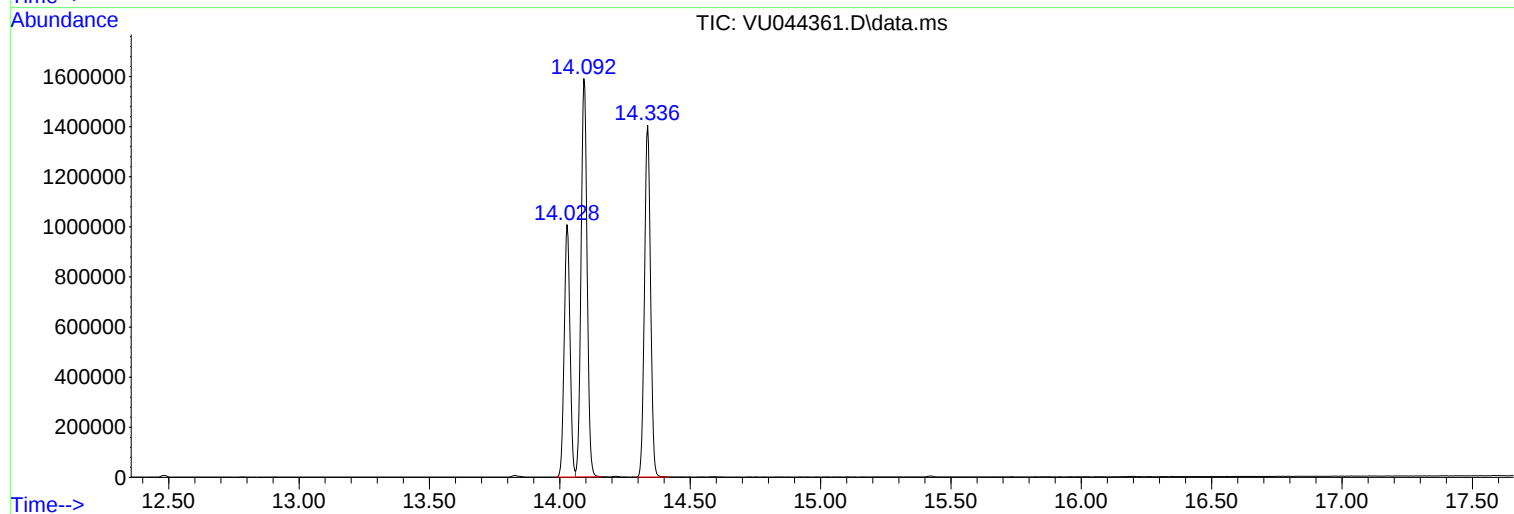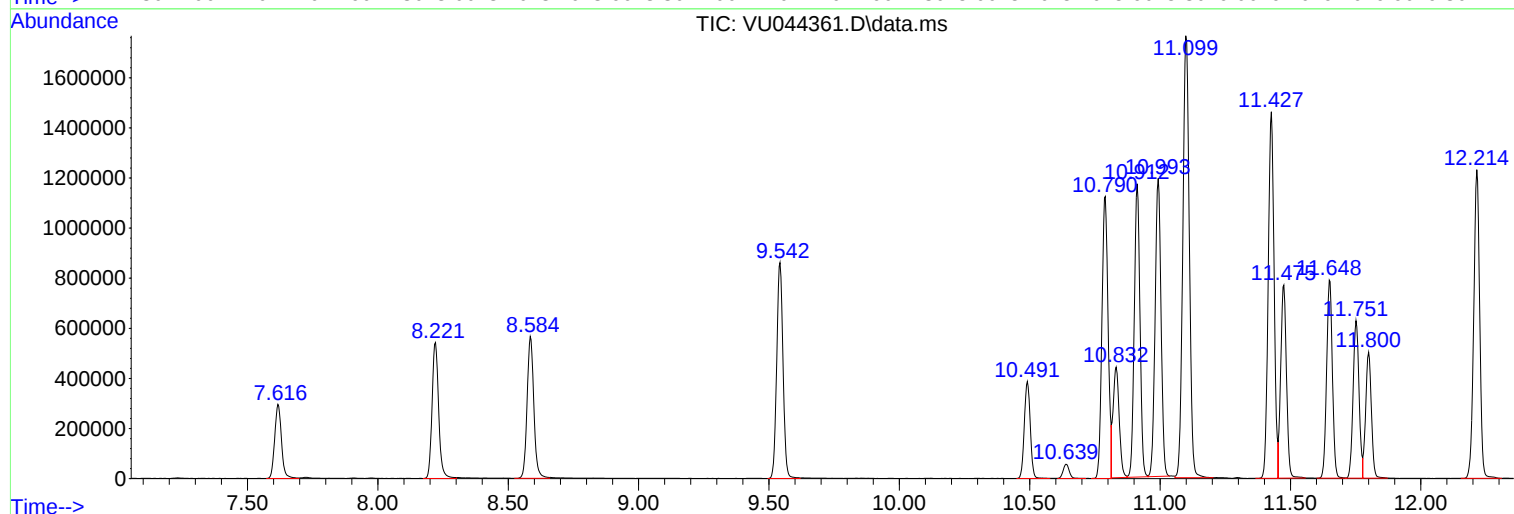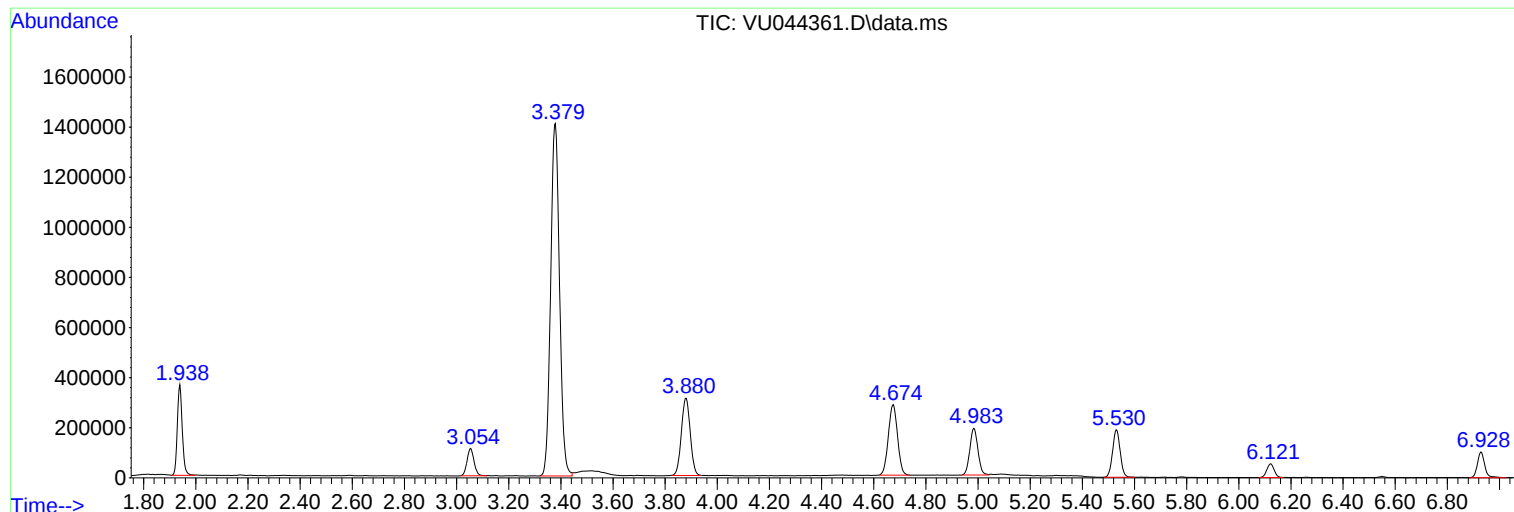

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071921\
Data File : VU044361.D
Acq On : 19 Jul 2021 14:28
Operator : SY/MD
Sample : M3035-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071921\
Data File : VU044361.D
Acq On : 19 Jul 2021 14:28
Operator : SY/MD
Sample : M3035-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc