


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071921\
 Data File : VU044354.D
 Acq On : 19 Jul 2021 08:50
 Operator : SY/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Fri Jul 16 14:36:39 2021

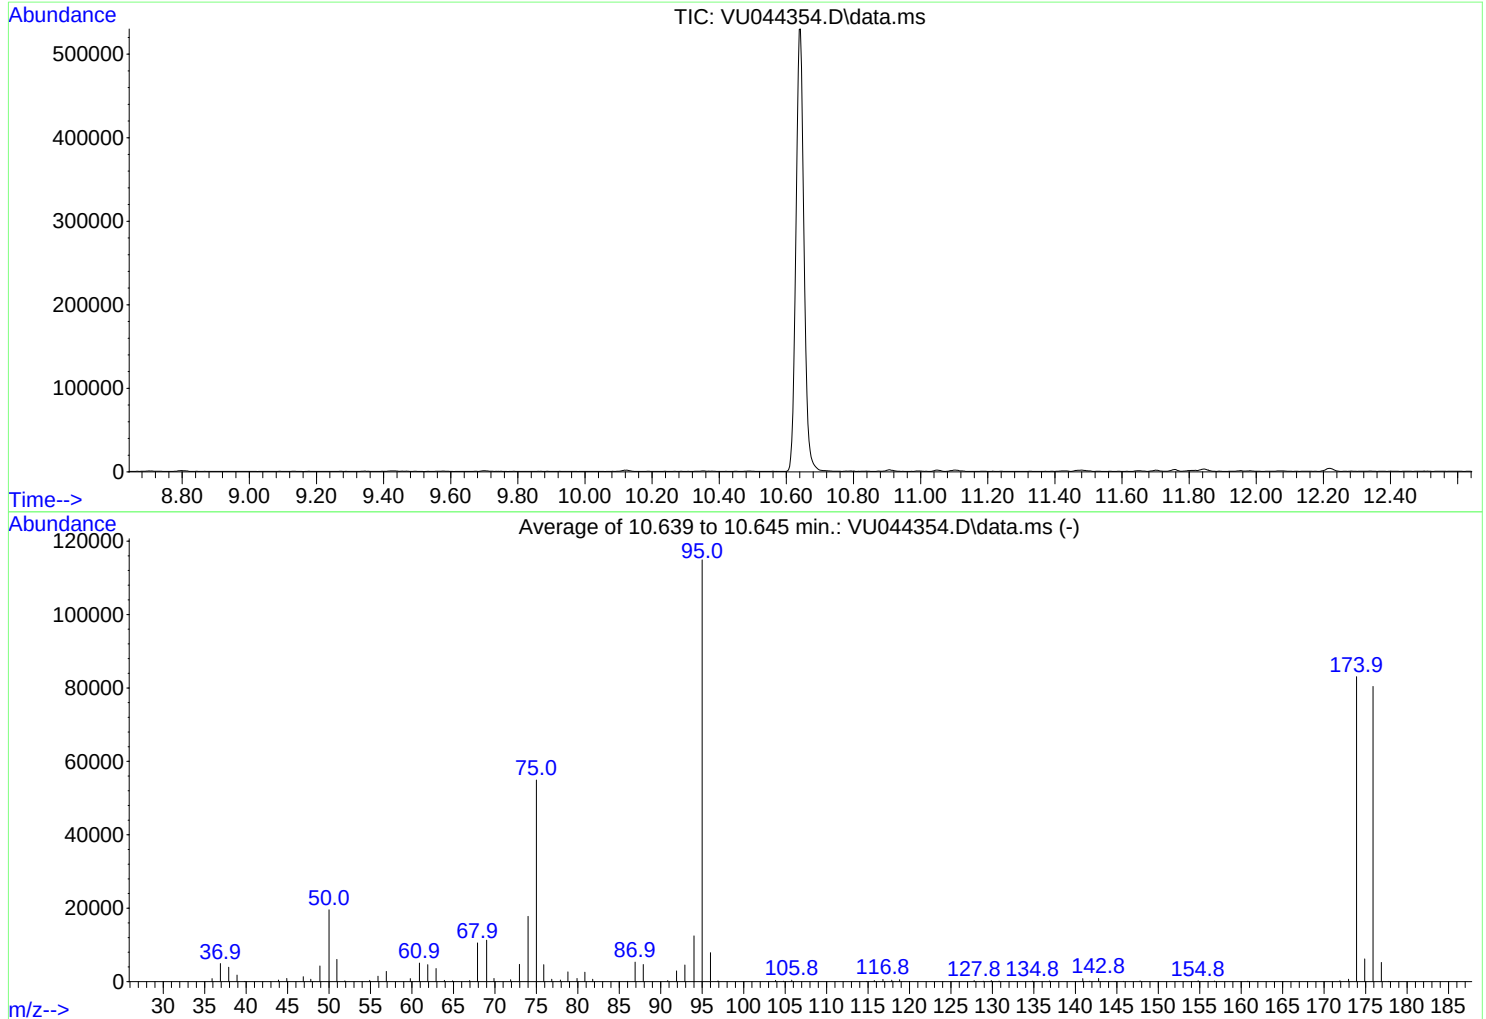

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	19579	PASS
75	95	30	60	47.8	54920	PASS
95	95	100	100	100.0	114901	PASS
96	95	5	9	6.9	7900	PASS
173	174	0.00	2	0.8	644	PASS
174	95	50	100	72.3	83096	PASS
175	174	5	9	7.4	6177	PASS
176	174	95	101	96.8	80424	PASS
177	176	5	9	6.5	5232	PASS