

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
 Data File : VU049788.D
 Acq On : 19 Jul 2022 16:26
 Operator : SY/MD
 Sample : N3738-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jul 20 02:18:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 19 02:09:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	177924	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	172576	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	72079	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	70488	46.954	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	93.900%		
7) Chloroethane-d5	1.903	69	54248	49.992	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	99.980%		
11) 1,1-Dichloroethene-d2	2.562	63	89960	33.925	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	67.860%		
21) 2-Butanone-d5	4.620	46	143819	112.223	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	112.220%		
24) Chloroform-d	5.063	84	130560	49.103	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.200%		
26) 1,2-Dichloroethane-d4	5.700	65	94397	52.456	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	104.920%		
32) Benzene-d6	5.726	84	245813	46.886	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.780%		
36) 1,2-Dichloropropane-d6	6.690	67	87584	49.666	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	99.340%		
41) Toluene-d8	7.896	98	203174	44.500	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.000%		
43) trans-1,3-Dichloroprop...	8.179	79	34871	46.934	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	93.860%		
47) 2-Hexanone-d5	8.632	63	72496	91.391	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	91.390%		
56) 1,1,2,2-Tetrachloroeth...	10.754	84	124570	50.485	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	100.980%		
66) 1,2-Dichlorobenzene-d4	12.192	152	70898	52.169	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	104.340%		
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.565	101	741	0.541	ug/L #	20
12) 1,1-Dichloroethene	2.562	96	655	0.515	ug/L #	1
16) Methylene chloride	3.041	84	2805	1.751	ug/L	96
35) Methylcyclohexane	6.690	83	19411	7.878	ug/L #	17
37) 1,2-Dichloropropane	6.690	63	9810	5.456	ug/L #	89
39) cis-1,3-Dichloropropene	7.565	75	2468	1.018	ug/L #	70
44) trans-1,3-Dichloropropene	8.176	75	1602	0.704	ug/L	87
60) 1,2,3-Trichloropropane	11.812	75	9688	5.046	ug/L #	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
Data File : VU049788.D
Acq On : 19 Jul 2022 16:26
Operator : SY/MD
Sample : N3738-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jul 20 02:18:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 19 02:09:49 2022
Response via : Initial Calibration

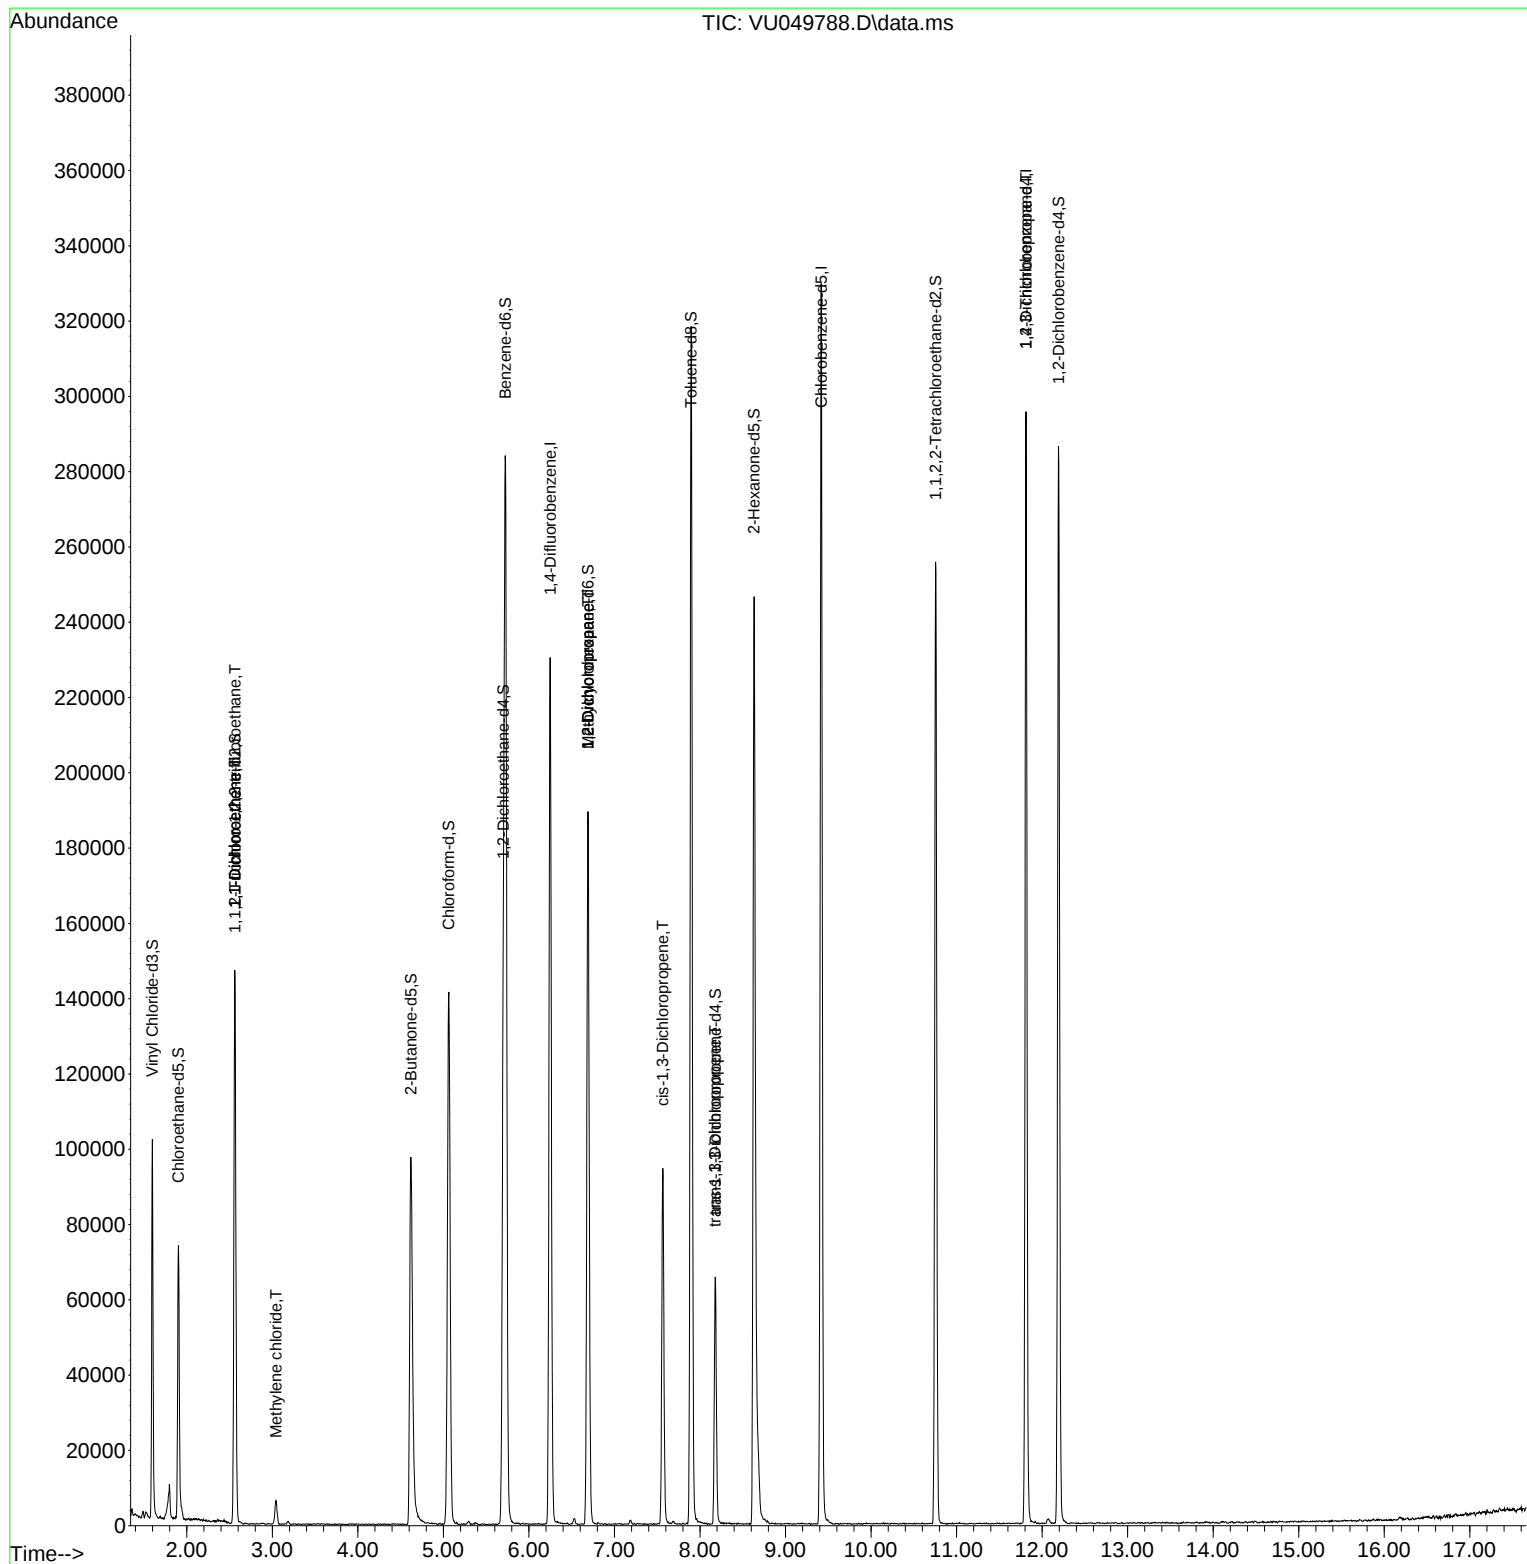

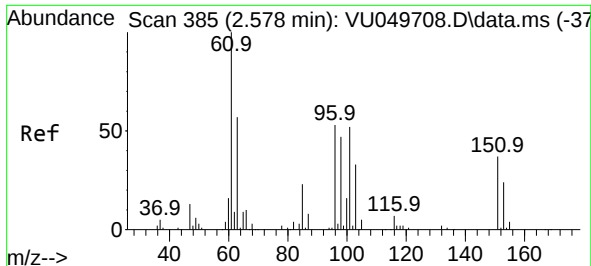

#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 0.541 ug/L

RT: 2.565 min Scan# 381

Delta R.T. -0.010 min

Lab File: VU049788.D





Acq: 19 Jul 2022 16:26

Instrument :

MSVOA_U

ClientSampleId :

Tgt Ion:	101	Resp:	741
Ion Ratio	Lower	Upper	
101	100		
85	0.0	37.3	55.9#
151	0.0	56.9	85.3#

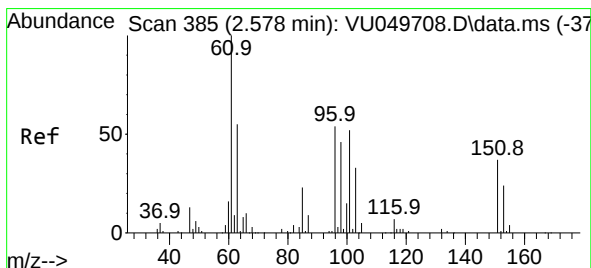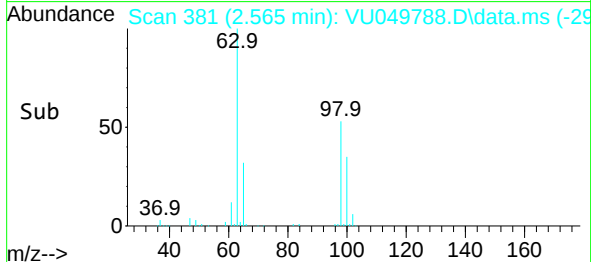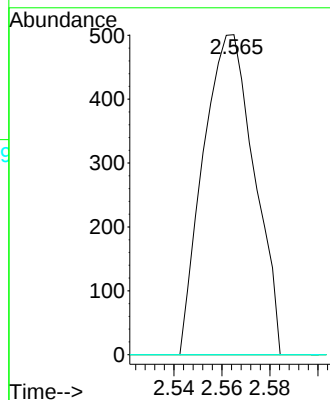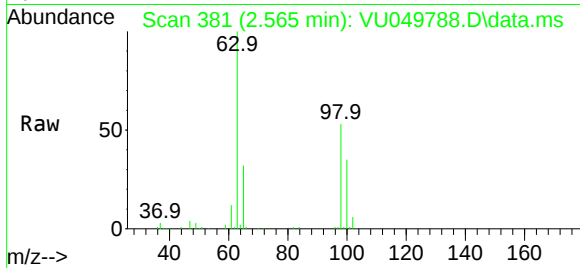

#12

1,1-Dichloroethene

Concen: 0.515 ug/L




RT: 2.562 min Scan# 380


Delta R.T. -0.013 min

Lab File: VU049788.D

Acq: 19 Jul 2022 16:26


Tgt Ion:	96	Resp:	655
Ion Ratio	Lower	Upper	
96	100		
61	1780.6	129.6	240.6#
63	14576.2	79.0	146.6#

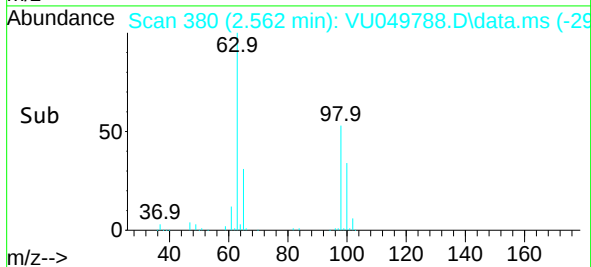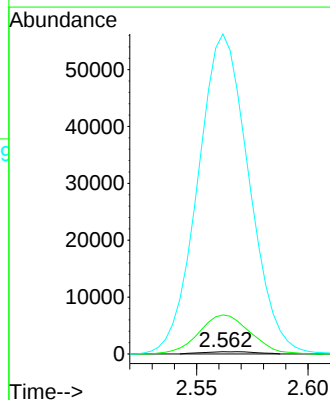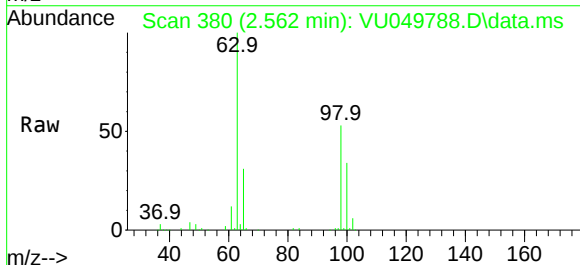



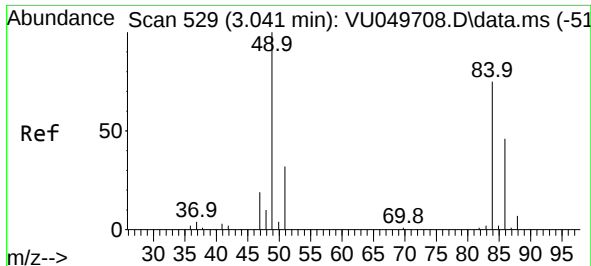


#16
Methylene chloride
Concen: 1.751 ug/L
RT: 3.041 min Scan# 51
Delta R.T. -0.000 min
Lab File: VU049788.D
Acq: 19 Jul 2022 16:26


Instrument :
MSVOA_U
ClientSampleId :

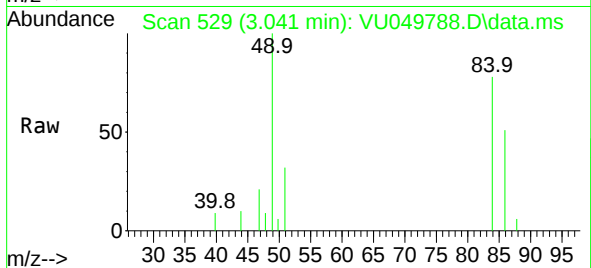



Tgt Ion: 84 Resp: 2805
Ion Ratio Lower Upper
84 100
86 65.6 45.6 84.6
49 128.5 94.4 175.4

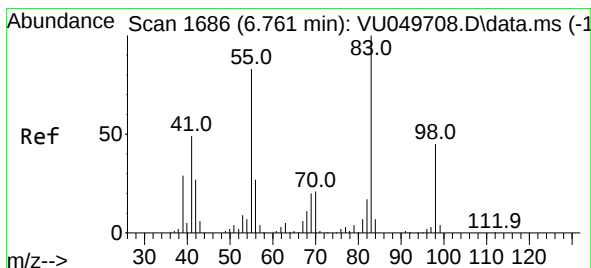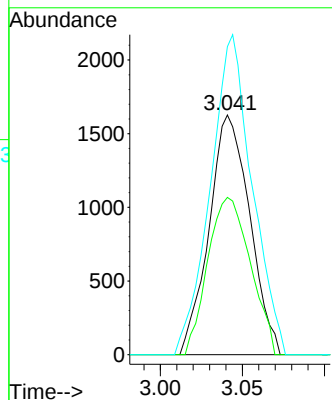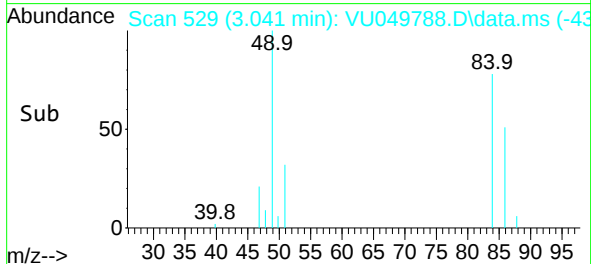


#35
Methylcyclohexane
Concen: 7.878 ug/L
RT: 6.690 min Scan# 1664
Delta R.T. -0.071 min
Lab File: VU049788.D
Acq: 19 Jul 2022 16:26

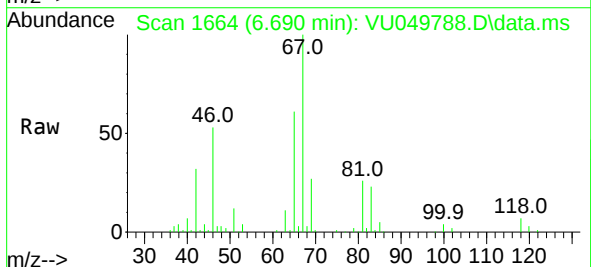

Tgt Ion: 83 Resp: 19411
Ion Ratio Lower Upper
83 100
55 0.2 66.0 99.0#
98 0.6 34.6 51.8#



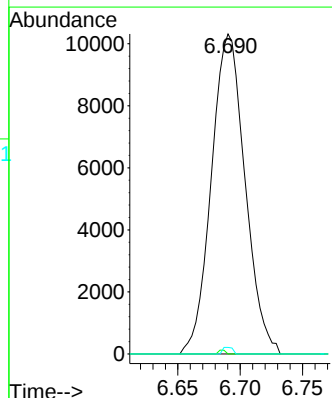
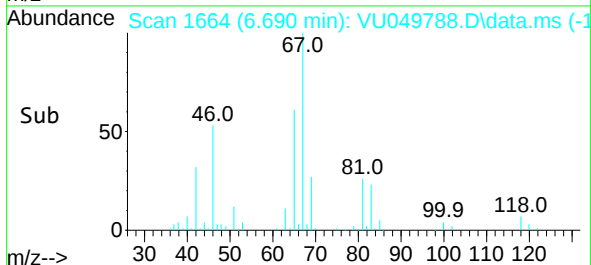


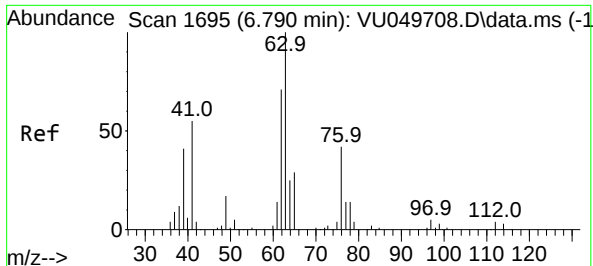

#37
1,2-Dichloropropane
Concen: 5.456 ug/L
RT: 6.690 min Scan# 11
Delta R.T. -0.100 min
Lab File: VU049788.D
Acq: 19 Jul 2022 16:26




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 63 Resp: 9810
Ion Ratio Lower Upper
63 100
112 0.0 2.8 4.2#

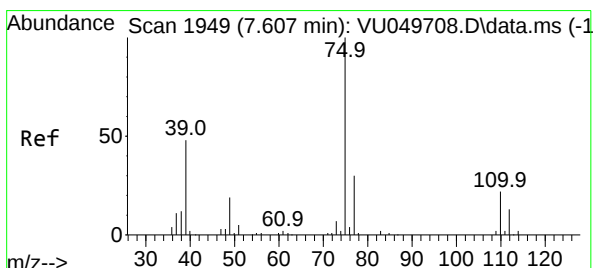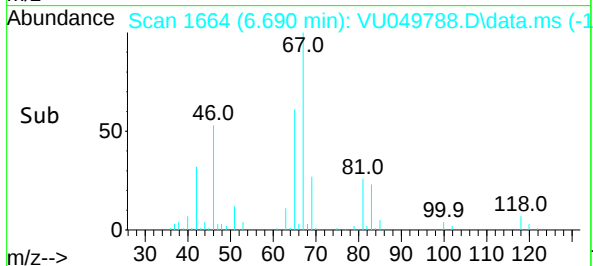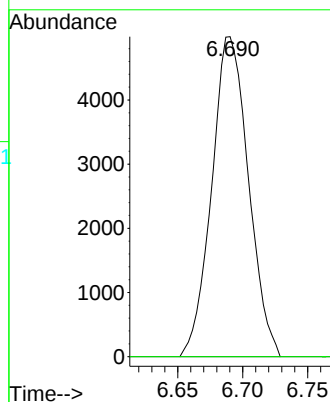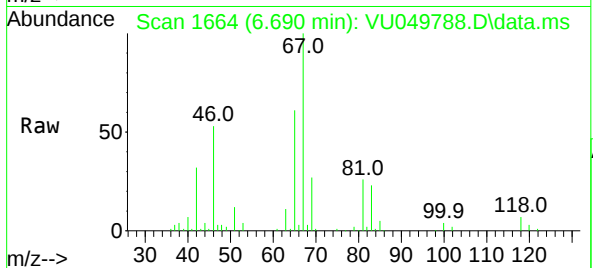

#39
cis-1,3-Dichloropropene
Concen: 1.018 ug/L
RT: 7.565 min Scan# 1936
Delta R.T. -0.042 min
Lab File: VU049788.D
Acq: 19 Jul 2022 16:26


Tgt Ion: 75 Resp: 2468
Ion Ratio Lower Upper
75 100
77 49.0 22.6 42.0#

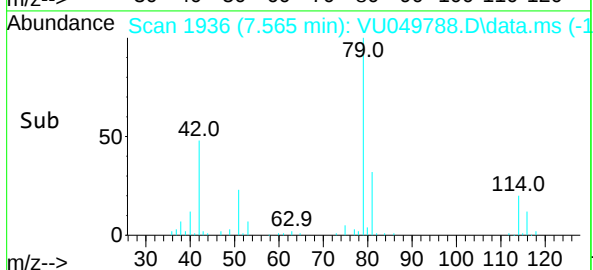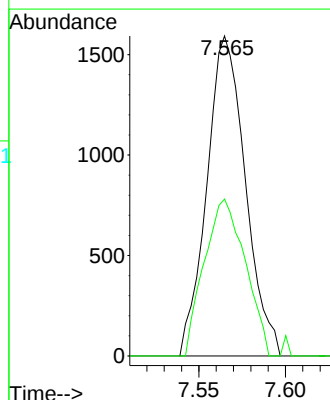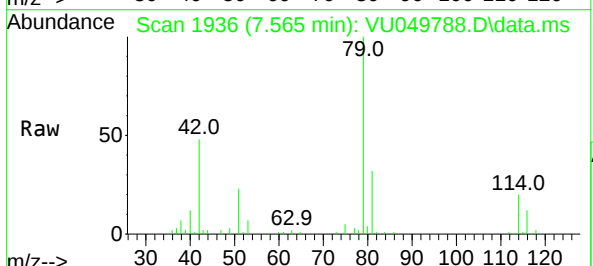



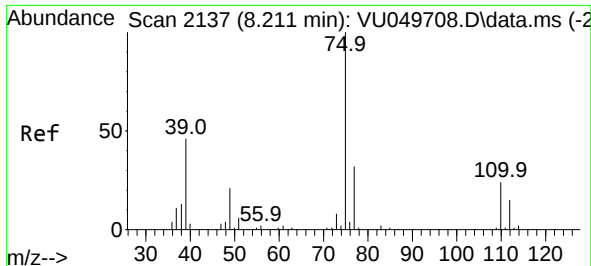


#44
trans-1,3-Dichloropropene
Concen: 0.704 ug/L
RT: 8.176 min Scan# 2137
Delta R.T. -0.032 min
Lab File: VU049788.D
Acq: 19 Jul 2022 16:26

Instrument :
MSVOA_U
ClientSampleId :

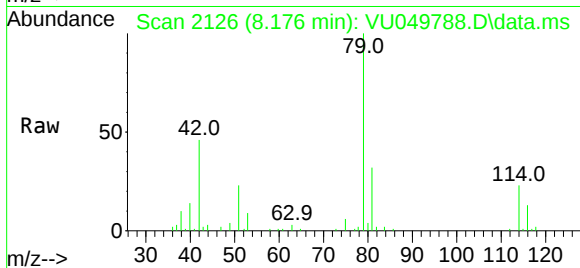

Tgt Ion: 75 Resp: 1602
Ion Ratio Lower Upper
75 100
77 25.1 22.5 41.9

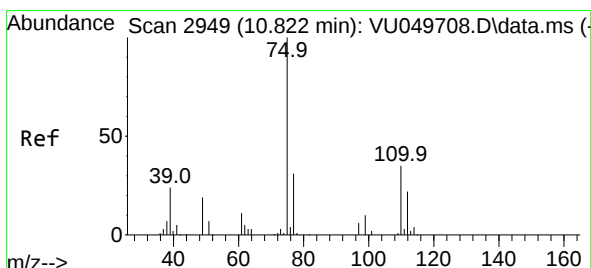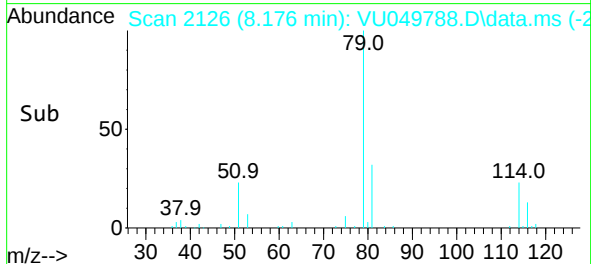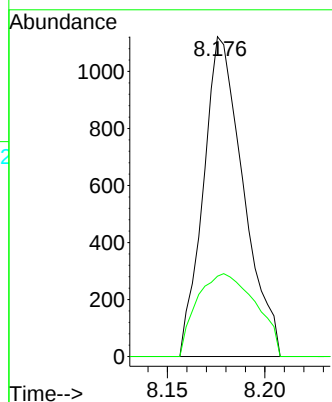

#60
1,2,3-Trichloropropane
Concen: 5.046 ug/L
RT: 11.812 min Scan# 3257
Delta R.T. 0.990 min
Lab File: VU049788.D
Acq: 19 Jul 2022 16:26

Tgt Ion: 75 Resp: 9688
Ion Ratio Lower Upper
75 100
77 37.2 25.5 38.3
110 0.2 28.9 43.3#

