

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
 Data File : VU049782.D
 Acq On : 19 Jul 2022 14:05
 Operator : SY/MD
 Sample : N3766-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COZD0

Quant Time: Jul 20 02:16:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 19 02:09:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	175657	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	167233	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	72180	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	69208	46.696	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	93.400%
7) Chloroethane-d5	1.900	69	53505	49.943	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	99.880%
11) 1,1-Dichloroethene-d2	2.562	63	87772	33.527	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.060%
21) 2-Butanone-d5	4.620	46	136242	107.683	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	107.680%
24) Chloroform-d	5.060	84	126982	48.374	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.740%
26) 1,2-Dichloroethane-d4	5.700	65	91708	51.619	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.240%
32) Benzene-d6	5.726	84	241160	47.468	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.940%
36) 1,2-Dichloropropane-d6	6.687	67	87536	51.225	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.440%
41) Toluene-d8	7.896	98	198608	44.890	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.780%
43) trans-1,3-Dichloroprop...	8.179	79	33680	46.779	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.560%
47) 2-Hexanone-d5	8.632	63	72140	93.848	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.850%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	119749	50.082	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	100.160%
66) 1,2-Dichlorobenzene-d4	12.192	152	69777	51.272	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.540%
Target Compounds						
13) Acetone	2.626	43	10675	8.878	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
Data File : VU049782.D
Acq On : 19 Jul 2022 14:05
Operator : SY/MD
Sample : N3766-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COZD0

Quant Time: Jul 20 02:16:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 19 02:09:49 2022
Response via : Initial Calibration

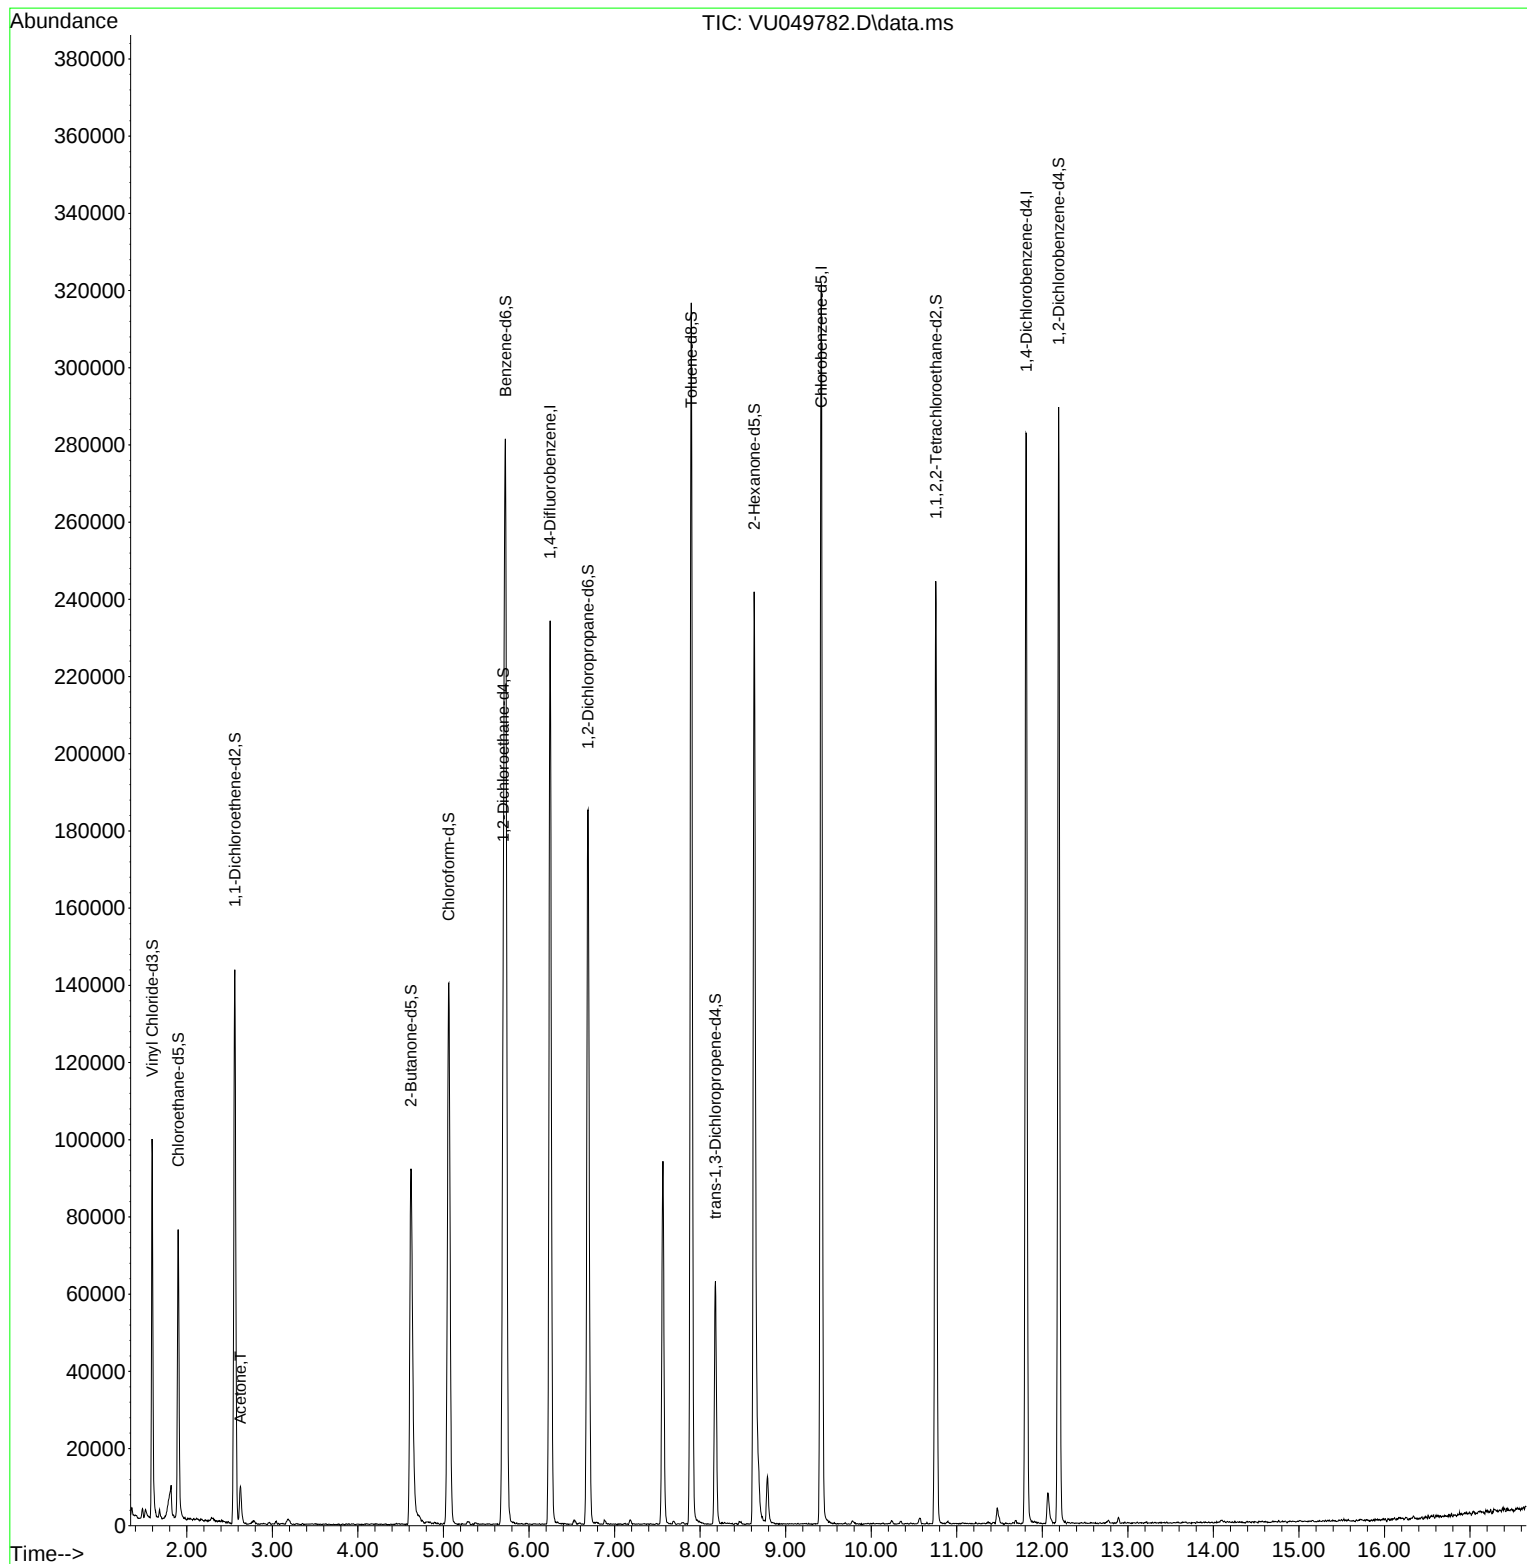

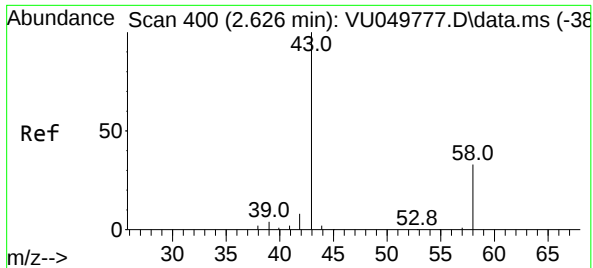

#13
 Acetone
 Concen: 8.878 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. 0.000 min
 Lab File: VU049782.D
 Acq: 19 Jul 2022 14:05

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ZD0

Tgt Ion: 43 Resp: 10675
 Ion Ratio Lower Upper
 43 100
 58 31.9 0.0 61.4

