

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
 Data File : VU049787.D
 Acq On : 19 Jul 2022 16:04
 Operator : SY/MD
 Sample : N3738-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ZC8

Quant Time: Jul 20 02:17:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 19 02:09:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	175156	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	166630	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	69222	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	74551	50.445	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	100.880%
7) Chloroethane-d5	1.903	69	57792	54.099	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	108.200%
11) 1,1-Dichloroethene-d2	2.562	63	91876	35.195	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.400%
21) 2-Butanone-d5	4.620	46	149574	118.558	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	118.560%
24) Chloroform-d	5.063	84	138054	52.742	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.480%
26) 1,2-Dichloroethane-d4	5.700	65	98503	55.603	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	111.200%
32) Benzene-d6	5.726	84	260744	51.508	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.020%
36) 1,2-Dichloropropane-d6	6.690	67	94034	55.227	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	110.460%
41) Toluene-d8	7.899	98	213559	48.444	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.880%
43) trans-1,3-Dichloroprop...	8.179	79	36796	51.292	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	102.580%
47) 2-Hexanone-d5	8.632	63	77026	100.567	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	100.570%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	126774	53.212	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	106.420%
66) 1,2-Dichlorobenzene-d4	12.192	152	71455	54.749	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	109.500%
Target Compounds						
					Qvalue	
13) Acetone	2.626	43	10711	8.933	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
Data File : VU049787.D
Acq On : 19 Jul 2022 16:04
Operator : SY/MD
Sample : N3738-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ZC8

Quant Time: Jul 20 02:17:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 19 02:09:49 2022
Response via : Initial Calibration

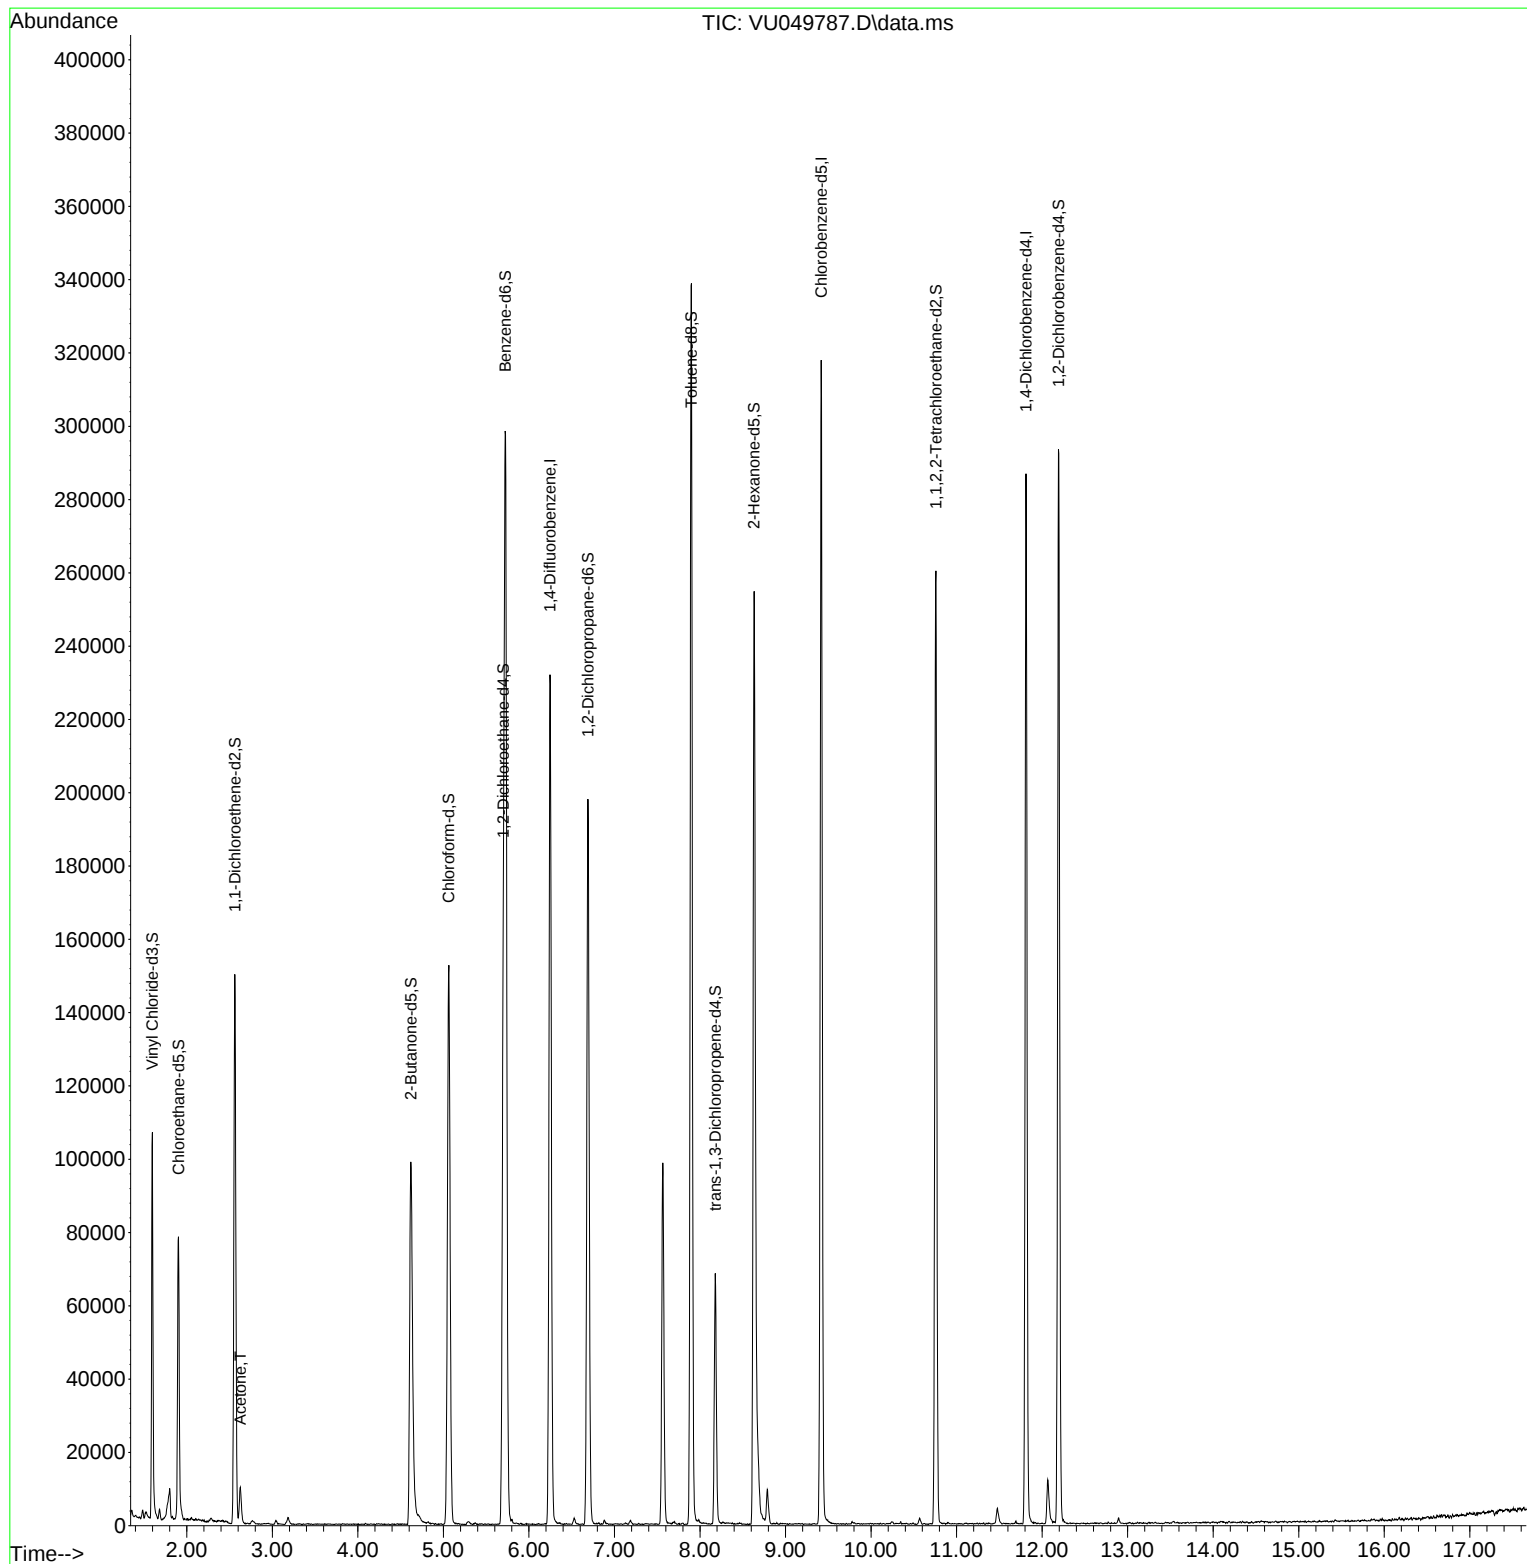

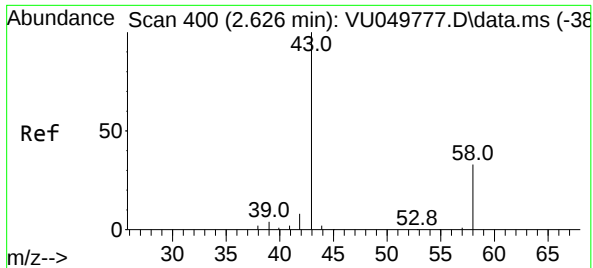

#13
 Acetone
 Concen: 8.933 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. -0.000 min
 Lab File: VU049787.D
 Acq: 19 Jul 2022 16:04

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ZC8

Tgt Ion: 43 Resp: 10711
 Ion Ratio Lower Upper
 43 100
 58 32.5 0.0 61.4

