

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
 Data File : VU049778.D
 Acq On : 19 Jul 2022 12:28
 Operator : SY/MD
 Sample : VU0719MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK160

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049778.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	94	rBV	106651	123021	15.16%	2.071%
2	1.806	126	145	152	rVB5	8668	19041	2.35%	0.321%
3	1.900	166	174	189	rBV	78441	104143	12.83%	1.753%
4	2.494	356	359	363	rBV	262	231	0.03%	0.004%
5	2.562	367	380	394	rBV	154516	247057	30.44%	4.159%
6	2.649	405	407	413	rBV2	262	198	0.02%	0.003%
7	2.719	426	429	431	rBV	233	165	0.02%	0.003%
8	2.784	442	449	462	rVB2	582	950	0.12%	0.016%
9	2.851	466	470	476	rBV2	222	238	0.03%	0.004%
10	2.977	506	509	513	rBV2	266	161	0.02%	0.003%
11	3.041	521	529	541	rVB2	4029	7089	0.87%	0.119%
12	3.179	568	572	573	rBV	392	291	0.04%	0.005%
13	3.260	594	597	603	rBV	241	203	0.03%	0.003%
14	3.356	625	627	634	rBV2	220	199	0.02%	0.003%
15	3.552	686	688	694	rVB2	260	186	0.02%	0.003%
16	3.613	703	707	711	rVB2	226	161	0.02%	0.003%
17	3.700	728	734	736	rBV2	265	337	0.04%	0.006%
18	3.764	749	754	756	rBV2	188	193	0.02%	0.003%
19	3.809	765	768	777	rVB2	194	242	0.03%	0.004%
20	3.871	782	787	790	rBV	195	204	0.03%	0.003%
21	3.980	816	821	824	rBV2	242	259	0.03%	0.004%
22	4.047	839	842	846	rBV2	251	201	0.02%	0.003%
23	4.298	916	920	923	rBV	178	180	0.02%	0.003%
24	4.343	930	934	938	rBV	355	266	0.03%	0.004%
25	4.417	952	957	960	rBV2	230	206	0.03%	0.003%
26	4.462	964	971	975	rBV2	209	279	0.03%	0.005%
27	4.620	1007	1020	1060	rVV	95771	235148	28.97%	3.959%
28	4.883	1100	1102	1105	rVB	446	187	0.02%	0.003%
29	4.980	1129	1132	1135	rBV2	233	167	0.02%	0.003%
30	5.060	1141	1157	1180	rBV	150303	324019	39.92%	5.455%
31	5.269	1219	1222	1224	rBV3	312	198	0.02%	0.003%
32	5.292	1225	1229	1237	rVB3	813	1027	0.13%	0.017%
33	5.382	1255	1257	1262	rVB	349	208	0.03%	0.004%
34	5.446	1274	1277	1280	rVB	256	173	0.02%	0.003%
35	5.510	1294	1297	1300	rBV	228	170	0.02%	0.003%
36	5.723	1341	1363	1388	rBV2	300412	811668	100.00%	13.665%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
 Data File : VU049778.D
 Acq On : 19 Jul 2022 12:28
 Operator : SY/MD
 Sample : VU0719MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK160

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	6.121	1484	1487	1491	rVB2	283	214	0.03%	0.004%
38	6.247	1512	1526	1552	rBV	236439	448786	55.29%	7.556%
39	6.359	1560	1561	1565	rBV2	259	185	0.02%	0.003%
40	6.440	1582	1586	1595	rVB2	244	302	0.04%	0.005%
41	6.530	1604	1614	1621	rVB4	1737	2895	0.36%	0.049%
42	6.690	1650	1664	1684	rBV	197008	379224	46.72%	6.384%
43	7.002	1757	1761	1766	rVV2	141	162	0.02%	0.003%
44	7.070	1777	1782	1784	rBV	178	156	0.02%	0.003%
45	7.186	1814	1818	1825	rVB3	1038	1102	0.14%	0.019%
46	7.269	1841	1844	1849	rVB2	230	198	0.02%	0.003%
47	7.385	1870	1880	1883	rBV	279	355	0.04%	0.006%
48	7.449	1894	1900	1903	rBV2	198	225	0.03%	0.004%
49	7.565	1924	1936	1953	rVV	98796	170606	21.02%	2.872%
50	7.690	1970	1975	1981	rVV4	823	1008	0.12%	0.017%
51	7.793	2004	2007	2010	rBV2	504	399	0.05%	0.007%
52	7.896	2026	2039	2057	rBV	336472	575563	70.91%	9.690%
53	7.986	2066	2067	2072	rVB	388	179	0.02%	0.003%
54	8.076	2093	2095	2099	rVB	351	196	0.02%	0.003%
55	8.179	2115	2127	2142	rBV	67682	110178	13.57%	1.855%
56	8.340	2174	2177	2181	rVB	417	279	0.03%	0.005%
57	8.369	2181	2186	2189	rBV2	279	240	0.03%	0.004%
58	8.391	2189	2193	2198	rVB2	247	254	0.03%	0.004%
59	8.526	2229	2235	2239	rBV	445	452	0.06%	0.008%
60	8.587	2249	2254	2256	rBV2	226	193	0.02%	0.003%
61	8.632	2256	2268	2301	rBV3	242035	476598	58.72%	8.024%
62	8.944	2362	2365	2371	rVB2	249	256	0.03%	0.004%
63	8.980	2372	2376	2378	rBV	215	158	0.02%	0.003%
64	9.089	2408	2410	2417	rVB2	272	301	0.04%	0.005%
65	9.417	2498	2512	2535	rBV	327688	543159	66.92%	9.144%
66	9.571	2553	2560	2564	rVB3	397	426	0.05%	0.007%
67	9.697	2594	2599	2602	rVV2	315	302	0.04%	0.005%
68	9.758	2613	2618	2623	rVB2	265	318	0.04%	0.005%
69	10.050	2706	2709	2712	rBV2	267	256	0.03%	0.004%
70	10.189	2749	2752	2757	rVB2	349	321	0.04%	0.005%
71	10.214	2757	2760	2765	rBV2	246	215	0.03%	0.004%
72	10.298	2783	2786	2792	rBV2	254	289	0.04%	0.005%
73	10.340	2796	2799	2808	rVB2	321	519	0.06%	0.009%
74	10.378	2808	2811	2813	rBV	332	238	0.03%	0.004%
75	10.523	2853	2856	2859	rBV2	228	167	0.02%	0.003%
76	10.587	2873	2876	2879	rBV	257	157	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
 Data File : VU049778.D
 Acq On : 19 Jul 2022 12:28
 Operator : SY/MD
 Sample : VU0719MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK160

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	10.610	2879	2883	2884	rBV	268	184	0.02%	0.003%
78	10.755	2916	2928	2950	rVV	259634	415874	51.24%	7.002%
79	11.092	3028	3033	3035	rBV2	433	364	0.04%	0.006%
80	11.176	3055	3059	3062	rBV2	154	174	0.02%	0.003%
81	11.211	3066	3070	3074	rVV2	224	171	0.02%	0.003%
82	11.462	3145	3148	3150	rBV	327	223	0.03%	0.004%
83	11.500	3155	3160	3163	rVB	479	387	0.05%	0.007%
84	11.549	3171	3175	3179	rBV2	221	249	0.03%	0.004%
85	11.745	3230	3236	3239	rBV4	372	381	0.05%	0.006%
86	11.812	3245	3257	3274	rBV	281538	447723	55.16%	7.538%
87	12.082	3338	3341	3343	rBV	231	156	0.02%	0.003%
88	12.131	3353	3356	3361	rBV2	295	328	0.04%	0.006%
89	12.192	3363	3375	3398	rVV	286730	458048	56.43%	7.712%
90	12.433	3447	3450	3453	rBV	266	170	0.02%	0.003%
91	12.455	3453	3457	3465	rVB2	319	361	0.04%	0.006%
92	12.777	3554	3557	3563	rBV	274	315	0.04%	0.005%
93	13.221	3691	3695	3696	rBV	635	451	0.06%	0.008%
94	13.542	3791	3795	3797	rBV	318	247	0.03%	0.004%
95	13.844	3882	3889	3900	rBV5	2309	3492	0.43%	0.059%
96	13.973	3925	3929	3932	rVB3	376	317	0.04%	0.005%
97	14.092	3958	3966	3980	rVB	5281	9049	1.11%	0.152%
98	14.240	4009	4012	4014	rBV2	271	198	0.02%	0.003%
99	14.336	4034	4042	4053	rVB5	3286	5031	0.62%	0.085%
100	15.610	4435	4438	4439	rBV	378	188	0.02%	0.003%




Sum of corrected areas: 5939778

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
Data File : VU049778.D
Acq On : 19 Jul 2022 12:28
Operator : SY/MD
Sample : VU0719MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK160

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

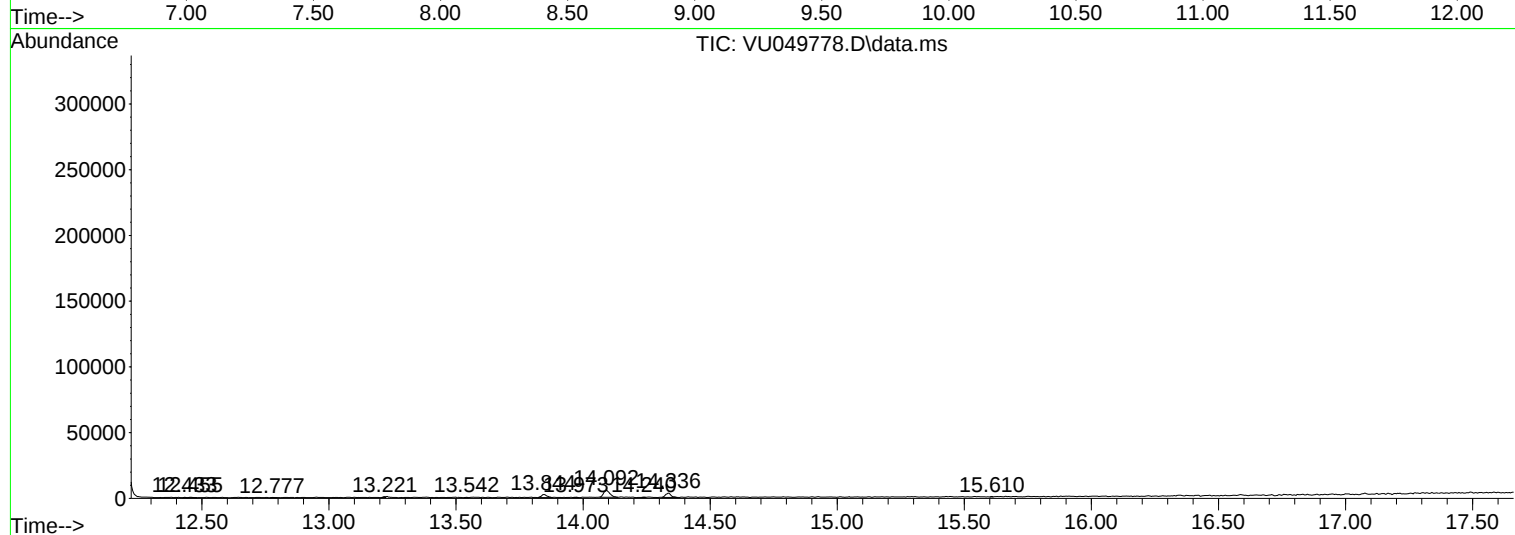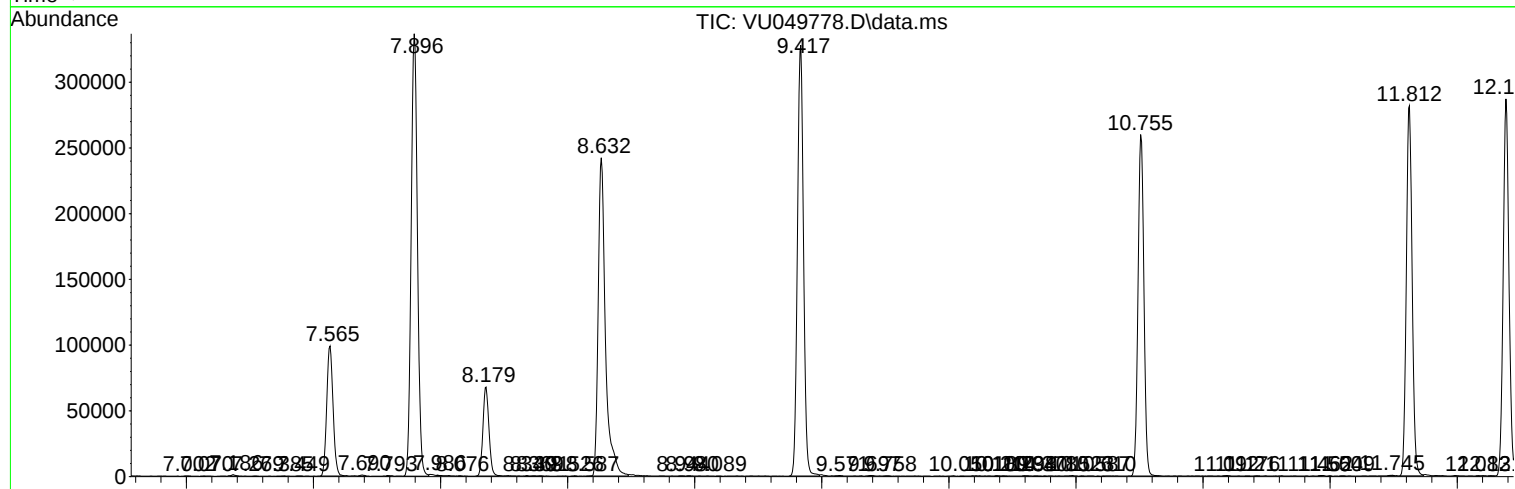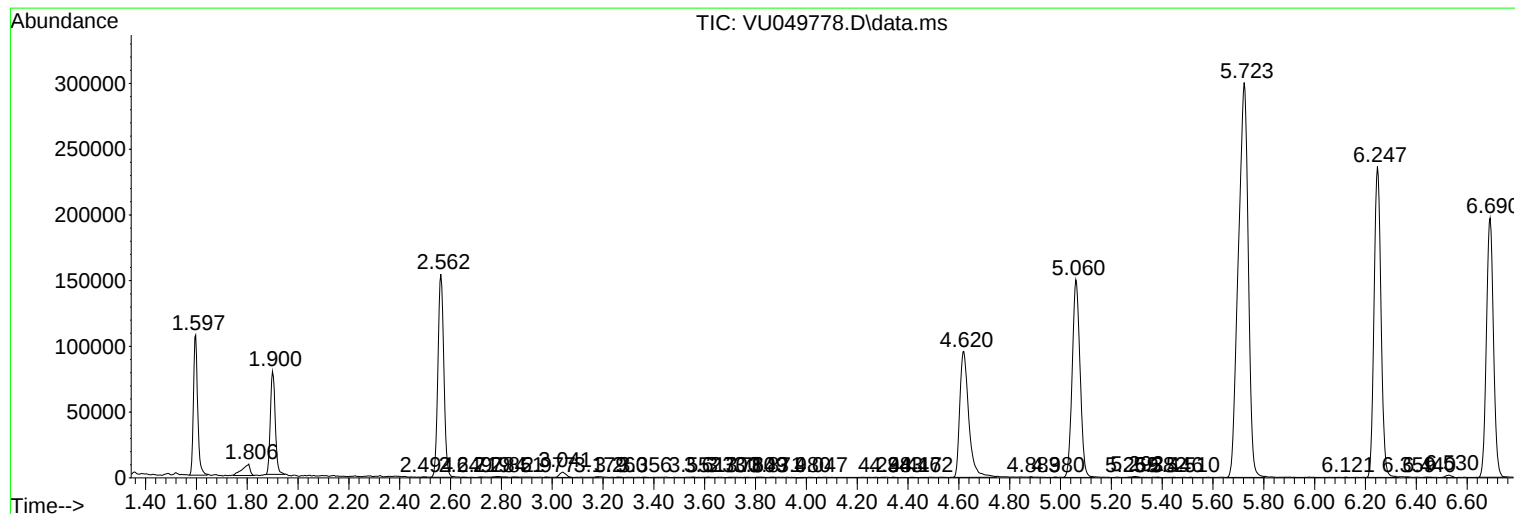

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
Data File : VU049778.D
Acq On : 19 Jul 2022 12:28
Operator : SY/MD
Sample : VU0719MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK160

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
Data File : VU049778.D
Acq On : 19 Jul 2022 12:28
Operator : SY/MD
Sample : VU0719MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK160

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------