

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
 Data File : VU049779.D
 Acq On : 19 Jul 2022 12:54
 Operator : SY/MD
 Sample : VU0719WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK161

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049779.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.359	3	6	11	rVB2	2024	1629	0.21%	0.028%
2	1.597	72	80	98	rVB	103278	118405	15.13%	2.041%
3	1.793	127	141	147	rBV6	6462	10514	1.34%	0.181%
4	1.906	167	176	193	rVB	76295	102220	13.06%	1.762%
5	2.269	287	289	293	rVB2	515	370	0.05%	0.006%
6	2.565	368	381	398	rBV	147239	238713	30.51%	4.115%
7	2.671	410	414	422	rVB2	283	321	0.04%	0.006%
8	2.710	422	426	430	rBV2	189	194	0.02%	0.003%
9	2.787	446	450	454	rVV	649	609	0.08%	0.010%
10	2.845	465	468	471	rBV	241	185	0.02%	0.003%
11	2.870	471	476	481	rVV2	222	306	0.04%	0.005%
12	3.044	520	530	540	rBV4	4382	8145	1.04%	0.140%
13	3.186	563	574	584	rVB	2054	3801	0.49%	0.066%
14	3.250	590	594	598	rVB2	278	271	0.03%	0.005%
15	3.272	598	601	604	rBV2	295	277	0.04%	0.005%
16	3.346	620	624	627	rBV	271	233	0.03%	0.004%
17	3.575	692	695	699	rBV2	261	273	0.03%	0.005%
18	3.742	745	747	751	rVB	311	216	0.03%	0.004%
19	3.768	751	755	758	rBV2	273	246	0.03%	0.004%
20	3.793	759	763	765	rBV2	221	161	0.02%	0.003%
21	3.870	785	787	791	rVB	310	217	0.03%	0.004%
22	3.944	808	810	813	rVB2	260	147	0.02%	0.003%
23	3.967	813	817	819	rBV	179	160	0.02%	0.003%
24	4.102	855	859	861	rBV	228	195	0.02%	0.003%
25	4.147	868	873	877	rBV2	177	216	0.03%	0.004%
26	4.224	893	897	899	rBV2	231	182	0.02%	0.003%
27	4.308	920	923	926	rBV	204	156	0.02%	0.003%
28	4.398	944	951	954	rBV	299	349	0.04%	0.006%
29	4.443	960	965	968	rBV	183	206	0.03%	0.004%
30	4.620	1007	1020	1049	rBV	91335	223108	28.51%	3.846%
31	4.893	1102	1105	1110	rVB2	293	260	0.03%	0.004%
32	5.063	1137	1158	1181	rBV	141754	310647	39.70%	5.355%
33	5.285	1218	1227	1229	rBV3	562	611	0.08%	0.011%
34	5.382	1254	1257	1260	rVV3	335	246	0.03%	0.004%
35	5.401	1260	1263	1269	rVB2	176	143	0.02%	0.002%
36	5.507	1290	1296	1298	rBV2	186	184	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
 Data File : VU049779.D
 Acq On : 19 Jul 2022 12:54
 Operator : SY/MD
 Sample : VU0719WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK161

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	5.578	1311	1318	1322	rBV2	305	501	0.06%	0.009%
38	5.722	1342	1363	1394	rBV2	284578	782490	100.00%	13.488%
39	5.902	1415	1419	1423	rBV	434	528	0.07%	0.009%
40	5.960	1432	1437	1442	rBV2	167	201	0.03%	0.003%
41	6.060	1464	1468	1472	rVB2	207	203	0.03%	0.003%
42	6.247	1513	1526	1547	rBV	228173	433681	55.42%	7.476%
43	6.356	1557	1560	1565	rBV2	284	241	0.03%	0.004%
44	6.501	1602	1605	1608	rBV	218	160	0.02%	0.003%
45	6.529	1608	1614	1622	rVB5	1728	2614	0.33%	0.045%
46	6.568	1622	1626	1629	rBV2	241	213	0.03%	0.004%
47	6.690	1647	1664	1685	rBV	188422	366491	46.84%	6.317%
48	7.060	1774	1779	1783	rBV2	236	217	0.03%	0.004%
49	7.185	1814	1818	1821	rBV3	804	629	0.08%	0.011%
50	7.401	1882	1885	1889	rVB	281	169	0.02%	0.003%
51	7.436	1893	1896	1900	rBV	269	226	0.03%	0.004%
52	7.478	1906	1909	1920	rVB	312	448	0.06%	0.008%
53	7.565	1924	1936	1951	rBV	96992	166958	21.34%	2.878%
54	7.787	2003	2005	2006	rBV	338	147	0.02%	0.003%
55	7.841	2018	2022	2025	rBV2	263	208	0.03%	0.004%
56	7.896	2025	2039	2058	rBV	321866	559543	71.51%	9.645%
57	8.063	2089	2091	2095	rVB2	329	189	0.02%	0.003%
58	8.082	2095	2097	2104	rBV3	270	203	0.03%	0.003%
59	8.179	2116	2127	2142	rBV	65093	107880	13.79%	1.860%
60	8.308	2161	2167	2172	rBV2	423	468	0.06%	0.008%
61	8.443	2207	2209	2217	rVB2	195	210	0.03%	0.004%
62	8.526	2230	2235	2238	rBV2	230	219	0.03%	0.004%
63	8.632	2255	2268	2302	rBV2	228459	460811	58.89%	7.943%
64	8.870	2335	2342	2345	rBV2	442	544	0.07%	0.009%
65	9.118	2414	2419	2421	rBV	155	160	0.02%	0.003%
66	9.182	2436	2439	2443	rBV2	194	144	0.02%	0.002%
67	9.417	2499	2512	2533	rBV	323160	531323	67.90%	9.159%
68	9.648	2581	2584	2587	rVB	302	179	0.02%	0.003%
69	9.674	2587	2592	2594	rBV2	200	211	0.03%	0.004%
70	9.719	2602	2606	2611	rBV2	207	209	0.03%	0.004%
71	9.828	2637	2640	2644	rBV2	178	157	0.02%	0.003%
72	9.857	2648	2649	2655	rBV2	193	154	0.02%	0.003%
73	9.909	2662	2665	2669	rVB	292	186	0.02%	0.003%
74	9.989	2686	2690	2693	rBV2	273	293	0.04%	0.005%
75	10.243	2763	2769	2772	rBV2	221	208	0.03%	0.004%
76	10.269	2774	2777	2781	rVB2	237	174	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
 Data File : VU049779.D
 Acq On : 19 Jul 2022 12:54
 Operator : SY/MD
 Sample : VU0719WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK161

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	10.700	2908	2911	2914	rVB	329	220	0.03%	0.004%
78	10.754	2914	2928	2949	rBV	245596	405478	51.82%	6.989%
79	10.934	2980	2984	2988	rBV2	195	214	0.03%	0.004%
80	11.005	3003	3006	3010	rBV	228	200	0.03%	0.003%
81	11.211	3067	3070	3074	rBV2	308	212	0.03%	0.004%
82	11.471	3148	3151	3156	rVB2	370	407	0.05%	0.007%
83	11.500	3156	3160	3166	rBV2	170	207	0.03%	0.004%
84	11.664	3208	3211	3212	rBV	224	146	0.02%	0.003%
85	11.745	3233	3236	3237	rBV	293	174	0.02%	0.003%
86	11.812	3244	3257	3275	rBV	289097	467432	59.74%	8.057%
87	12.060	3331	3334	3337	rBV2	233	167	0.02%	0.003%
88	12.192	3363	3375	3391	rBV	296754	475588	60.78%	8.198%
89	12.703	3531	3534	3538	rBV	254	222	0.03%	0.004%
90	12.725	3538	3541	3544	rVB	309	205	0.03%	0.004%
91	12.983	3619	3621	3626	rVB2	307	209	0.03%	0.004%
92	13.085	3646	3653	3656	rBV2	299	399	0.05%	0.007%
93	13.214	3690	3693	3697	rBV3	377	304	0.04%	0.005%
94	13.680	3835	3838	3841	rBV	236	183	0.02%	0.003%
95	13.889	3901	3903	3906	rBV	405	162	0.02%	0.003%
96	14.092	3960	3966	3974	rBV3	1755	2735	0.35%	0.047%
97	14.330	4037	4040	4049	rVB3	1204	1362	0.17%	0.023%
98	14.677	4144	4148	4151	rBV2	310	335	0.04%	0.006%
99	14.925	4223	4225	4227	rBV	340	231	0.03%	0.004%
100	16.217	4624	4627	4631	rBV2	718	636	0.08%	0.011%




Sum of corrected areas: 5801334

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
Data File : VU049779.D
Acq On : 19 Jul 2022 12:54
Operator : SY/MD
Sample : VU0719WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK161

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

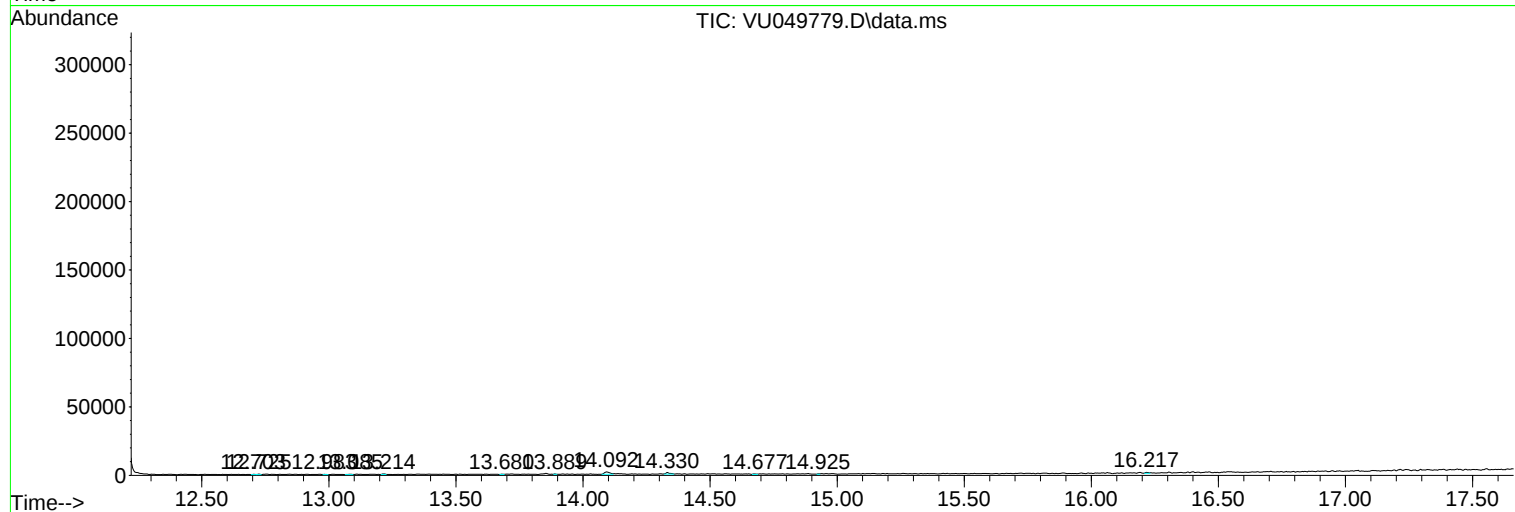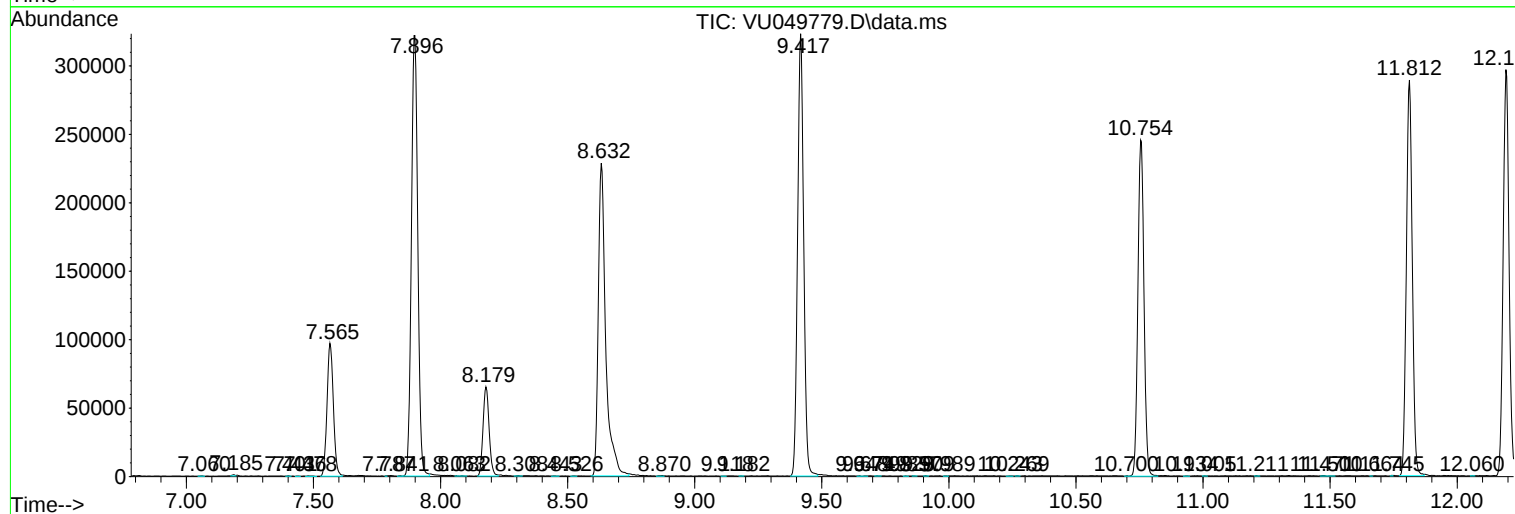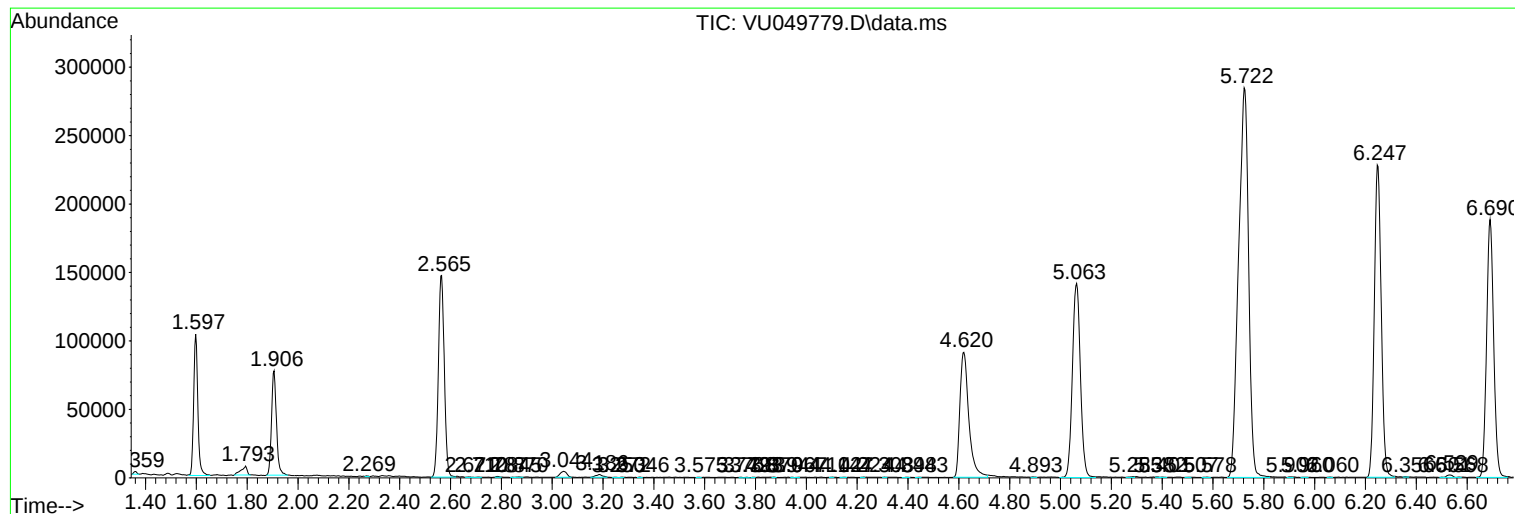

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
Data File : VU049779.D
Acq On : 19 Jul 2022 12:54
Operator : SY/MD
Sample : VU0719WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK161

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
Data File : VU049779.D
Acq On : 19 Jul 2022 12:54
Operator : SY/MD
Sample : VU0719WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK161

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc