

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
 Data File : VU049786.D
 Acq On : 19 Jul 2022 15:40
 Operator : SY/MD
 Sample : N3748-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049786.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	50	rVB3	2105	2384	0.30%	0.040%
2	1.517	51	55	59	rBV	2333	2417	0.30%	0.041%
3	1.597	72	80	97	rBV	104226	121450	15.13%	2.049%
4	1.899	165	174	184	rBV	77231	102155	12.73%	1.724%
5	2.256	282	285	286	rBV2	514	263	0.03%	0.004%
6	2.395	324	328	333	rBV2	524	632	0.08%	0.011%
7	2.446	342	344	351	rVB4	798	648	0.08%	0.011%
8	2.562	368	380	397	rBV	152534	245802	30.63%	4.148%
9	2.758	437	441	446	rBV2	294	214	0.03%	0.004%
10	2.790	446	451	462	rVB2	307	398	0.05%	0.007%
11	2.899	483	485	488	rVB2	304	165	0.02%	0.003%
12	2.922	489	492	498	rBV2	174	164	0.02%	0.003%
13	2.951	498	501	507	rBV2	137	167	0.02%	0.003%
14	3.041	519	529	541	rVB3	5138	9105	1.13%	0.154%
15	3.179	568	572	575	rBV2	436	408	0.05%	0.007%
16	3.446	652	655	658	rBV	205	165	0.02%	0.003%
17	3.542	679	685	692	rBV2	155	244	0.03%	0.004%
18	3.822	768	772	776	rBV2	201	160	0.02%	0.003%
19	4.173	877	881	887	rBB2	165	192	0.02%	0.003%
20	4.272	907	912	915	rBV2	209	214	0.03%	0.004%
21	4.330	926	930	934	rVV2	184	206	0.03%	0.003%
22	4.526	988	991	995	rVB2	192	146	0.02%	0.002%
23	4.562	1000	1002	1005	rVB	235	147	0.02%	0.002%
24	4.620	1007	1020	1049	rBV	97001	232136	28.93%	3.917%
25	4.767	1064	1066	1071	rVB3	381	236	0.03%	0.004%
26	4.841	1084	1089	1091	rBV	317	261	0.03%	0.004%
27	4.886	1100	1103	1105	rBV2	210	147	0.02%	0.002%
28	4.960	1123	1126	1131	rVB3	256	253	0.03%	0.004%
29	5.063	1139	1158	1178	rBV	146835	319330	39.79%	5.388%
30	5.276	1219	1224	1225	rBV2	452	336	0.04%	0.006%
31	5.353	1244	1248	1251	rBV2	208	201	0.03%	0.003%
32	5.465	1277	1283	1286	rBV2	173	196	0.02%	0.003%
33	5.722	1342	1363	1385	rBV3	296273	802491	100.00%	13.541%
34	6.057	1464	1467	1470	rVV2	296	192	0.02%	0.003%
35	6.102	1474	1481	1484	rVB2	239	269	0.03%	0.005%
36	6.124	1484	1488	1492	rBV2	288	252	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
 Data File : VU049786.D
 Acq On : 19 Jul 2022 15:40
 Operator : SY/MD
 Sample : N3748-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	6.247	1511	1526	1548	rBV	244909	461426	57.50%	7.786%
38	6.456	1588	1591	1594	rVB2	300	172	0.02%	0.003%
39	6.523	1606	1612	1614	rBV4	1398	1581	0.20%	0.027%
40	6.690	1650	1664	1682	rBV2	196365	376110	46.87%	6.347%
41	6.800	1693	1698	1700	rBV3	288	283	0.04%	0.005%
42	6.816	1700	1703	1707	rVB3	435	286	0.04%	0.005%
43	6.874	1716	1721	1728	rBV2	343	540	0.07%	0.009%
44	7.185	1805	1818	1825	rBV5	1143	1916	0.24%	0.032%
45	7.218	1825	1828	1833	rVB2	189	171	0.02%	0.003%
46	7.369	1872	1875	1884	rVB2	232	344	0.04%	0.006%
47	7.407	1884	1887	1891	rBV2	150	153	0.02%	0.003%
48	7.430	1891	1894	1898	rVB2	228	148	0.02%	0.002%
49	7.468	1902	1906	1912	rBV2	263	281	0.04%	0.005%
50	7.565	1923	1936	1953	rBV	96025	167937	20.93%	2.834%
51	7.690	1966	1975	1977	rBV2	789	1067	0.13%	0.018%
52	7.896	2026	2039	2056	rBV	328953	565365	70.45%	9.540%
53	8.115	2103	2107	2111	rBV2	214	184	0.02%	0.003%
54	8.179	2116	2127	2140	rBV	66641	109423	13.64%	1.846%
55	8.398	2192	2195	2201	rBV2	293	341	0.04%	0.006%
56	8.632	2256	2268	2301	rBV2	251920	488667	60.89%	8.246%
57	8.845	2332	2334	2337	rVB2	332	190	0.02%	0.003%
58	9.115	2414	2418	2421	rBV2	181	170	0.02%	0.003%
59	9.163	2430	2433	2436	rVB	323	234	0.03%	0.004%
60	9.185	2436	2440	2446	rBV2	332	447	0.06%	0.008%
61	9.356	2486	2493	2495	rBV	244	302	0.04%	0.005%
62	9.417	2499	2512	2531	rBV	332684	549736	68.50%	9.276%
63	9.568	2556	2559	2564	rVB3	237	170	0.02%	0.003%
64	9.616	2571	2574	2577	rBV2	205	156	0.02%	0.003%
65	9.632	2577	2579	2583	rVB	267	168	0.02%	0.003%
66	9.658	2583	2587	2590	rBV2	162	154	0.02%	0.003%
67	9.816	2633	2636	2642	rBV2	184	205	0.03%	0.003%
68	9.938	2669	2674	2681	rBV2	365	613	0.08%	0.010%
69	10.076	2710	2717	2723	rBV	384	632	0.08%	0.011%
70	10.224	2756	2763	2766	rBV2	296	348	0.04%	0.006%
71	10.362	2803	2806	2810	rVB2	272	206	0.03%	0.003%
72	10.754	2916	2928	2944	rBV	252863	408434	50.90%	6.892%
73	10.825	2948	2950	2953	rVB2	520	279	0.03%	0.005%
74	10.848	2953	2957	2962	rBV	387	482	0.06%	0.008%
75	10.873	2963	2965	2971	rVB	261	190	0.02%	0.003%
76	10.915	2975	2978	2982	rVB	205	147	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
 Data File : VU049786.D
 Acq On : 19 Jul 2022 15:40
 Operator : SY/MD
 Sample : N3748-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	11.140	3045	3048	3053	rBV2	194	170	0.02%	0.003%
78	11.192	3060	3064	3066	rBV2	311	243	0.03%	0.004%
79	11.269	3085	3088	3095	rVB2	361	353	0.04%	0.006%
80	11.404	3127	3130	3137	rVB2	197	201	0.03%	0.003%
81	11.529	3165	3169	3173	rBV2	227	237	0.03%	0.004%
82	11.812	3242	3257	3275	rBV	295682	473962	59.06%	7.998%
83	12.192	3363	3375	3391	rBV	287878	461841	57.55%	7.793%
84	12.410	3440	3443	3446	rVV	310	193	0.02%	0.003%
85	12.510	3471	3474	3478	rVB	257	171	0.02%	0.003%
86	12.552	3484	3487	3492	rVB	276	234	0.03%	0.004%
87	12.584	3493	3497	3499	rBV2	268	187	0.02%	0.003%
88	12.658	3517	3520	3523	rBV	236	189	0.02%	0.003%
89	12.931	3602	3605	3611	rBV2	343	358	0.04%	0.006%
90	13.198	3685	3688	3696	rVB2	334	348	0.04%	0.006%
91	13.278	3710	3713	3718	rVB	377	270	0.03%	0.005%
92	13.304	3718	3721	3723	rBV2	242	167	0.02%	0.003%
93	13.536	3790	3793	3799	rBV3	356	391	0.05%	0.007%
94	13.757	3859	3862	3864	rBV2	297	174	0.02%	0.003%
95	13.803	3873	3876	3878	rBV2	282	208	0.03%	0.004%
96	14.047	3949	3952	3954	rBV	477	315	0.04%	0.005%
97	14.230	4006	4009	4013	rBV	349	388	0.05%	0.007%
98	14.671	4143	4146	4150	rBV3	371	313	0.04%	0.005%
99	15.005	4247	4250	4254	rBV2	463	509	0.06%	0.009%
100	16.185	4612	4617	4619	rBV3	986	992	0.12%	0.017%




Sum of corrected areas: 5926218

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
Data File : VU049786.D
Acq On : 19 Jul 2022 15:40
Operator : SY/MD
Sample : N3748-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

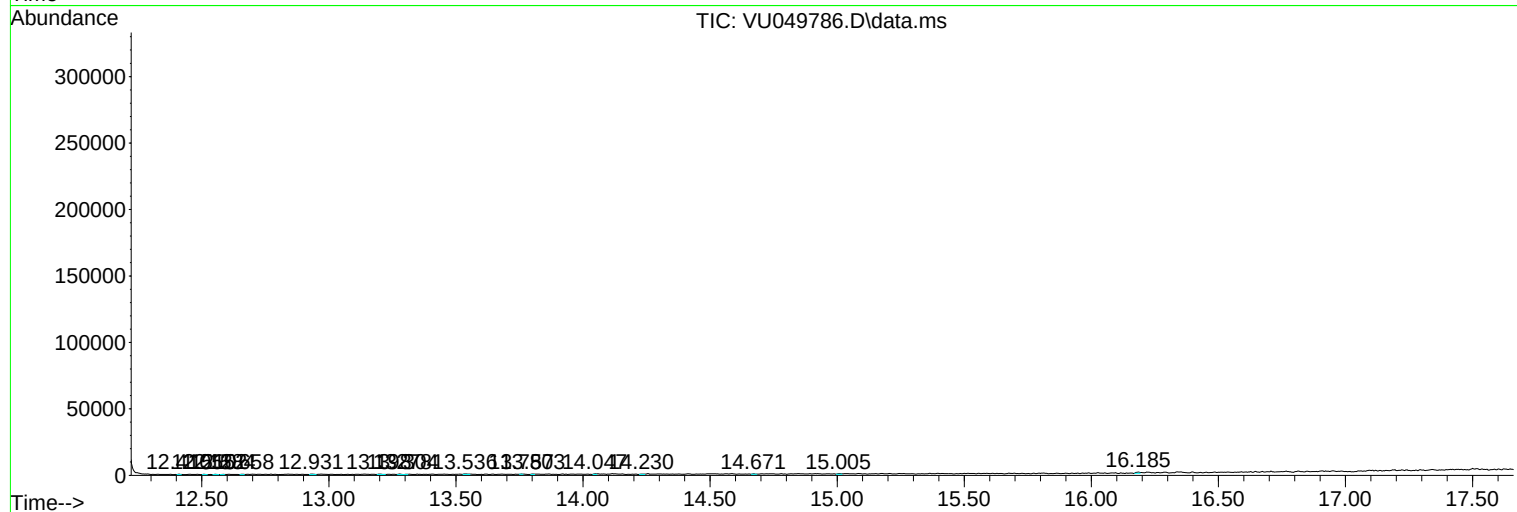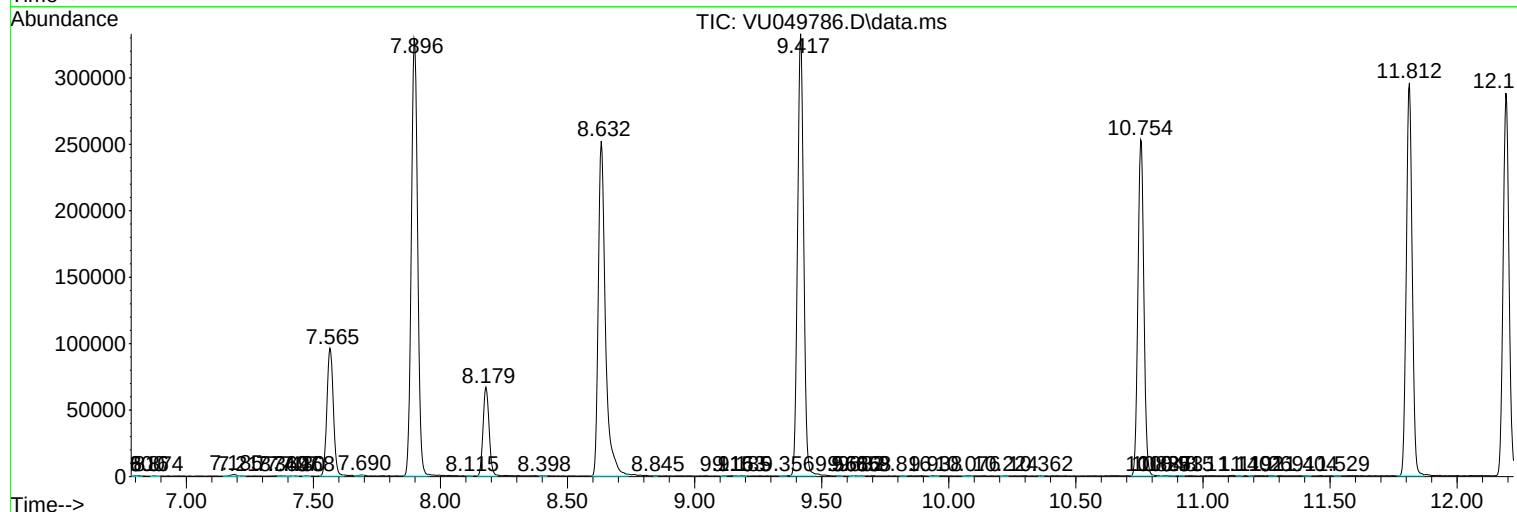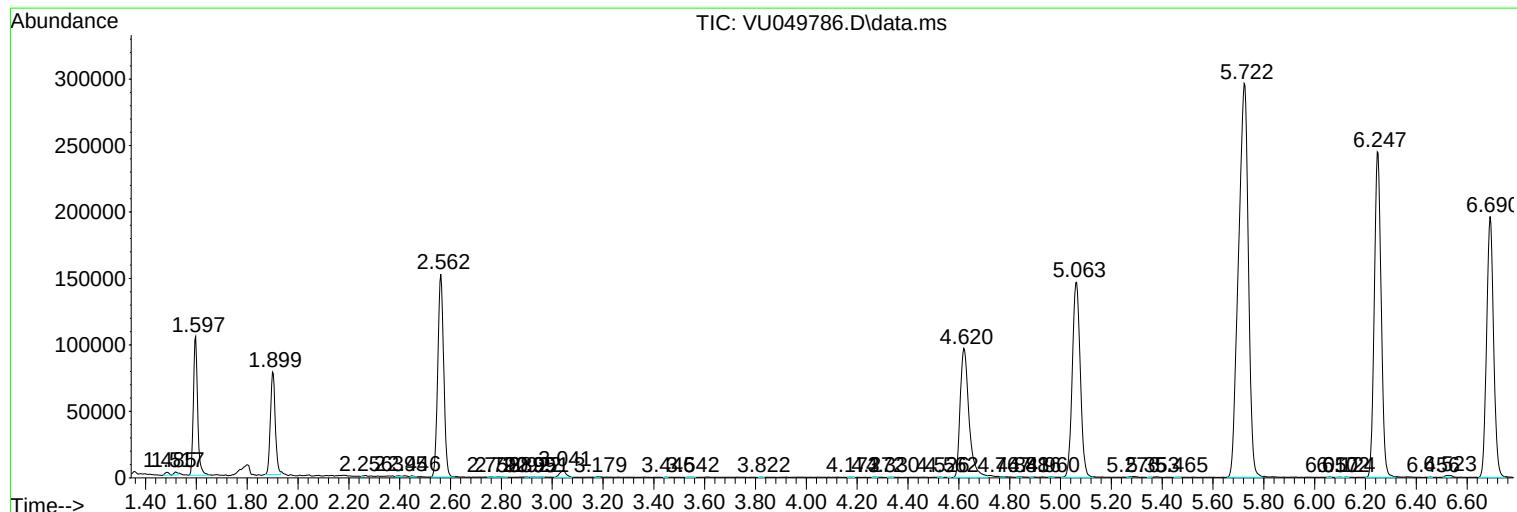

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
Data File : VU049786.D
Acq On : 19 Jul 2022 15:40
Operator : SY/MD
Sample : N3748-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
Data File : VU049786.D
Acq On : 19 Jul 2022 15:40
Operator : SY/MD
Sample : N3748-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------