


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071922\
Data File : VU049776.D
Acq On : 19 Jul 2022 11:08
Operator : SY/MD
Sample : BFB107
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB107

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Title : VOC Analysis
Last Update : Wed Jul 20 04:27:32 2022

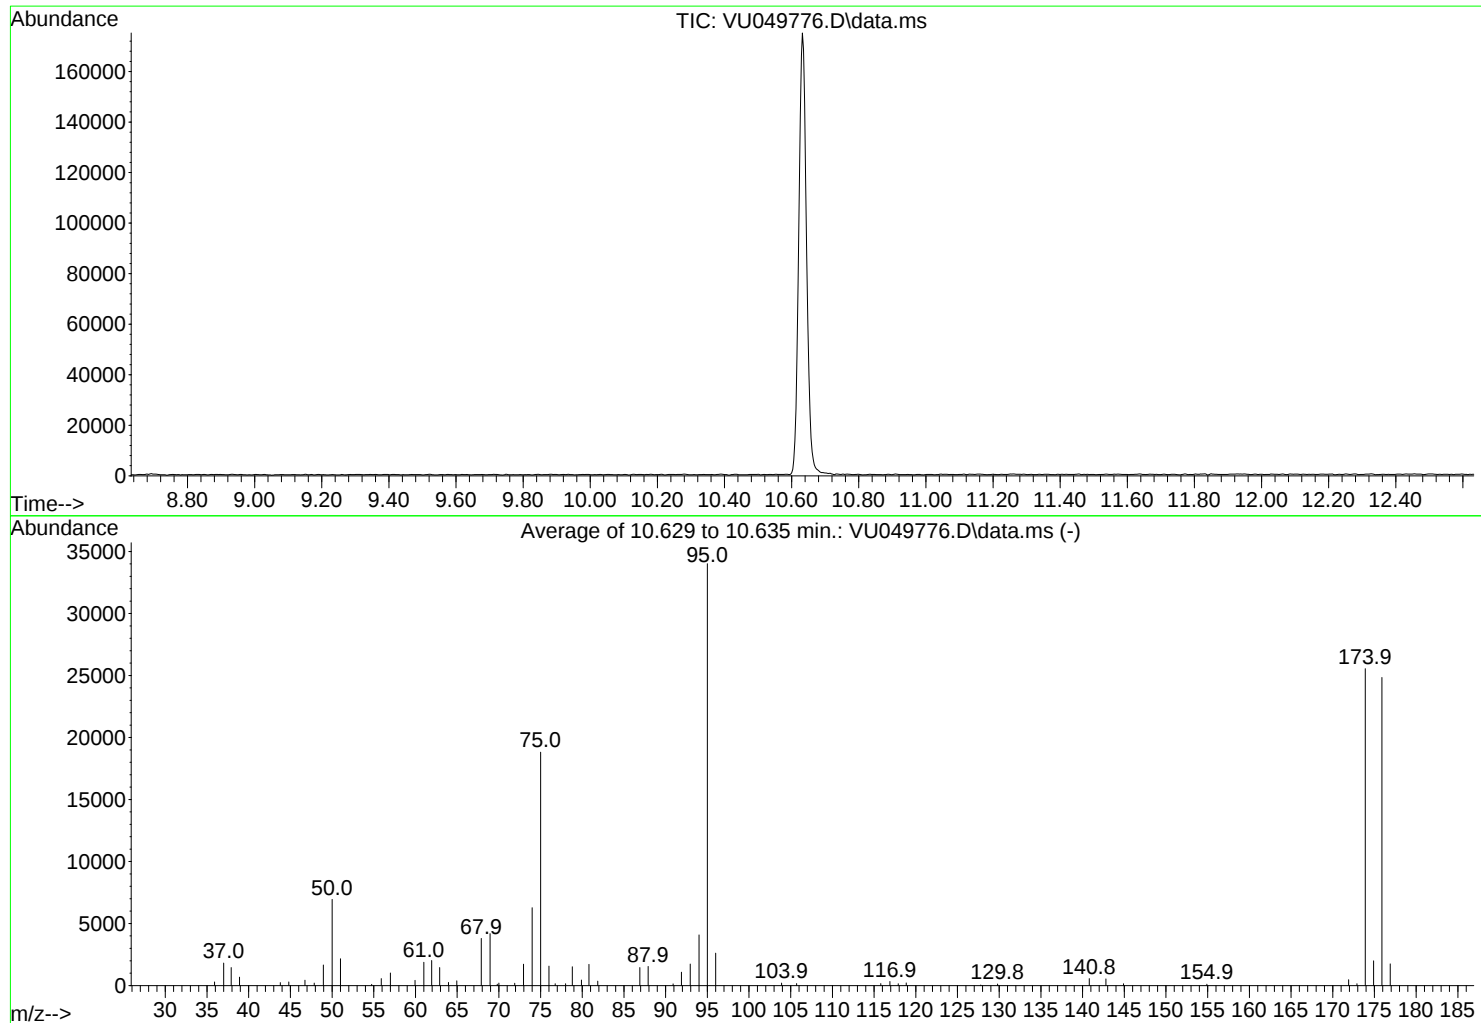

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	6955	PASS
75	95	30	80	55.3	18824	PASS
95	95	100	100	100.0	34011	PASS
96	95	5	9	7.7	2615	PASS
173	174	0.00	2	0.6	147	PASS
174	95	50	120	75.1	25557	PASS
175	174	5	9	7.8	1990	PASS
176	174	95	101	97.2	24840	PASS
177	176	5	9	7.0	1747	PASS

m/z	Abundance
39.90	210.0
43.80	339.0

Instrument :
MSVOA_U
ClientSampleId :
BFB107

m/z	Abundance
35.90	322.0
37.00	1912.0
37.90	1461.0
38.90	642.0
43.80	526.0
44.80	343.0
46.80	491.0
47.90	174.0
48.90	1615.0
50.00	7110.0
51.00	2213.0
54.80	100.0
55.90	550.0
57.00	918.0
60.00	493.0
61.00	1937.0
62.00	1965.0
62.90	1356.0
63.90	226.0
64.90	382.0
67.90	3746.0
69.00	4217.0
69.80	325.0
71.90	185.0
72.90	1794.0
74.00	6235.0
75.00	18504.0
76.00	1602.0
76.70	147.0
77.90	166.0
78.80	1482.0
79.90	463.0
80.80	1611.0
81.90	349.0
86.90	1222.0
87.90	1547.0
90.90	143.0
91.90	1112.0
92.90	1677.0
94.00	3970.0
95.00	32968.0
96.00	2619.0
103.80	211.0
105.70	170.0
115.80	123.0
116.80	346.0
117.90	144.0
118.80	224.0
129.80	142.0
140.80	488.0
142.80	543.0
144.90	184.0
154.90	120.0
171.90	454.0
172.90	442.0
173.90	24416.0
174.90	2028.0
175.90	23704.0
176.90	1651.0

Instrument :
MSVOA_U
ClientSampleId :
BFB107

m/z	Abundance
35.90	282.0
37.00	1856.0
37.90	1501.0
38.90	706.0
39.70	117.0
43.90	571.0
44.80	293.0
46.70	445.0
47.80	214.0
48.90	1693.0
50.00	7217.0
51.00	2265.0
54.80	105.0
55.90	602.0
57.00	1028.0
60.00	415.0
61.00	1909.0
61.90	2079.0
62.90	1488.0
64.00	259.0
64.90	392.0
67.90	3890.0
68.90	4324.0
70.00	302.0
71.90	183.0
72.90	1775.0
74.00	6442.0
75.00	19352.0
76.00	1595.0
76.80	151.0
78.00	157.0
78.80	1572.0
79.90	452.0
80.80	1798.0
81.90	356.0
86.90	1521.0
87.90	1583.0
90.90	139.0
91.90	1114.0
92.90	1814.0
94.00	4193.0
95.00	34952.0
96.00	2743.0
103.90	199.0
105.70	163.0
115.80	174.0
116.90	340.0
117.90	149.0
118.80	218.0
129.80	137.0
140.80	585.0
142.80	565.0
144.90	149.0
154.90	115.0
171.90	512.0
173.90	26432.0
174.90	2086.0
175.90	25720.0
176.90	1842.0

Instrument :
MSVOA_U
ClientSampleId :
BFB107

m/z	Abundance
35.90	265.0
37.00	1660.0
37.90	1383.0
38.90	680.0
39.70	162.0
43.90	627.0
44.80	243.0
46.70	365.0
47.90	230.0
49.00	1667.0
50.00	6537.0
51.00	2014.0
54.70	103.0
55.90	546.0
57.00	1082.0
59.90	344.0
61.00	1808.0
61.90	2019.0
62.90	1512.0
64.00	252.0
65.00	375.0
67.90	3767.0
68.90	4014.0
70.00	284.0
71.90	188.0
73.00	1611.0
74.00	6172.0
75.00	18616.0
76.00	1492.0
76.80	139.0
78.10	132.0
78.80	1493.0
79.90	425.0
80.80	1704.0
81.80	355.0
86.90	1618.0
87.90	1484.0
90.90	136.0
91.90	1013.0
93.00	1732.0
94.00	4106.0
95.00	34112.0
96.00	2483.0
104.00	171.0
105.70	149.0
115.80	203.0
117.00	288.0
117.90	154.0
118.90	214.0
127.80	120.0
129.80	106.0
140.80	601.0
142.80	491.0
144.90	130.0
154.90	104.0
171.90	461.0
173.90	25824.0
174.90	1857.0
175.90	25096.0
176.90	1748.0

Instrument :
MSVOA_U
ClientSampleId :
BFB107