

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071923\
 Data File : VU054816.D
 Acq On : 19 Jul 2023 13:20
 Operator : MD/SY
 Sample : VU0719WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK101

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
 Title : VOC Analysis

Signal : TIC: VU054816.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	112	rBV	93028	123567	15.06%	1.806%
2	2.557	383	394	409	rBV	146047	236054	28.77%	3.451%
3	3.332	632	635	638	rBV2	764	597	0.07%	0.009%
4	3.422	660	663	666	rBV2	645	454	0.06%	0.007%
5	3.640	728	731	734	rBV2	529	427	0.05%	0.006%
6	3.679	739	743	745	rBV2	663	479	0.06%	0.007%
7	3.978	834	836	839	rBV2	412	302	0.04%	0.004%
8	4.068	859	864	869	rVB6	765	721	0.09%	0.011%
9	4.222	908	912	918	rBV3	653	726	0.09%	0.011%
10	4.332	943	946	950	rVB4	587	354	0.04%	0.005%
11	4.361	953	955	959	rVB2	386	230	0.03%	0.003%
12	4.402	965	968	971	rBV4	527	453	0.06%	0.007%
13	4.476	987	991	992	rBV2	437	294	0.04%	0.004%
14	4.502	996	999	1000	rBV	380	274	0.03%	0.004%
15	4.615	1024	1034	1065	rBV2	82174	198084	24.14%	2.896%
16	5.055	1157	1171	1189	rBV	150726	333064	40.59%	4.869%
17	5.380	1270	1272	1276	rBB3	488	239	0.03%	0.003%
18	5.438	1286	1290	1291	rBV3	609	385	0.05%	0.006%
19	5.480	1301	1303	1307	rVB2	646	341	0.04%	0.005%
20	5.541	1318	1322	1325	rVB3	452	285	0.03%	0.004%
21	5.579	1331	1334	1338	rBV3	532	366	0.04%	0.005%
22	5.605	1338	1342	1346	rBV3	542	528	0.06%	0.008%
23	5.718	1357	1377	1397	rBV3	297240	820583	100.00%	11.995%
24	5.939	1444	1446	1455	rBV5	672	847	0.10%	0.012%
25	6.017	1464	1470	1473	rBV4	518	554	0.07%	0.008%
26	6.042	1476	1478	1481	rVB3	526	262	0.03%	0.004%
27	6.113	1497	1500	1504	rBV3	455	275	0.03%	0.004%
28	6.168	1514	1517	1522	rVB3	420	300	0.04%	0.004%
29	6.245	1527	1541	1562	rBV	296133	563740	68.70%	8.241%
30	6.451	1602	1605	1608	rBV	530	330	0.04%	0.005%
31	6.483	1613	1615	1618	rBV2	514	289	0.04%	0.004%
32	6.589	1642	1648	1650	rBV4	698	670	0.08%	0.010%
33	6.685	1664	1678	1698	rBV	201175	395080	48.15%	5.775%
34	6.885	1736	1740	1744	rVB3	941	786	0.10%	0.011%
35	6.952	1759	1761	1764	rBV3	584	265	0.03%	0.004%
36	6.975	1765	1768	1769	rBV2	521	212	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071923\
 Data File : VU054816.D
 Acq On : 19 Jul 2023 13:20
 Operator : MD/SY
 Sample : VU0719WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK101

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
 Title : VOC Analysis

37	7.017	1777	1781	1783	rBV2	524	409	0.05%	0.006%
38	7.071	1793	1798	1803	rBV5	427	470	0.06%	0.007%
39	7.264	1857	1858	1861	rVB2	667	193	0.02%	0.003%
40	7.306	1868	1871	1876	rVB3	650	387	0.05%	0.006%
41	7.338	1876	1881	1885	rBV4	463	552	0.07%	0.008%
42	7.370	1888	1891	1893	rBV2	339	238	0.03%	0.003%
43	7.415	1904	1905	1910	rVB2	655	406	0.05%	0.006%
44	7.447	1912	1915	1918	rBV3	587	437	0.05%	0.006%
45	7.499	1927	1931	1936	rBV4	922	706	0.09%	0.010%
46	7.563	1939	1951	1971	rBV2	114485	204877	24.97%	2.995%
47	7.746	2006	2008	2010	rBV3	579	240	0.03%	0.004%
48	7.894	2041	2054	2076	rBV	383702	663085	80.81%	9.693%
49	8.058	2101	2105	2106	rBV2	452	280	0.03%	0.004%
50	8.177	2128	2142	2164	rBV	80719	137703	16.78%	2.013%
51	8.386	2203	2207	2208	rBV	582	433	0.05%	0.006%
52	8.557	2257	2260	2263	rVB2	696	429	0.05%	0.006%
53	8.631	2271	2283	2319	rBV2	240138	459091	55.95%	6.711%
54	8.827	2342	2344	2345	rBV2	464	211	0.03%	0.003%
55	8.901	2364	2367	2370	rBV3	612	491	0.06%	0.007%
56	8.978	2387	2391	2397	rBV3	509	468	0.06%	0.007%
57	9.004	2397	2399	2402	rBV2	537	356	0.04%	0.005%
58	9.045	2410	2412	2417	rBV3	543	419	0.05%	0.006%
59	9.129	2435	2438	2439	rBV2	415	222	0.03%	0.003%
60	9.267	2479	2481	2484	rBV2	420	282	0.03%	0.004%
61	9.415	2514	2527	2548	rBV	425256	707860	86.26%	10.347%
62	9.743	2626	2629	2631	rBV2	535	280	0.03%	0.004%
63	9.881	2670	2672	2675	rBV2	399	255	0.03%	0.004%
64	9.955	2693	2695	2697	rBV	421	208	0.03%	0.003%
65	10.004	2708	2710	2713	rBV2	364	202	0.02%	0.003%
66	10.023	2713	2716	2720	rBV3	493	490	0.06%	0.007%
67	10.106	2737	2742	2743	rBV3	976	701	0.09%	0.010%
68	10.225	2774	2779	2782	rBV4	500	476	0.06%	0.007%
69	10.296	2799	2801	2807	rVB4	651	473	0.06%	0.007%
70	10.489	2855	2861	2862	rBV	935	852	0.10%	0.012%
71	10.608	2895	2898	2902	rVB2	489	361	0.04%	0.005%
72	10.631	2902	2905	2908	rBV2	701	546	0.07%	0.008%
73	10.685	2919	2922	2925	rVB2	597	346	0.04%	0.005%
74	10.753	2930	2943	2961	rBV	330798	530511	64.65%	7.755%
75	10.859	2973	2976	2979	rBV3	585	509	0.06%	0.007%
76	11.026	3026	3028	3031	rVB2	530	290	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071923\
 Data File : VU054816.D
 Acq On : 19 Jul 2023 13:20
 Operator : MD/SY
 Sample : VU0719WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK101

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
 Title : VOC Analysis

77	11.042	3031	3033	3034	rBV2	505	269	0.03%	0.004%
78	11.090	3046	3048	3049	rBV2	658	252	0.03%	0.004%
79	11.319	3117	3119	3123	rBV4	475	357	0.04%	0.005%
80	11.434	3151	3155	3160	rBV2	669	682	0.08%	0.010%
81	11.463	3160	3164	3165	rBV2	915	690	0.08%	0.010%
82	11.653	3216	3223	3226	rBV4	623	705	0.09%	0.010%
83	11.711	3238	3241	3242	rBV2	686	440	0.05%	0.006%
84	11.807	3260	3271	3291	rBV	463124	751789	91.62%	10.989%
85	12.061	3348	3350	3356	rBV2	534	606	0.07%	0.009%
86	12.100	3356	3362	3364	rVV3	875	849	0.10%	0.012%
87	12.145	3373	3376	3377	rBV2	507	253	0.03%	0.004%
88	12.190	3378	3390	3408	rVV	414160	678115	82.64%	9.912%
89	12.431	3463	3465	3467	rBV2	645	408	0.05%	0.006%
90	12.553	3498	3503	3507	rBV4	758	817	0.10%	0.012%
91	12.585	3512	3513	3516	rBV	410	235	0.03%	0.003%
92	12.711	3549	3552	3554	rBV2	544	364	0.04%	0.005%
93	12.862	3597	3599	3606	rVB3	775	525	0.06%	0.008%
94	12.994	3638	3640	3643	rVV3	523	276	0.03%	0.004%
95	13.219	3706	3710	3712	rBV	1125	929	0.11%	0.014%
96	13.454	3781	3783	3790	rVB4	855	707	0.09%	0.010%
97	13.489	3791	3794	3796	rBV2	434	285	0.03%	0.004%
98	14.007	3953	3955	3959	rBV2	687	566	0.07%	0.008%
99	15.306	4354	4359	4363	rBV4	1192	1318	0.16%	0.019%
100	15.476	4410	4412	4413	rBV2	854	477	0.06%	0.007%




Sum of corrected areas: 6841076

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071923\
Data File : VU054816.D
Acq On : 19 Jul 2023 13:20
Operator : MD/SY
Sample : VU0719WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK101

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

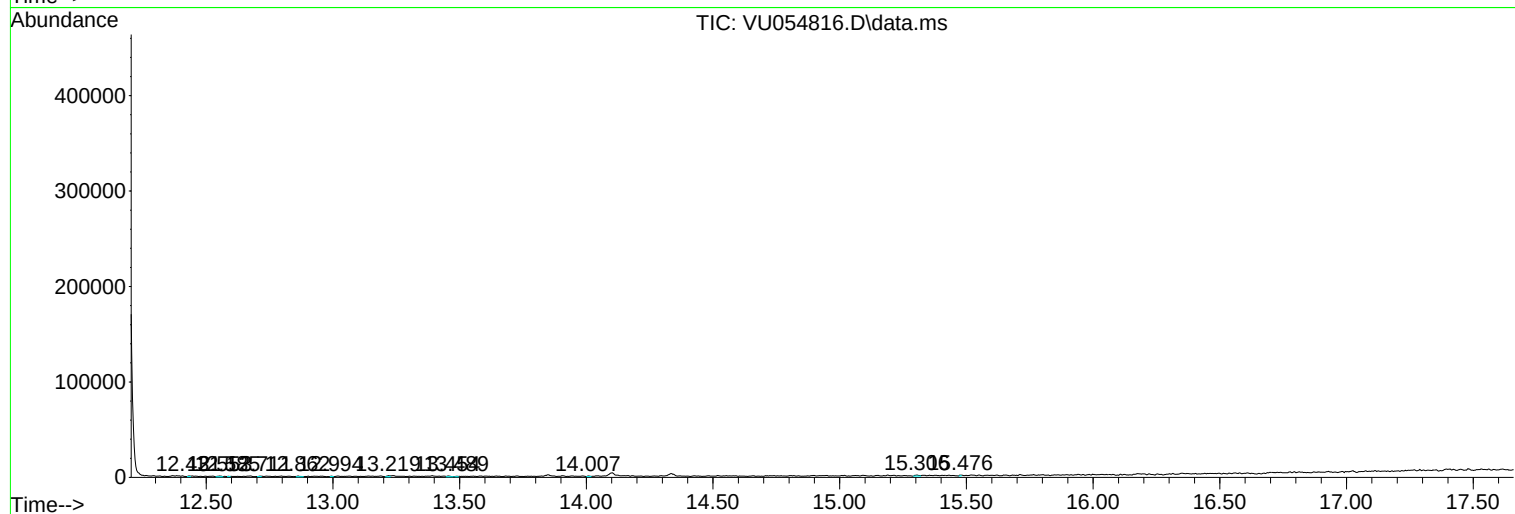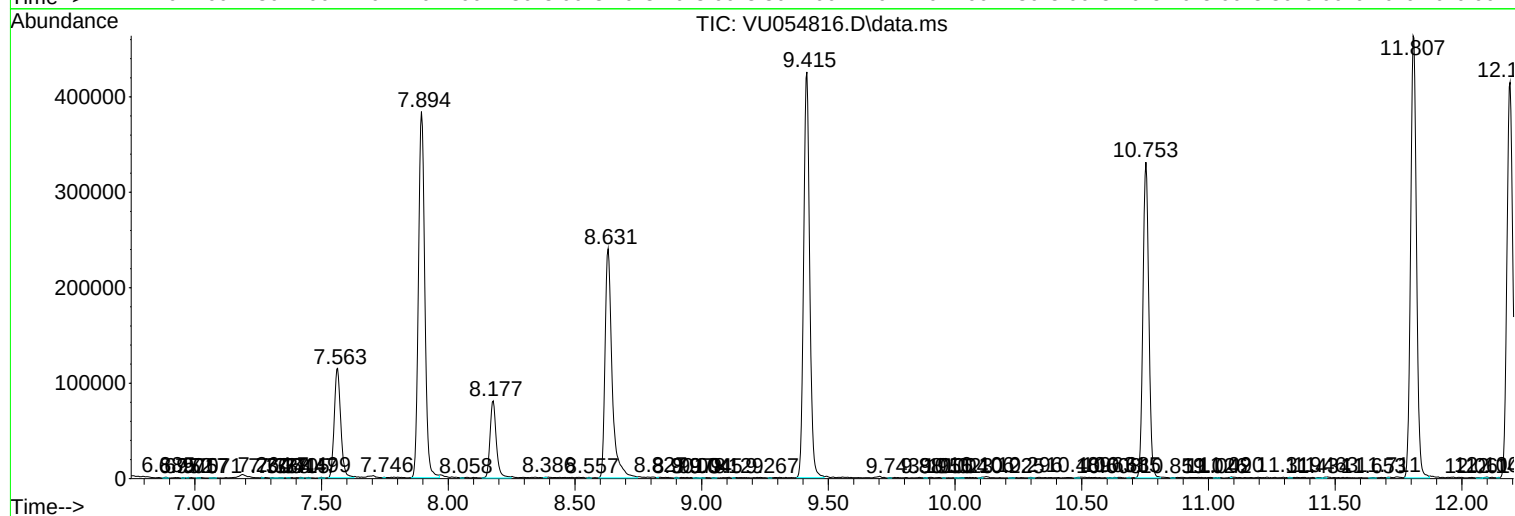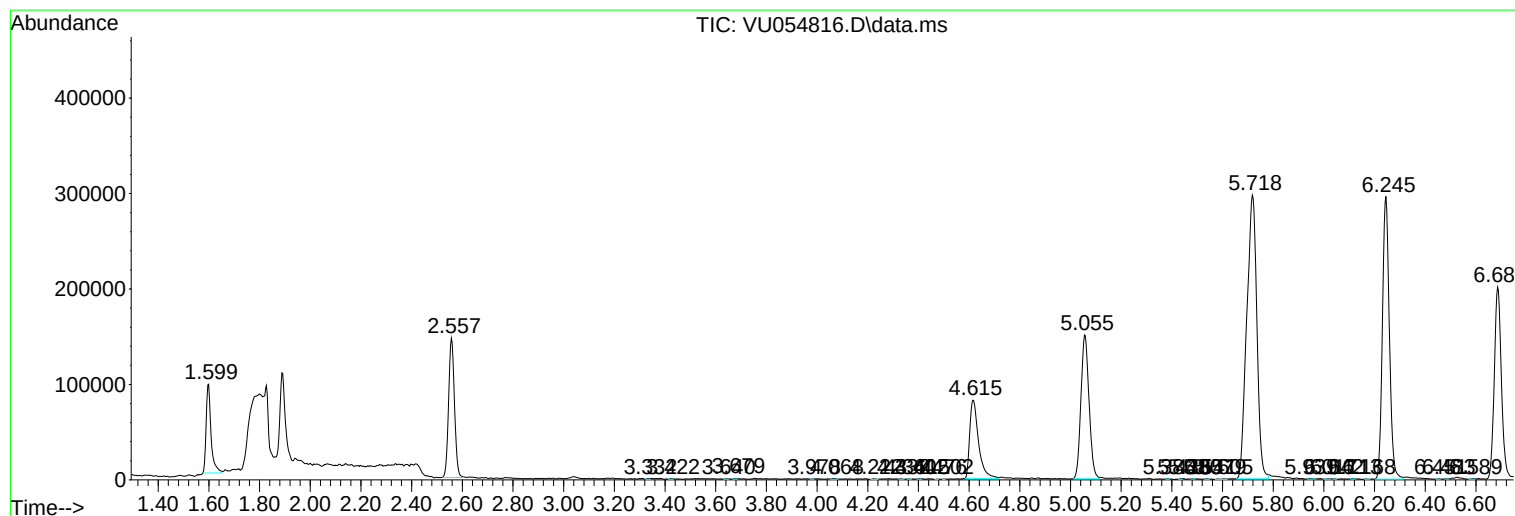

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071923\
Data File : VU054816.D
Acq On : 19 Jul 2023 13:20
Operator : MD/SY
Sample : VU0719WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK101

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071923\
Data File : VU054816.D
Acq On : 19 Jul 2023 13:20
Operator : MD/SY
Sample : VU0719WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK101

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------