

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071923\
 Data File : VU054818.D
 Acq On : 19 Jul 2023 14:14
 Operator : MD/SY
 Sample : 03656-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH2X1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
 Title : VOC Analysis

Signal : TIC: VU054818.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	108	rBV	87522	115138	15.09%	1.614%
2	2.557	383	394	410	rVB	132240	216154	28.32%	3.029%
3	2.753	453	455	456	rBV2	681	219	0.03%	0.003%
4	3.132	571	573	576	rVB2	625	331	0.04%	0.005%
5	3.181	576	588	598	rBV3	4806	11438	1.50%	0.160%
6	3.341	629	638	639	rBV5	2120	2046	0.27%	0.029%
7	3.444	667	670	671	rBV2	500	330	0.04%	0.005%
8	3.673	739	741	743	rBV	361	206	0.03%	0.003%
9	3.808	780	783	785	rBV2	505	325	0.04%	0.005%
10	3.820	785	787	789	rVV2	536	247	0.03%	0.003%
11	3.904	811	813	818	rBV2	606	381	0.05%	0.005%
12	3.962	829	831	834	rVB2	430	246	0.03%	0.003%
13	3.978	834	836	838	rBV	334	220	0.03%	0.003%
14	4.052	857	859	862	rBV2	558	309	0.04%	0.004%
15	4.084	866	869	873	rVV2	286	220	0.03%	0.003%
16	4.277	926	929	931	rBV3	410	271	0.04%	0.004%
17	4.290	931	933	937	rVV3	555	321	0.04%	0.004%
18	4.515	1001	1003	1006	rBV3	321	190	0.02%	0.003%
19	4.557	1014	1016	1019	rBV	404	263	0.03%	0.004%
20	4.618	1022	1035	1045	rBV	77739	199313	26.11%	2.793%
21	5.055	1156	1171	1193	rBV	139744	314194	41.17%	4.403%
22	5.290	1241	1244	1249	rVB2	632	638	0.08%	0.009%
23	5.319	1249	1253	1256	rBV3	336	325	0.04%	0.005%
24	5.434	1285	1289	1290	rBV	405	274	0.04%	0.004%
25	5.467	1295	1299	1301	rVV	479	347	0.05%	0.005%
26	5.480	1301	1303	1305	rVB	587	241	0.03%	0.003%
27	5.496	1305	1308	1310	rBV2	639	340	0.04%	0.005%
28	5.566	1326	1330	1332	rBV2	881	571	0.07%	0.008%
29	5.605	1336	1342	1344	rBV	556	532	0.07%	0.007%
30	5.717	1354	1377	1401	rBV3	274504	755739	99.02%	10.591%
31	6.039	1474	1477	1481	rBV4	802	580	0.08%	0.008%
32	6.058	1481	1483	1486	rVB2	699	354	0.05%	0.005%
33	6.164	1513	1516	1518	rBV	490	321	0.04%	0.004%
34	6.245	1526	1541	1558	rBV	294514	562891	73.75%	7.888%
35	6.422	1594	1596	1600	rBV2	436	390	0.05%	0.005%
36	6.505	1617	1622	1623	rBV2	801	651	0.09%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071923\
 Data File : VU054818.D
 Acq On : 19 Jul 2023 14:14
 Operator : MD/SY
 Sample : 03656-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH2X1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
 Title : VOC Analysis

37	6.537	1623	1632	1647	rBV7	16919	36133	4.73%	0.506%
38	6.685	1665	1678	1696	rBV	183345	354860	46.49%	4.973%
39	7.004	1774	1777	1778	rBV	426	264	0.03%	0.004%
40	7.039	1785	1788	1791	rBV3	447	269	0.04%	0.004%
41	7.084	1798	1802	1805	rBV2	576	422	0.06%	0.006%
42	7.190	1818	1835	1840	rBV6	4090	8577	1.12%	0.120%
43	7.264	1856	1858	1861	rVB2	531	228	0.03%	0.003%
44	7.303	1868	1870	1871	rBV2	545	262	0.03%	0.004%
45	7.351	1883	1885	1890	rBV4	473	333	0.04%	0.005%
46	7.422	1905	1907	1908	rBV	382	181	0.02%	0.003%
47	7.505	1931	1933	1936	rVB	387	241	0.03%	0.003%
48	7.563	1936	1951	1970	rBV2	105466	192678	25.24%	2.700%
49	7.698	1986	1993	1997	rBV6	1800	2422	0.32%	0.034%
50	7.894	2041	2054	2077	rBV	353098	616037	80.71%	8.633%
51	8.177	2130	2142	2155	rBV2	73347	123454	16.17%	1.730%
52	8.328	2186	2189	2194	rBV4	805	742	0.10%	0.010%
53	8.547	2245	2257	2273	rBV	287417	494164	64.74%	6.925%
54	8.630	2273	2283	2313	rVB2	237889	447622	58.65%	6.273%
55	8.836	2345	2347	2349	rVB2	657	251	0.03%	0.004%
56	8.859	2349	2354	2357	rBV5	778	804	0.11%	0.011%
57	8.923	2372	2374	2379	rBV2	649	638	0.08%	0.009%
58	9.068	2417	2419	2424	rVB2	539	407	0.05%	0.006%
59	9.139	2438	2441	2445	rBV2	510	366	0.05%	0.005%
60	9.370	2510	2513	2514	rBV	372	220	0.03%	0.003%
61	9.412	2514	2526	2552	rVV	418785	711244	93.19%	9.967%
62	9.566	2571	2574	2585	rVB3	1009	1342	0.18%	0.019%
63	9.637	2593	2596	2599	rBV4	742	374	0.05%	0.005%
64	9.659	2602	2603	2607	rVV	428	275	0.04%	0.004%
65	9.704	2607	2617	2624	rVV5	1397	2892	0.38%	0.041%
66	9.817	2648	2652	2654	rBV3	324	286	0.04%	0.004%
67	9.881	2669	2672	2676	rVB3	573	414	0.05%	0.006%
68	9.901	2676	2678	2681	rBV2	454	281	0.04%	0.004%
69	9.952	2690	2694	2697	rBV2	293	260	0.03%	0.004%
70	10.077	2729	2733	2736	rBV3	690	491	0.06%	0.007%
71	10.322	2806	2809	2811	rBV2	439	283	0.04%	0.004%
72	10.476	2853	2857	2863	rBV4	739	1055	0.14%	0.015%
73	10.563	2880	2884	2887	rBV2	514	373	0.05%	0.005%
74	10.624	2899	2903	2904	rBV	422	252	0.03%	0.004%
75	10.708	2925	2929	2930	rBV2	408	280	0.04%	0.004%
76	10.753	2931	2943	2963	rVV	328335	527522	69.12%	7.393%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071923\
 Data File : VU054818.D
 Acq On : 19 Jul 2023 14:14
 Operator : MD/SY
 Sample : 03656-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH2X1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
 Title : VOC Analysis

77	10.881	2979	2983	2984	rBV	348	207	0.03%	0.003%
78	10.933	2997	2999	3002	rBV	438	305	0.04%	0.004%
79	11.016	3020	3025	3029	rBV5	603	523	0.07%	0.007%
80	11.039	3030	3032	3034	rBV	411	201	0.03%	0.003%
81	11.093	3045	3049	3052	rBV4	813	649	0.09%	0.009%
82	11.167	3070	3072	3077	rVB	784	615	0.08%	0.009%
83	11.193	3077	3080	3082	rBV2	614	403	0.05%	0.006%
84	11.209	3082	3085	3090	rVB2	464	327	0.04%	0.005%
85	11.235	3090	3093	3095	rBV2	615	328	0.04%	0.005%
86	11.460	3158	3163	3166	rBV2	929	990	0.13%	0.014%
87	11.531	3183	3185	3189	rBV2	418	362	0.05%	0.005%
88	11.666	3226	3227	3230	rBV	309	201	0.03%	0.003%
89	11.753	3252	3254	3258	rVB3	963	612	0.08%	0.009%
90	11.807	3258	3271	3299	rBV	478575	763251	100.00%	10.696%
91	12.042	3339	3344	3345	rBV2	578	491	0.06%	0.007%
92	12.190	3377	3390	3410	rBV	390859	642913	84.23%	9.010%
93	12.511	3486	3490	3492	rBV	493	317	0.04%	0.004%
94	12.659	3535	3536	3540	rVB	421	259	0.03%	0.004%
95	12.778	3569	3573	3576	rBV2	611	443	0.06%	0.006%
96	12.990	3636	3639	3644	rBV3	612	624	0.08%	0.009%
97	13.048	3653	3657	3665	rBV3	766	924	0.12%	0.013%
98	13.617	3829	3834	3838	rBV4	996	895	0.12%	0.013%
99	13.852	3902	3907	3909	rBV4	1369	1430	0.19%	0.020%
100	14.103	3980	3985	3997	rBV7	1528	2652	0.35%	0.037%




Sum of corrected areas: 7135677

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071923\
Data File : VU054818.D
Acq On : 19 Jul 2023 14:14
Operator : MD/SY
Sample : 03656-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH2X1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

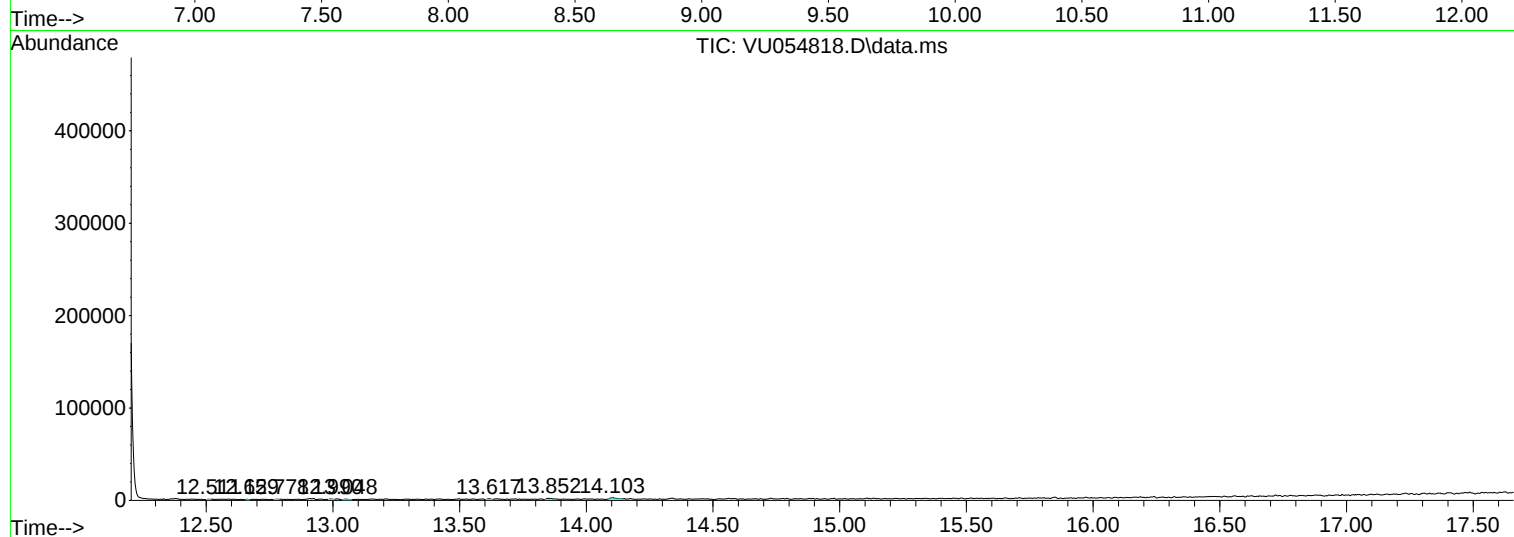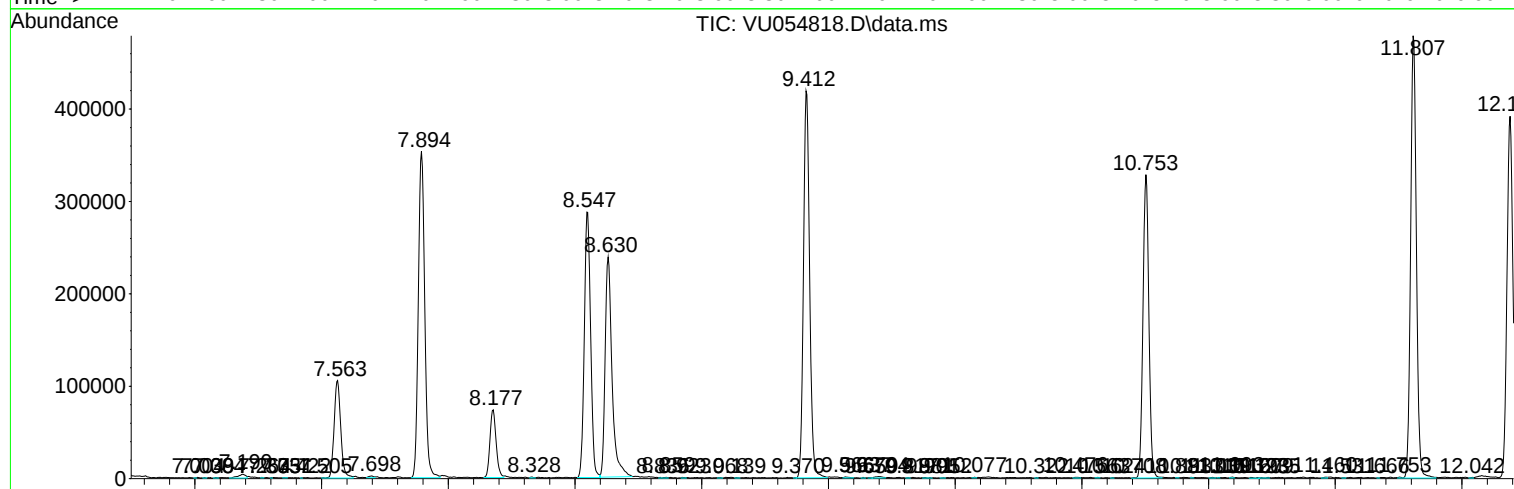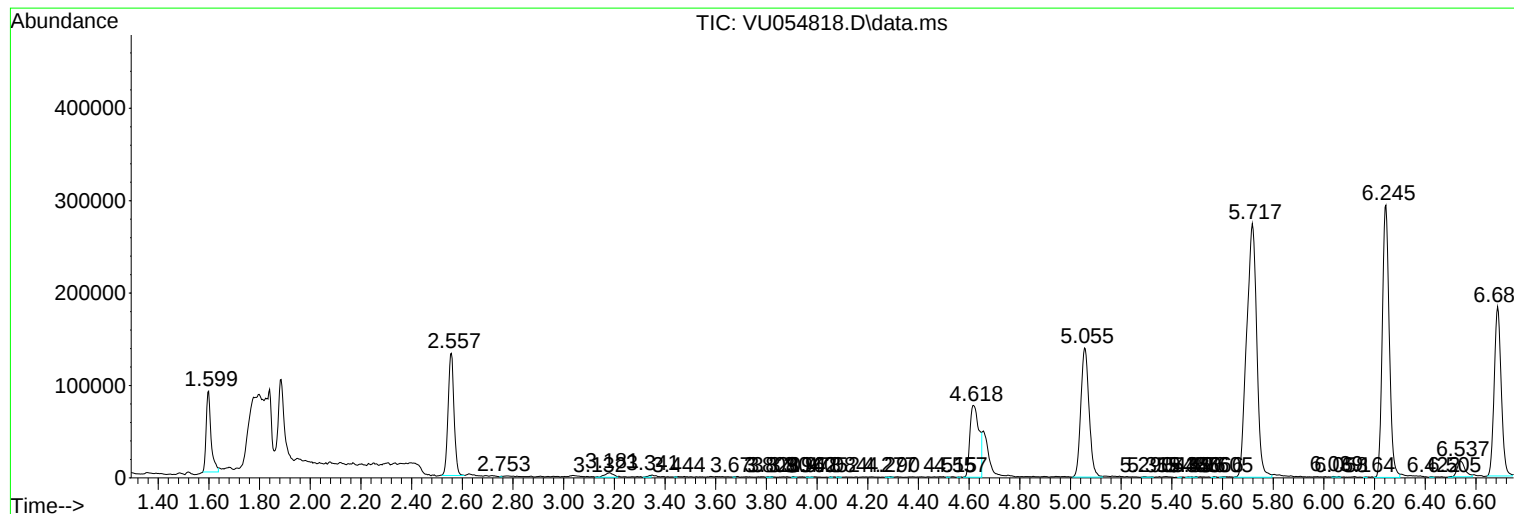

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071923\
Data File : VU054818.D
Acq On : 19 Jul 2023 14:14
Operator : MD/SY
Sample : 03656-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH2X1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071923\
Data File : VU054818.D
Acq On : 19 Jul 2023 14:14
Operator : MD/SY
Sample : 03656-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH2X1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------