

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071923\
 Data File : VU054823.D
 Acq On : 19 Jul 2023 16:34
 Operator : MD/SY
 Sample : VIBLK102
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK102

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
 Title : VOC Analysis

Signal : TIC: VU054823.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.975	522	524	527	rBV	581	299	0.07%	0.009%
2	3.020	535	538	539	rBV	540	344	0.08%	0.010%
3	3.525	694	695	697	rVB	196	54	0.01%	0.002%
4	3.647	728	733	735	rBV	422	271	0.06%	0.008%
5	3.660	735	737	739	rBV	196	89	0.02%	0.003%
6	3.772	768	772	773	rBV2	452	304	0.07%	0.009%
7	3.988	835	839	842	rBV	331	295	0.07%	0.009%
8	4.132	883	884	886	rVB	377	102	0.02%	0.003%
9	4.203	903	906	909	rBV	445	416	0.10%	0.012%
10	4.235	914	916	917	rBV	289	142	0.03%	0.004%
11	4.264	923	925	930	rVB2	424	285	0.07%	0.008%
12	4.322	938	943	948	rBV2	350	367	0.08%	0.011%
13	4.402	966	968	970	rBV	278	99	0.02%	0.003%
14	4.415	970	972	973	rBV	274	129	0.03%	0.004%
15	4.512	1000	1002	1005	rVB	255	109	0.02%	0.003%
16	4.557	1011	1016	1021	rBV2	493	619	0.14%	0.018%
17	4.618	1024	1035	1061	rBV	47975	116729	26.67%	3.370%
18	4.891	1118	1120	1122	rBV2	448	223	0.05%	0.006%
19	4.981	1145	1148	1155	rBV2	358	329	0.08%	0.009%
20	5.055	1155	1171	1191	rBV	84974	185110	42.29%	5.345%
21	5.300	1243	1247	1249	rBV2	391	272	0.06%	0.008%
22	5.354	1263	1264	1265	rBV2	138	40	0.01%	0.001%
23	5.383	1266	1273	1278	rVV2	436	635	0.15%	0.018%
24	5.573	1330	1332	1334	rBV	206	82	0.02%	0.002%
25	5.647	1353	1355	1356	rBV	170	71	0.02%	0.002%
26	5.718	1359	1377	1402	rVV3	158874	437728	100.00%	12.639%
27	5.894	1430	1432	1437	rVB2	1210	856	0.20%	0.025%
28	5.959	1451	1452	1453	rBV	248	83	0.02%	0.002%
29	6.081	1488	1490	1492	rBV	323	198	0.05%	0.006%
30	6.245	1527	1541	1558	rBV	150978	291417	66.57%	8.414%
31	6.480	1612	1614	1615	rBV	367	155	0.04%	0.004%
32	6.624	1658	1659	1661	rBV	242	110	0.03%	0.003%
33	6.685	1664	1678	1697	rBV	109717	213356	48.74%	6.160%
34	6.914	1748	1749	1750	rBV	275	98	0.02%	0.003%
35	7.078	1797	1800	1802	rBV	249	177	0.04%	0.005%
36	7.251	1852	1854	1856	rBV	422	283	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071923\
 Data File : VU054823.D
 Acq On : 19 Jul 2023 16:34
 Operator : MD/SY
 Sample : VIBLK102
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK102

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
 Title : VOC Analysis

37	7.299	1867	1869	1871	rBV	374	234	0.05%	0.007%
38	7.444	1911	1914	1916	rBV	342	238	0.05%	0.007%
39	7.560	1940	1950	1972	rBV	61254	109067	24.92%	3.149%
40	7.788	2017	2021	2023	rBV2	344	286	0.07%	0.008%
41	7.894	2042	2054	2076	rBV	196553	344316	78.66%	9.942%
42	8.174	2131	2141	2154	rBV2	42329	73752	16.85%	2.130%
43	8.325	2185	2188	2192	rBV3	423	240	0.05%	0.007%
44	8.496	2236	2241	2248	rBV2	545	787	0.18%	0.023%
45	8.631	2273	2283	2297	rBV2	137979	251553	57.47%	7.263%
46	8.881	2360	2361	2362	rBV	255	56	0.01%	0.002%
47	8.920	2371	2373	2376	rBV	601	386	0.09%	0.011%
48	8.952	2380	2383	2385	rBV	250	143	0.03%	0.004%
49	9.039	2408	2410	2411	rBV	136	59	0.01%	0.002%
50	9.197	2456	2459	2461	rBV	307	222	0.05%	0.006%
51	9.209	2461	2463	2467	rVV2	654	412	0.09%	0.012%
52	9.225	2467	2468	2470	rVB	393	97	0.02%	0.003%
53	9.351	2505	2507	2511	rBV	430	317	0.07%	0.009%
54	9.412	2516	2526	2544	rVV	225402	370560	84.66%	10.700%
55	9.595	2582	2583	2584	rBV	321	99	0.02%	0.003%
56	9.643	2595	2598	2600	rBV	433	259	0.06%	0.007%
57	9.688	2610	2612	2614	rBV	300	158	0.04%	0.005%
58	9.824	2653	2654	2655	rVB	411	79	0.02%	0.002%
59	10.094	2734	2738	2739	rBV	260	200	0.05%	0.006%
60	10.254	2786	2788	2791	rBV	442	189	0.04%	0.005%
61	10.450	2846	2849	2851	rBV3	439	298	0.07%	0.009%
62	10.541	2874	2877	2879	rBV2	547	220	0.05%	0.006%
63	10.598	2892	2895	2898	rBV	510	358	0.08%	0.010%
64	10.753	2933	2943	2959	rVB	185990	303480	69.33%	8.763%
65	10.872	2978	2980	2981	rBV	427	154	0.04%	0.004%
66	11.081	3042	3045	3047	rBV	158	99	0.02%	0.003%
67	11.190	3076	3079	3081	rBV	363	200	0.05%	0.006%
68	11.566	3194	3196	3199	rBV	284	124	0.03%	0.004%
69	11.627	3214	3215	3217	rBV	189	96	0.02%	0.003%
70	11.807	3259	3271	3290	rBV	253961	393780	89.96%	11.370%
71	12.190	3380	3390	3405	rVB	219148	358375	81.87%	10.348%
72	12.296	3421	3423	3429	rBV	544	395	0.09%	0.011%
73	15.007	4264	4266	4267	rBV	480	168	0.04%	0.005%




Sum of corrected areas: 3463332

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071923\
Data File : VU054823.D
Acq On : 19 Jul 2023 16:34
Operator : MD/SY
Sample : VIBLK102
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK102

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

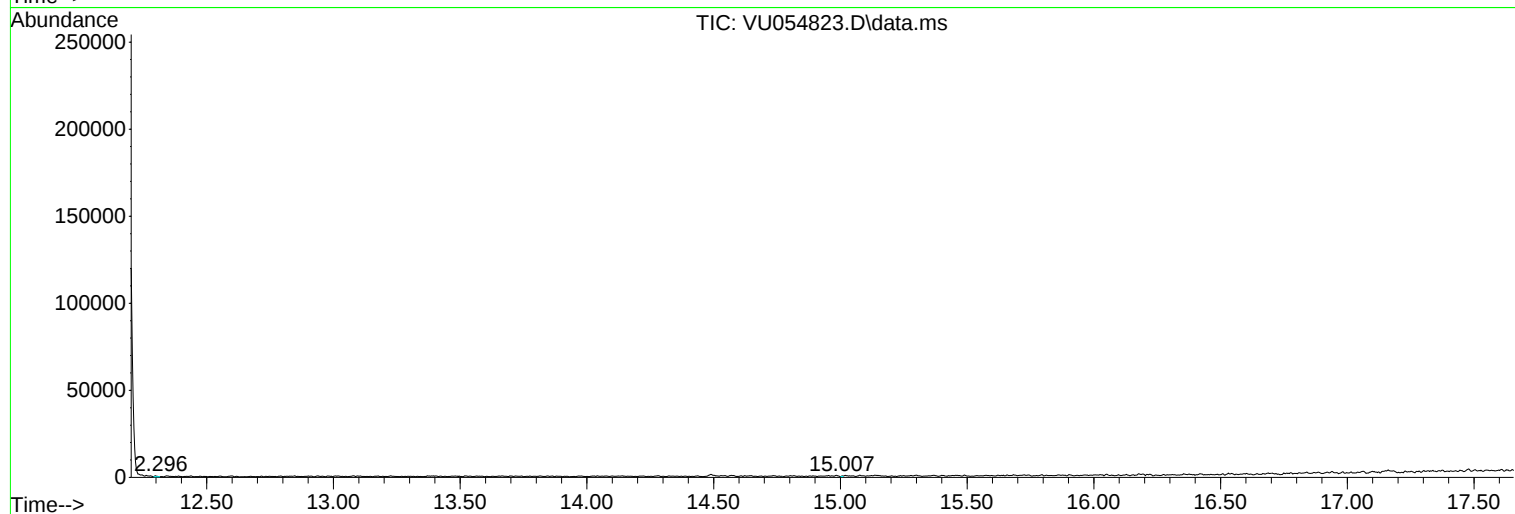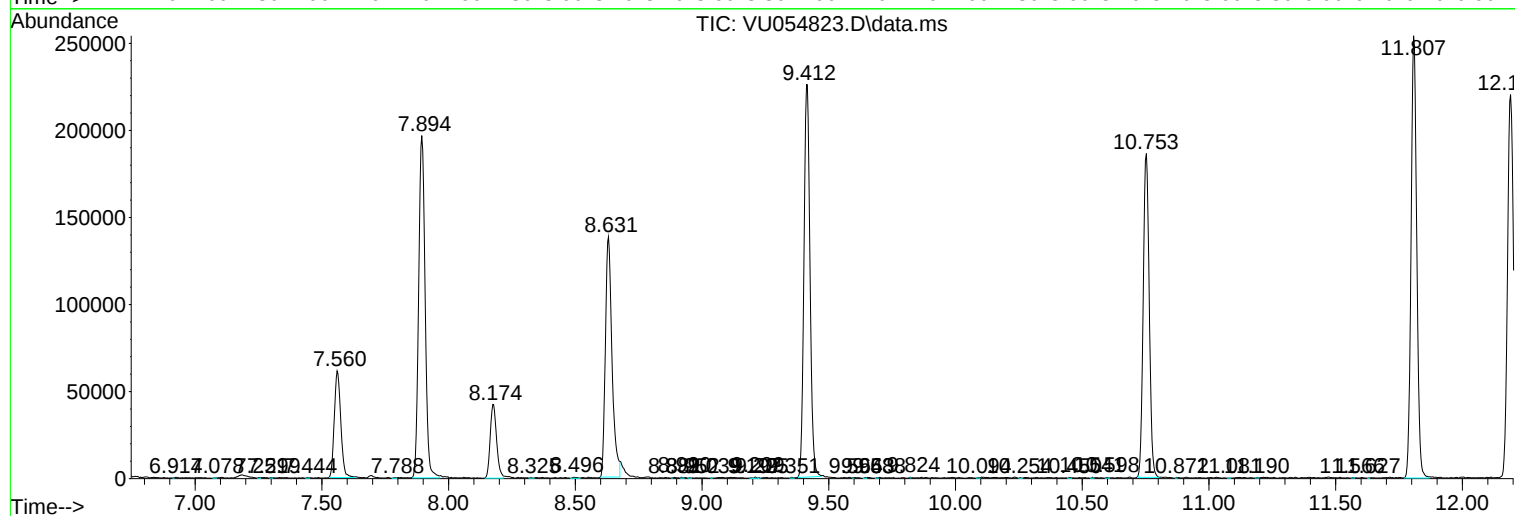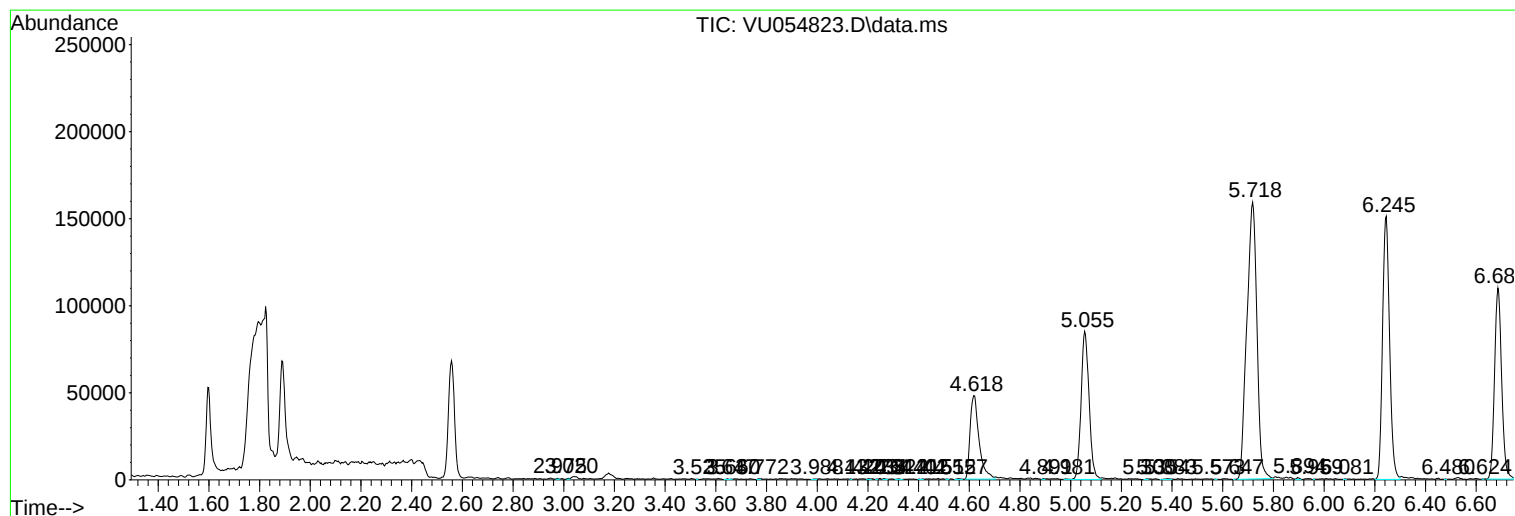

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071923\
Data File : VU054823.D
Acq On : 19 Jul 2023 16:34
Operator : MD/SY
Sample : VIBLK102
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK102

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071923\
Data File : VU054823.D
Acq On : 19 Jul 2023 16:34
Operator : MD/SY
Sample : VIBLK102
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK102

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------