

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072018\
 Data File : VU025540.D
 Acq On : 20 Jul 2018 14:38
 Operator : MD/SY
 Sample : J4039-08
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jul 21 01:30:42 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 21 01:28:05 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	337631	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	300439	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	136407	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	53076	27.54	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	55.08%#
7) Chloroethane-d5	1.68	69	52124	32.78	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	65.56%#
11) 1,1-Dichloroethene-d2	2.27	63	94216	23.48	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	46.96%#
21) 2-Butanone-d5	4.18	46	149529	100.48	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.48%
24) Chloroform-d	4.65	84	168446	39.23	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.46%
26) 1,2-Dichloroethane-d4	5.31	65	116767	41.12	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.24%
32) Benzene-d6	5.35	84	310557	40.30	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.60%
36) 1,2-Dichloropropane-d6	6.34	67	108210	43.58	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	87.16%
41) Toluene-d8	7.57	98	284656	38.52	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	77.04%#
43) trans-1,3-Dichloropropene-	7.85	79	50584	39.89	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.78%
47) 2-Hexanone-d5	8.31	63	106916	102.84	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	102.84%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	156906	45.19	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.38%
64) 1,2-Dichlorobenzene-d4	11.86	152	122423	44.28	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.56%


Target Compounds					Ovalue
37) 1,2-Dichloropropane	6.33	63	12441	5.274 ug/L	# 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU072018\
Data File : VU025540.D
Acq On : 20 Jul 2018 14:38
Operator : MD/SY
Sample : J4039-08
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jul 21 01:30:42 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 21 01:28:05 2018
Response via : Initial Calibration

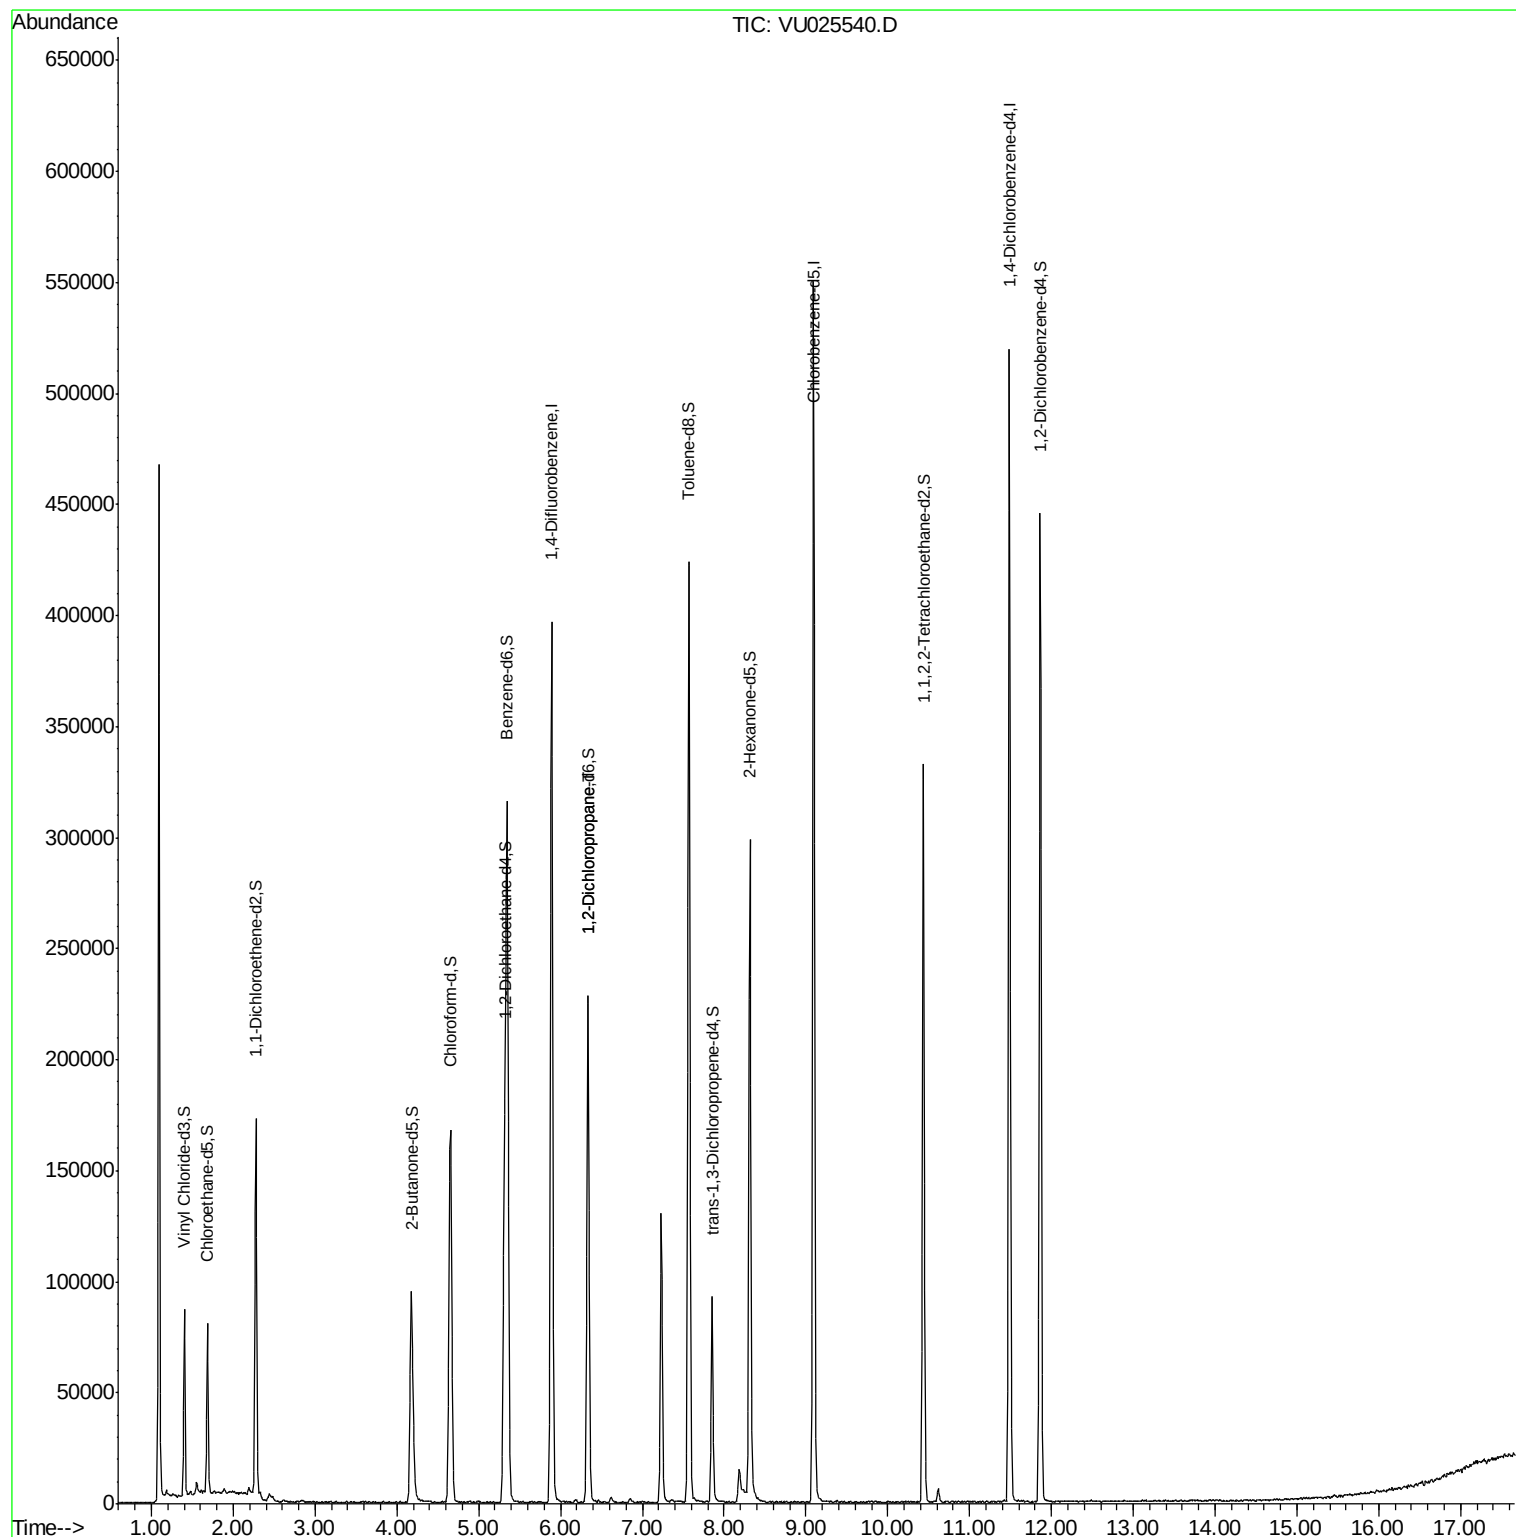

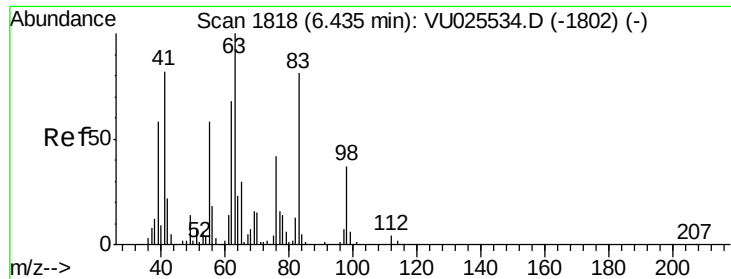

#37

1,2-Dichloropropane

Concen: 5.274 ug/L

RT: 6.33 min Scan# 1786

Delta R.T. -0.10 min

Lab File: VU025540.D

Acq: 20 Jul 2018 14:38

Instrument :
MSVOA_U
ClientSampleId :

Tot Ion: 63 Resp: 12441

Ion Ratio Lower Upper

63 100

112 0.0 3.3 4.9#

