

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072018\
 Data File : VU025554.D
 Acq On : 20 Jul 2018 20:03
 Operator : MD/SY
 Sample : J4097-04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AA3

Quant Time: Jul 21 03:19:22 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 21 02:53:20 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	318019	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	289718	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	133953	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	79046	43.54	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.08%
7) Chloroethane-d5	1.68	69	67855	45.31	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.62%
11) 1,1-Dichloroethene-d2	2.27	63	130395	34.50	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.00%
21) 2-Butanone-d5	4.18	46	146102	104.24	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	104.24%
24) Chloroform-d	4.65	84	183646	45.41	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.82%
26) 1,2-Dichloroethane-d4	5.31	65	125658	46.98	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.96%
32) Benzene-d6	5.35	84	355985	47.91	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.82%
36) 1,2-Dichloropropane-d6	6.34	67	115957	48.43	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.86%
41) Toluene-d8	7.57	98	333303	46.77	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.54%
43) trans-1,3-Dichloropropene-	7.85	79	56500	46.20	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.40%
47) 2-Hexanone-d5	8.31	63	108582	108.31	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	108.31%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	156975	46.88	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.76%
64) 1,2-Dichlorobenzene-d4	11.86	152	133638	49.23	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.46%


Target Compounds					Ovalue
18) Methyl tert-butyl Ether	3.00	73	17469	2.60 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU072018\
Data File : VU025554.D
Acq On : 20 Jul 2018 20:03
Operator : MD/SY
Sample : J4097-04
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AA3

Quant Time: Jul 21 03:19:22 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 21 02:53:20 2018
Response via : Initial Calibration

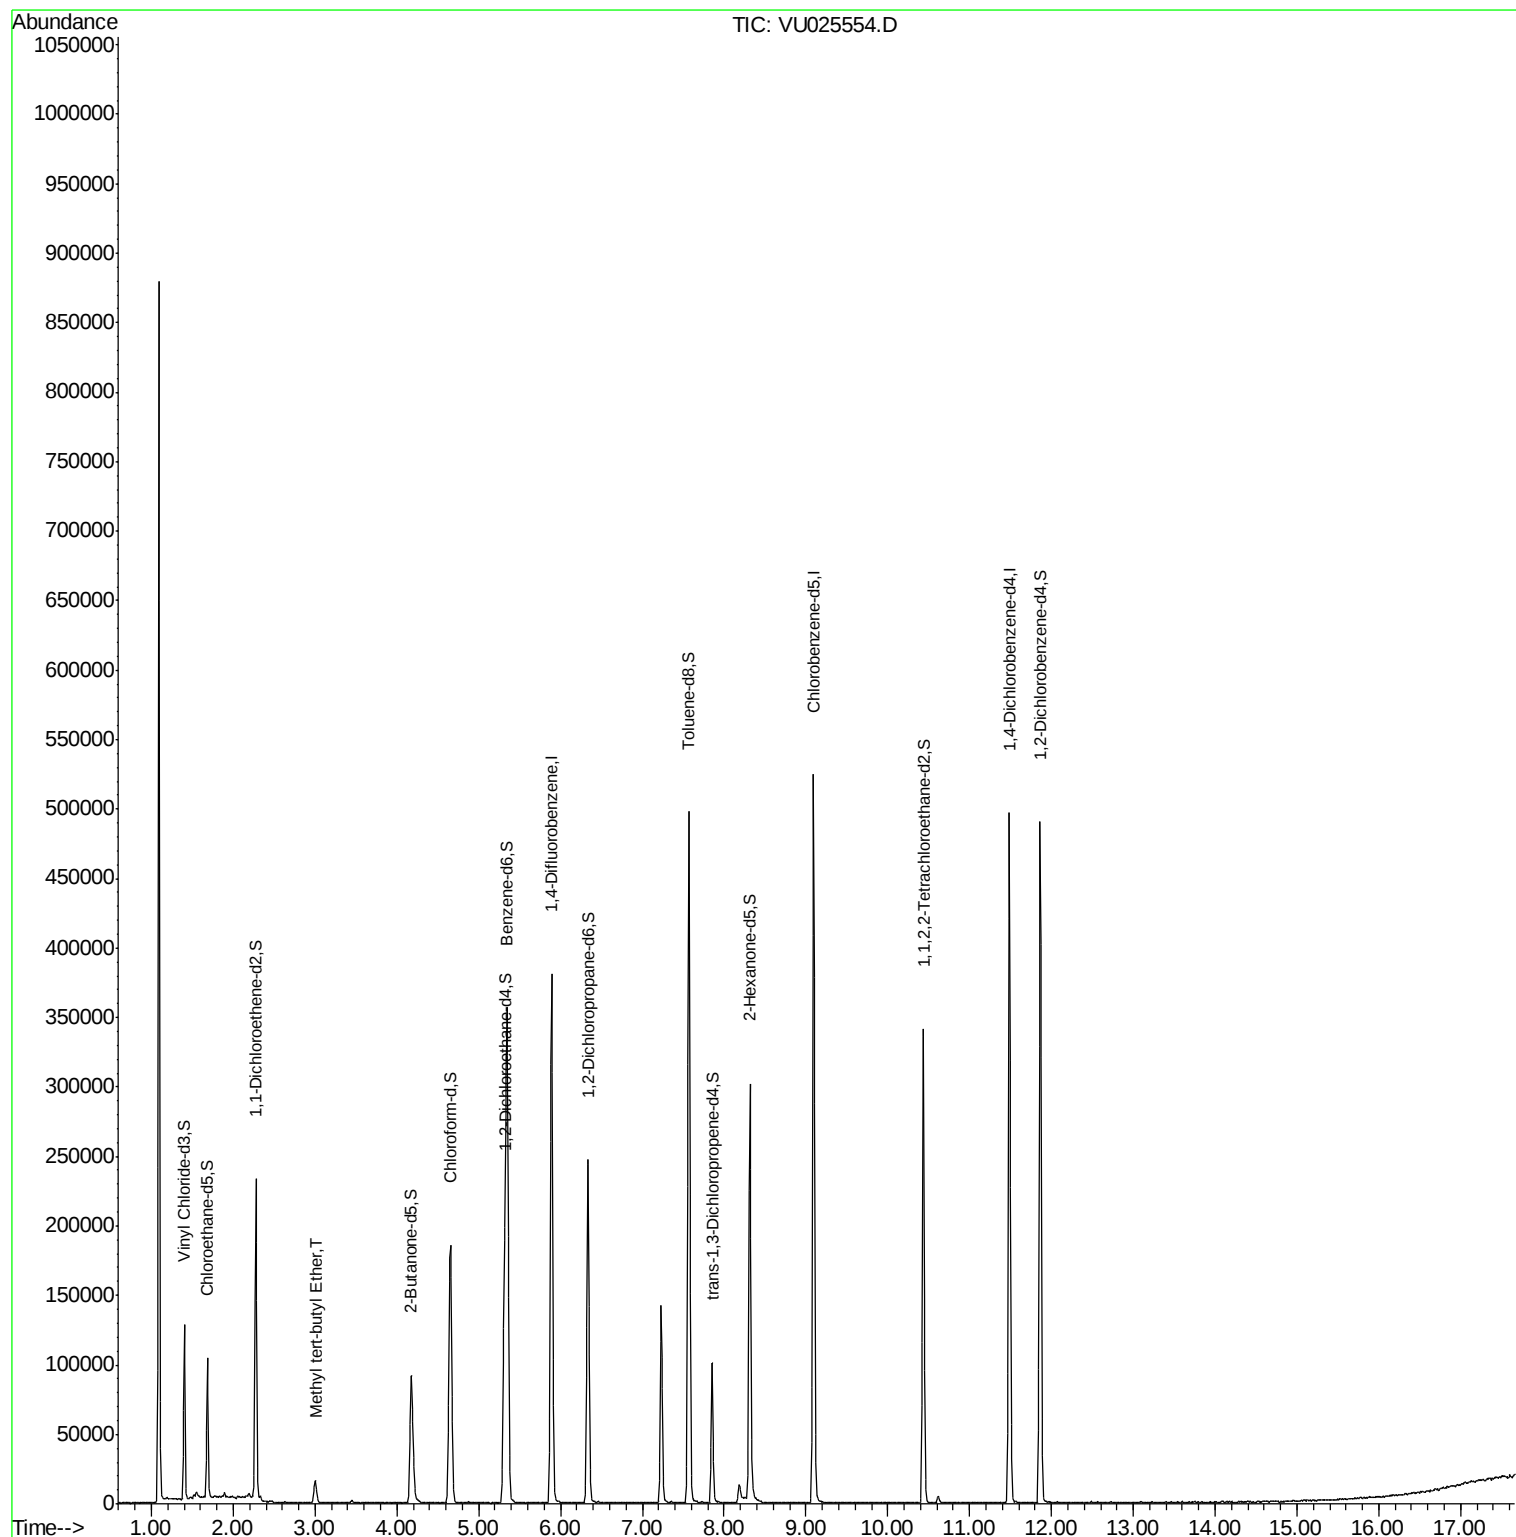

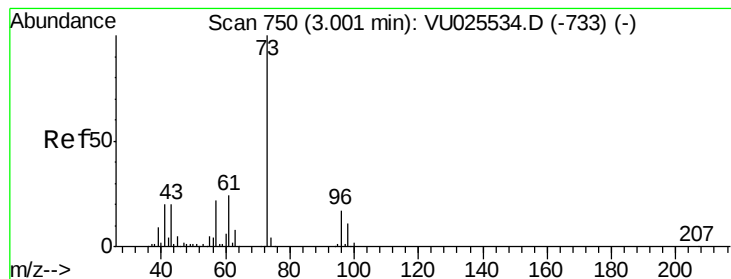

#18

Methyl tert-butyl Ether

Concen: 2.60 ug/L

RT: 3.00 min Scan# 750

Delta R.T. 0.00 min

Lab File: VU025554.D

Acq: 20 Jul 2018 20:03

Instrument :

MSVOA_U

ClientSampleId :

H0AA3

Tot Ion: 73 Resp: 17469

Ion Ratio Lower Upper

73 100

43 22.1 16.2 24.2

57 20.3 17.1 25.7

