

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072018\
 Data File : VU025555.D
 Acq On : 20 Jul 2018 20:26
 Operator : MD/SY
 Sample : J4097-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AA4

Quant Time: Jul 21 03:21:03 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 21 02:53:20 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	323825	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	294824	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	134045	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	80486	43.54	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.08%
7) Chloroethane-d5	1.68	69	68693	45.05	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.10%
11) 1,1-Dichloroethene-d2	2.27	63	131633	34.20	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.40%
21) 2-Butanone-d5	4.18	46	144428	101.19	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	101.19%
24) Chloroform-d	4.65	84	183885	44.66	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.32%
26) 1,2-Dichloroethane-d4	5.31	65	126765	46.55	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.10%
32) Benzene-d6	5.35	84	360496	47.68	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.36%
36) 1,2-Dichloropropane-d6	6.34	67	115803	47.53	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.06%
41) Toluene-d8	7.57	98	332595	45.87	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.74%
43) trans-1,3-Dichloropropene-	7.85	79	56158	45.12	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.24%
47) 2-Hexanone-d5	8.31	63	107550	105.42	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	105.42%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	162902	47.81	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.62%
64) 1,2-Dichlorobenzene-d4	11.86	152	133869	49.28	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.56%


Target Compounds					Ovalue
18) Methyl tert-butyl Ether	3.00	73	22252	3.25 ug/L	96
19) 1,1-Dichloroethane	3.45	63	21950	5.48 ug/L	99




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU072018\
Data File : VU025555.D
Acq On : 20 Jul 2018 20:26
Operator : MD/SY
Sample : J4097-05
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AA4

Quant Time: Jul 21 03:21:03 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 21 02:53:20 2018
Response via : Initial Calibration




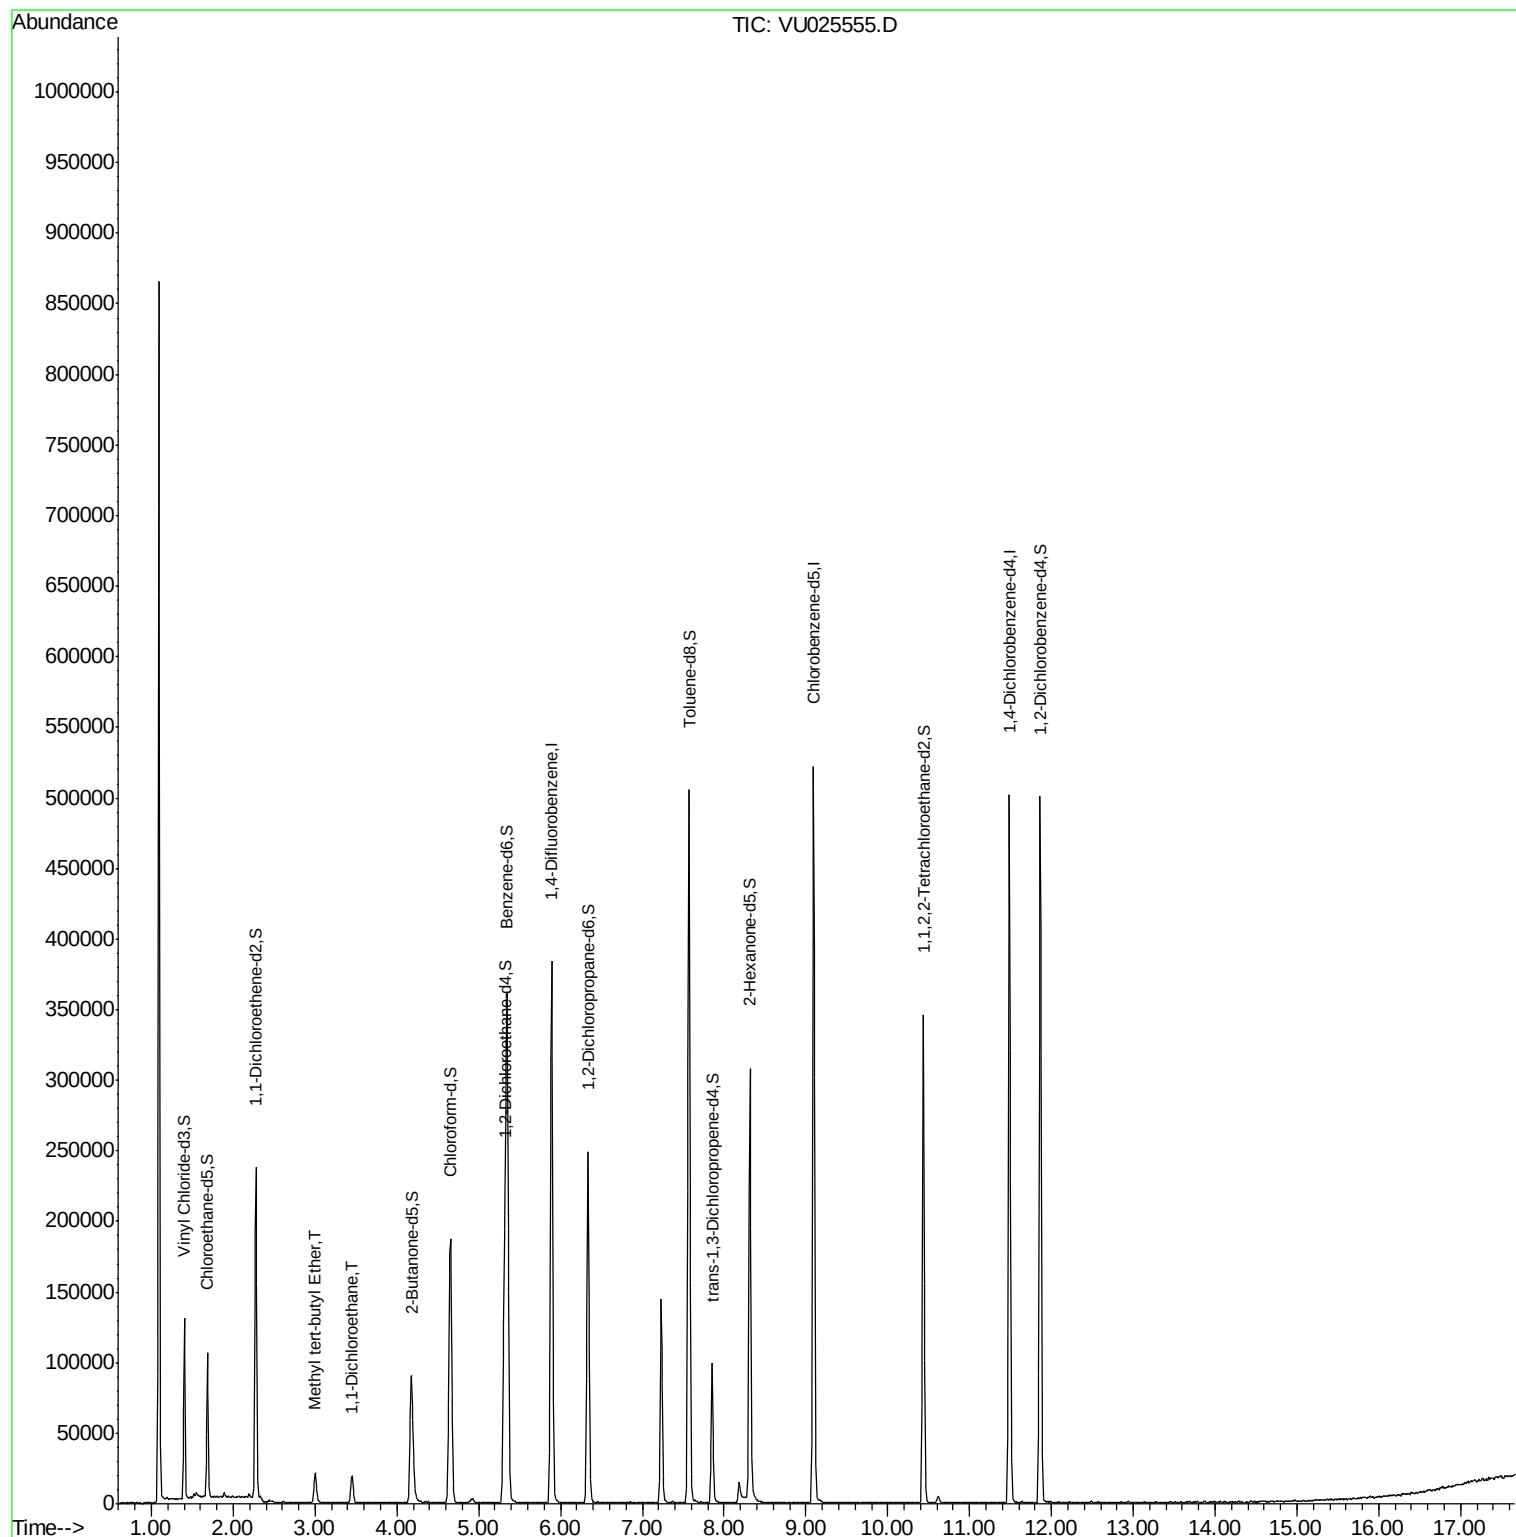


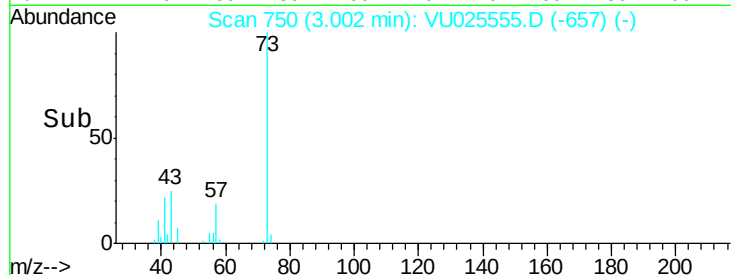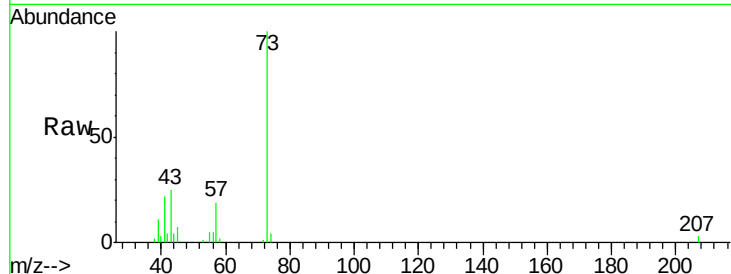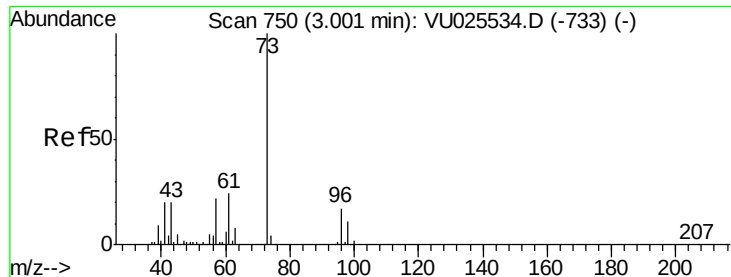

#18
Methyl tert-butyl Ether
Concen: 3.25 ug/L
RT: 3.00 min Scan# 750
Delta R.T. 0.00 min
Lab File: VU025555.D
Acq: 20 Jul 2018 20:26

Instrument :
MSVOA_U
ClientSampleId :
H0AA4

Tot Ion	Ratio	Lower	Upper
73	100		
43	23.1	16.2	24.2
57	20.8	17.1	25.7

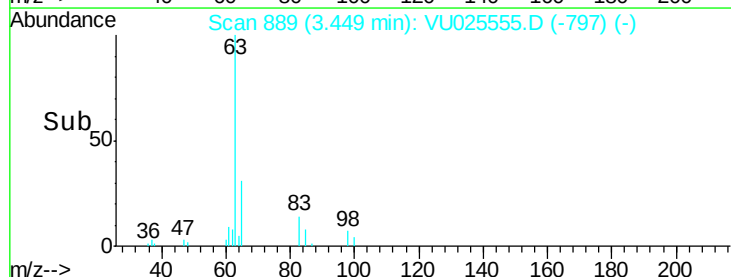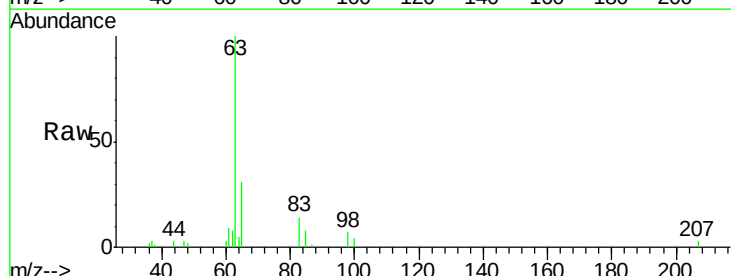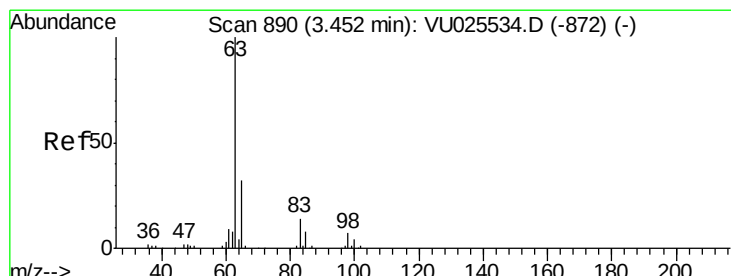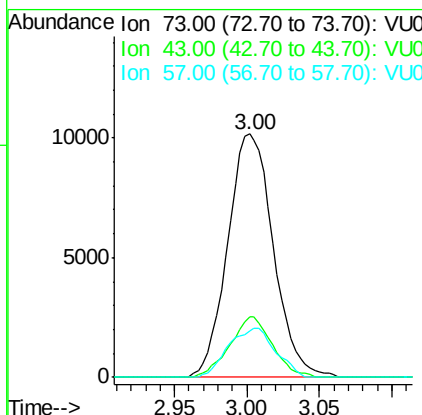

#19
1,1-Dichloroethane
Concen: 5.48 ug/L
RT: 3.45 min Scan# 889
Delta R.T. -0.00 min
Lab File: VU025555.D
Acq: 20 Jul 2018 20:26

Tgt Ion	Ratio	Lower	Upper
63	100		
65	31.2	22.0	41.0
83	14.5	9.6	17.8

