

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072018\
 Data File : VU025557.D
 Acq On : 20 Jul 2018 21:13
 Operator : MD/SY
 Sample : J4097-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AA6

Manual Integrations
 APPROVED

MMDadoda
 7/24/2018 9:30:11 AM

Quant Time: Jul 23 07:26:20 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 21 02:53:20 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	319834	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	291035	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	133630	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	80399	44.03	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	88.06%
7) Chloroethane-d5	1.68	69	69663	46.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.50%
11) 1,1-Dichloroethene-d2	2.27	63	132508	34.86	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.72%
21) 2-Butanone-d5	4.18	46	146419	103.87	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	103.87%
24) Chloroform-d	4.65	84	186497	45.85	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.70%
26) 1,2-Dichloroethane-d4	5.31	65	130692	48.59	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.18%
32) Benzene-d6	5.35	84	365313	48.94	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.88%
36) 1,2-Dichloropropane-d6	6.34	67	119490	49.68	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.36%
41) Toluene-d8	7.57	98	339358	47.41	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.82%
43) trans-1,3-Dichloropropene-	7.85	79	55805	45.42	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.84%
47) 2-Hexanone-d5	8.31	63	110948	110.17	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	110.17%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	162433	48.29	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.58%
64) 1,2-Dichlorobenzene-d4	11.86	152	136350	50.35	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.70%

Target Compounds						Ovalue
18) Methyl tert-butyl Ether	3.00	73	15337	2.27	ug/L	97
20) cis-1,2-Dichloroethene	4.24	96	4376m	1.87	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU072018\
Data File : VU025557.D
Acq On : 20 Jul 2018 21:13
Operator : MD/SY
Sample : J4097-07
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 31 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
H0AA6

Manual Integrations
APPROVED

MMDadoda
7/24/2018 9:30:11 AM

Quant Time: Jul 23 07:26:20 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 21 02:53:20 2018
Response via : Initial Calibration

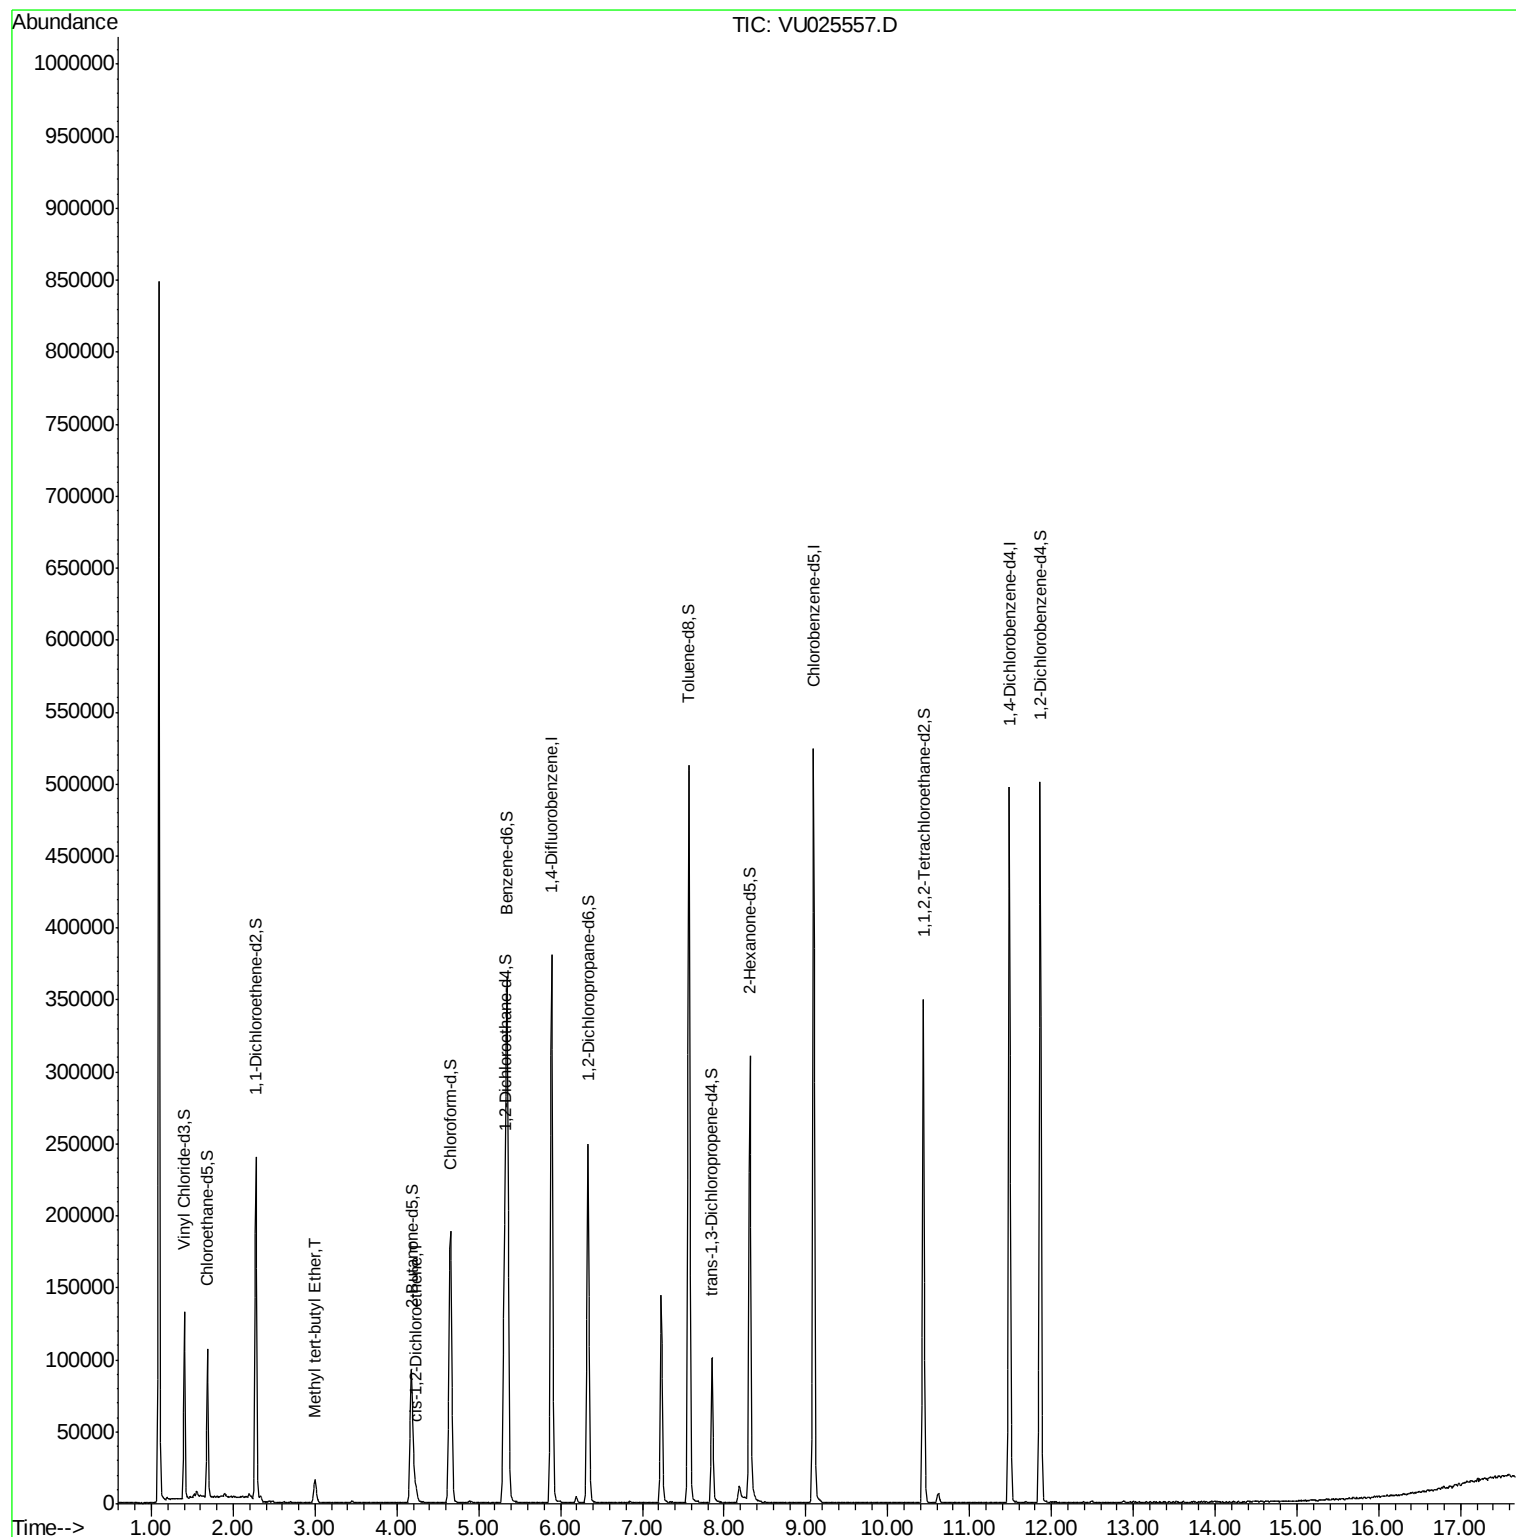

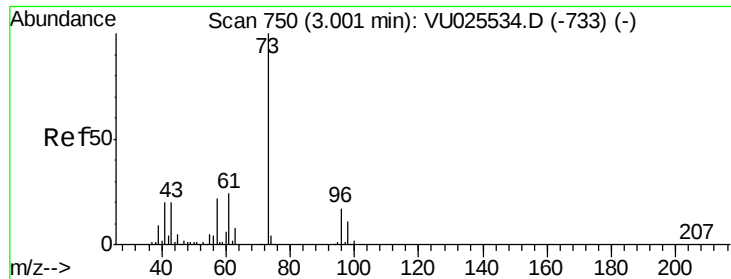





#18
Methvl tert-butvl Ether
Concen: 2.27 ug/L
RT: 3.00 min Scan# 750
Delta R.T. 0.00 min
Lab File: VU025557.D
Acq: 20 Jul 2018 21:13

Instrument :
MSVOA_U
ClientSampleId :
H0AA6

Tot Ion:	73	Resp:	15337
Ion	Ratio	Lower	Upper
73	100		
43	22.4	16.2	24.2
57	21.7	17.1	25.7

Manual Integrations
APPROVED

MMDadoda
7/24/2018 9:30:11 AM

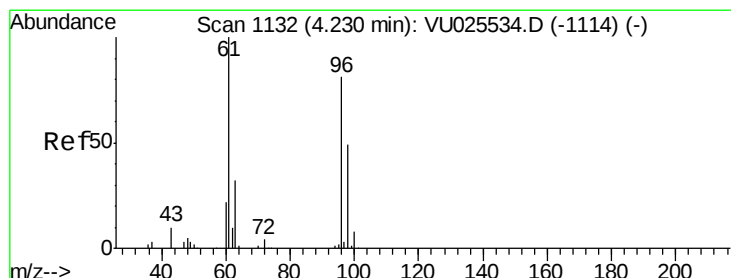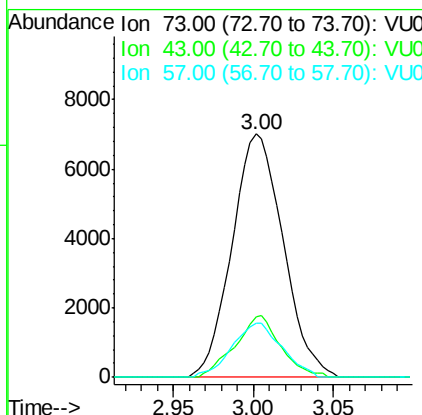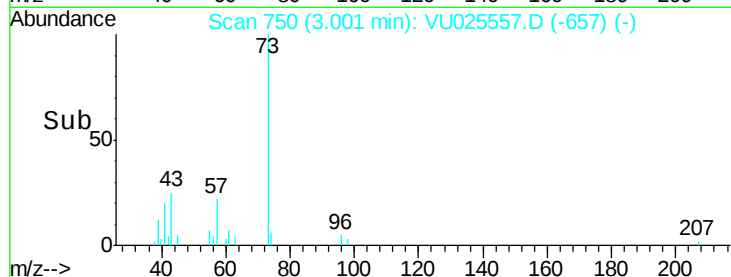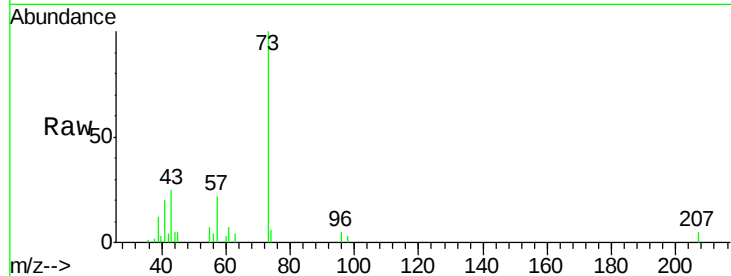

#20
cis-1,2-Dichloroethene
Concen: 1.87 ug/L m
RT: 4.24 min Scan# 1134
Delta R.T. 0.00 min
Lab File: VU025557.D
Acq: 20 Jul 2018 21:13

Tgt Ion:	96	Resp:	4376
Ion	Ratio	Lower	Upper
96	100		
61	116.4	87.4	162.2
68	0.0	0.0	0.0

