

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072018\
 Data File : VU025540.D
 Acq On : 20 Jul 2018 14:38
 Operator : MD/SY
 Sample : J4039-08
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB1P6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.687	26	30	31	rBV2	236	158	0.02%	0.002%
2	0.719	38	40	48	rVB3	330	255	0.03%	0.003%
3	0.767	52	55	57	rBV	251	150	0.02%	0.002%
4	0.834	74	76	78	rBV	189	126	0.01%	0.001%
5	0.886	88	92	95	rBV3	255	188	0.02%	0.002%
6	0.976	116	120	122	rBV	246	166	0.02%	0.002%
7	0.992	122	125	127	rBV	186	145	0.02%	0.002%
8	1.015	130	132	136	rVB2	223	131	0.01%	0.002%
9	1.088	136	155	172	rBV	467398	538886	56.90%	6.357%
10	1.404	246	253	265	rBV	83660	88739	9.37%	1.047%
11	1.683	334	340	355	rVB	76526	96865	10.23%	1.143%
12	2.275	516	524	536	rVB	168618	251889	26.60%	2.972%
13	2.574	614	617	620	rBV	371	233	0.02%	0.003%
14	2.944	729	732	735	rBV2	293	197	0.02%	0.002%
15	2.992	744	747	752	rVB2	588	449	0.05%	0.005%
16	3.085	773	776	781	rBV3	316	270	0.03%	0.003%
17	3.169	798	802	804	rBV2	271	183	0.02%	0.002%
18	3.256	825	829	832	rBV2	539	449	0.05%	0.005%
19	3.349	851	858	861	rBV3	326	369	0.04%	0.004%
20	3.384	864	869	874	rVB3	675	555	0.06%	0.007%
21	3.410	874	877	880	rVB	280	176	0.02%	0.002%
22	3.445	886	888	890	rBV	331	196	0.02%	0.002%
23	3.477	896	898	903	rVB2	336	177	0.02%	0.002%
24	3.516	907	910	915	rVB	249	238	0.03%	0.003%
25	3.542	915	918	919	rBV2	325	201	0.02%	0.002%
26	3.612	937	940	945	rBV2	528	425	0.04%	0.005%
27	3.834	1004	1009	1013	rBV3	486	505	0.05%	0.006%
28	3.876	1019	1022	1023	rBV	197	123	0.01%	0.001%
29	3.902	1028	1030	1037	rVB3	381	285	0.03%	0.003%
30	4.030	1069	1070	1078	rVB	460	349	0.04%	0.004%
31	4.108	1091	1094	1098	rBV2	386	236	0.02%	0.003%
32	4.178	1098	1116	1143	rBV	95285	246999	26.08%	2.914%
33	4.452	1197	1201	1203	rBV	300	229	0.02%	0.003%
34	4.551	1228	1232	1236	rBV4	656	525	0.06%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072018\
 Data File : VU025540.D
 Acq On : 20 Jul 2018 14:38
 Operator : MD/SY
 Sample : J4039-08
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB1P6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

35	4.580	1239	1241	1245	rBV	268	162	0.002%	0.0002%
36	4.654	1245	1264	1284	rBV	167851	395133	41.72%	4.662%
37	4.789	1301	1306	1310	rBV2	322	287	0.03%	0.003%
38	4.825	1316	1317	1320	rVB3	328	145	0.02%	0.002%
39	4.879	1331	1334	1335	rBV2	784	423	0.04%	0.005%
40	4.989	1362	1368	1369	rBV2	666	619	0.07%	0.007%
41	5.101	1401	1403	1407	rVB2	455	291	0.03%	0.003%
42	5.140	1408	1415	1421	rBV4	655	721	0.08%	0.009%
43	5.233	1441	1444	1447	rBV	188	144	0.02%	0.002%
44	5.346	1455	1479	1501	rBV2	315436	947046	100.00%	11.173%
45	5.513	1527	1531	1533	rBV2	481	313	0.03%	0.004%
46	5.603	1553	1559	1564	rBV2	344	477	0.05%	0.006%
47	5.628	1564	1567	1569	rBV	359	207	0.02%	0.002%
48	5.744	1601	1603	1606	rBV2	383	211	0.02%	0.002%
49	5.805	1619	1622	1627	rVB2	415	290	0.03%	0.003%
50	5.837	1627	1632	1633	rBV	270	218	0.02%	0.003%
51	5.892	1633	1649	1669	rBV	396165	778115	82.16%	9.180%
52	6.095	1710	1712	1714	rBV	333	176	0.02%	0.002%
53	6.146	1725	1728	1731	rBV2	249	207	0.02%	0.002%
54	6.178	1731	1738	1739	rBV3	1002	1157	0.12%	0.014%
55	6.227	1749	1753	1756	rBV2	264	205	0.02%	0.002%
56	6.252	1756	1761	1766	rBV2	416	454	0.05%	0.005%
57	6.336	1772	1787	1807	rBV	227932	448620	47.37%	5.293%
58	6.461	1819	1826	1831	rBV3	897	975	0.10%	0.012%
59	6.487	1831	1834	1837	rBV2	368	233	0.02%	0.003%
60	6.526	1842	1846	1847	rBV2	276	178	0.02%	0.002%
61	6.612	1866	1873	1874	rBV3	2167	2005	0.21%	0.024%
62	6.757	1916	1918	1922	rVB3	286	195	0.02%	0.002%
63	6.783	1922	1926	1929	rVB2	267	189	0.02%	0.002%
64	6.844	1940	1945	1948	rBV5	1551	1695	0.18%	0.020%
65	6.902	1961	1963	1970	rVB3	215	128	0.01%	0.002%
66	6.976	1984	1986	1988	rVB	442	183	0.02%	0.002%
67	7.059	2009	2012	2013	rBV2	262	156	0.02%	0.002%
68	7.085	2018	2020	2023	rVB	290	130	0.01%	0.002%
69	7.233	2052	2066	2087	rBV2	130311	230998	24.39%	2.725%
70	7.323	2092	2094	2096	rVB2	507	216	0.02%	0.003%
71	7.355	2098	2104	2106	rBV4	1052	1041	0.11%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072018\
 Data File : VU025540.D
 Acq On : 20 Jul 2018 14:38
 Operator : MD/SY
 Sample : J4039-08
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB1P6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

72	7.567	2157	2170	2187	rBV	423000	737750	77.90%	8.703%
73	7.744	2222	2225	2226	rBV	529	246	0.03%	0.003%
74	7.853	2248	2259	2276	rBV	92366	153356	16.19%	1.809%
75	8.053	2318	2321	2325	rBV	550	316	0.03%	0.004%
76	8.098	2331	2335	2339	rVB2	345	303	0.03%	0.004%
77	8.185	2349	2362	2371	rBV2	15109	33880	3.58%	0.400%
78	8.313	2391	2402	2431	rVB	296839	517926	54.69%	6.110%
79	8.561	2477	2479	2482	rVB	426	271	0.03%	0.003%
80	8.580	2482	2485	2486	rBV2	413	228	0.02%	0.003%
81	8.635	2498	2502	2505	rVB3	544	365	0.04%	0.004%
82	8.892	2580	2582	2585	rBV	398	221	0.02%	0.003%
83	9.005	2614	2617	2620	rBV2	453	254	0.03%	0.003%
84	9.024	2620	2623	2625	rVB	331	178	0.02%	0.002%
85	9.091	2631	2644	2669	rBV	549656	896429	94.66%	10.575%
86	9.352	2722	2725	2727	rBV	380	261	0.03%	0.003%
87	9.381	2730	2734	2739	rVB3	846	968	0.10%	0.011%
88	9.760	2850	2852	2857	rBV2	369	300	0.03%	0.004%
89	9.882	2888	2890	2894	rBV2	245	170	0.02%	0.002%
90	10.098	2955	2957	2961	rVV2	328	220	0.02%	0.003%
91	10.123	2963	2965	2970	rVB2	480	340	0.04%	0.004%
92	10.246	3000	3003	3007	rBV2	334	284	0.03%	0.003%
93	10.435	3049	3062	3080	rBV	331996	529767	55.94%	6.250%
94	10.535	3090	3093	3094	rBV	343	130	0.01%	0.002%
95	10.615	3109	3118	3132	rVB2	6103	11079	1.17%	0.131%
96	10.670	3132	3135	3137	rBV2	231	156	0.02%	0.002%
97	10.969	3224	3228	3231	rBV2	557	512	0.05%	0.006%
98	11.487	3376	3389	3413	rBV	519112	822114	86.81%	9.699%
99	11.863	3494	3506	3528	rBV	445136	722842	76.33%	8.528%
100	12.114	3581	3584	3589	rBV3	611	639	0.07%	0.008%


Sum of corrected areas: 8476515

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU072018\
Data File : VU025540.D
Acq On : 20 Jul 2018 14:38
Operator : MD/SY
Sample : J4039-08
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB1P6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

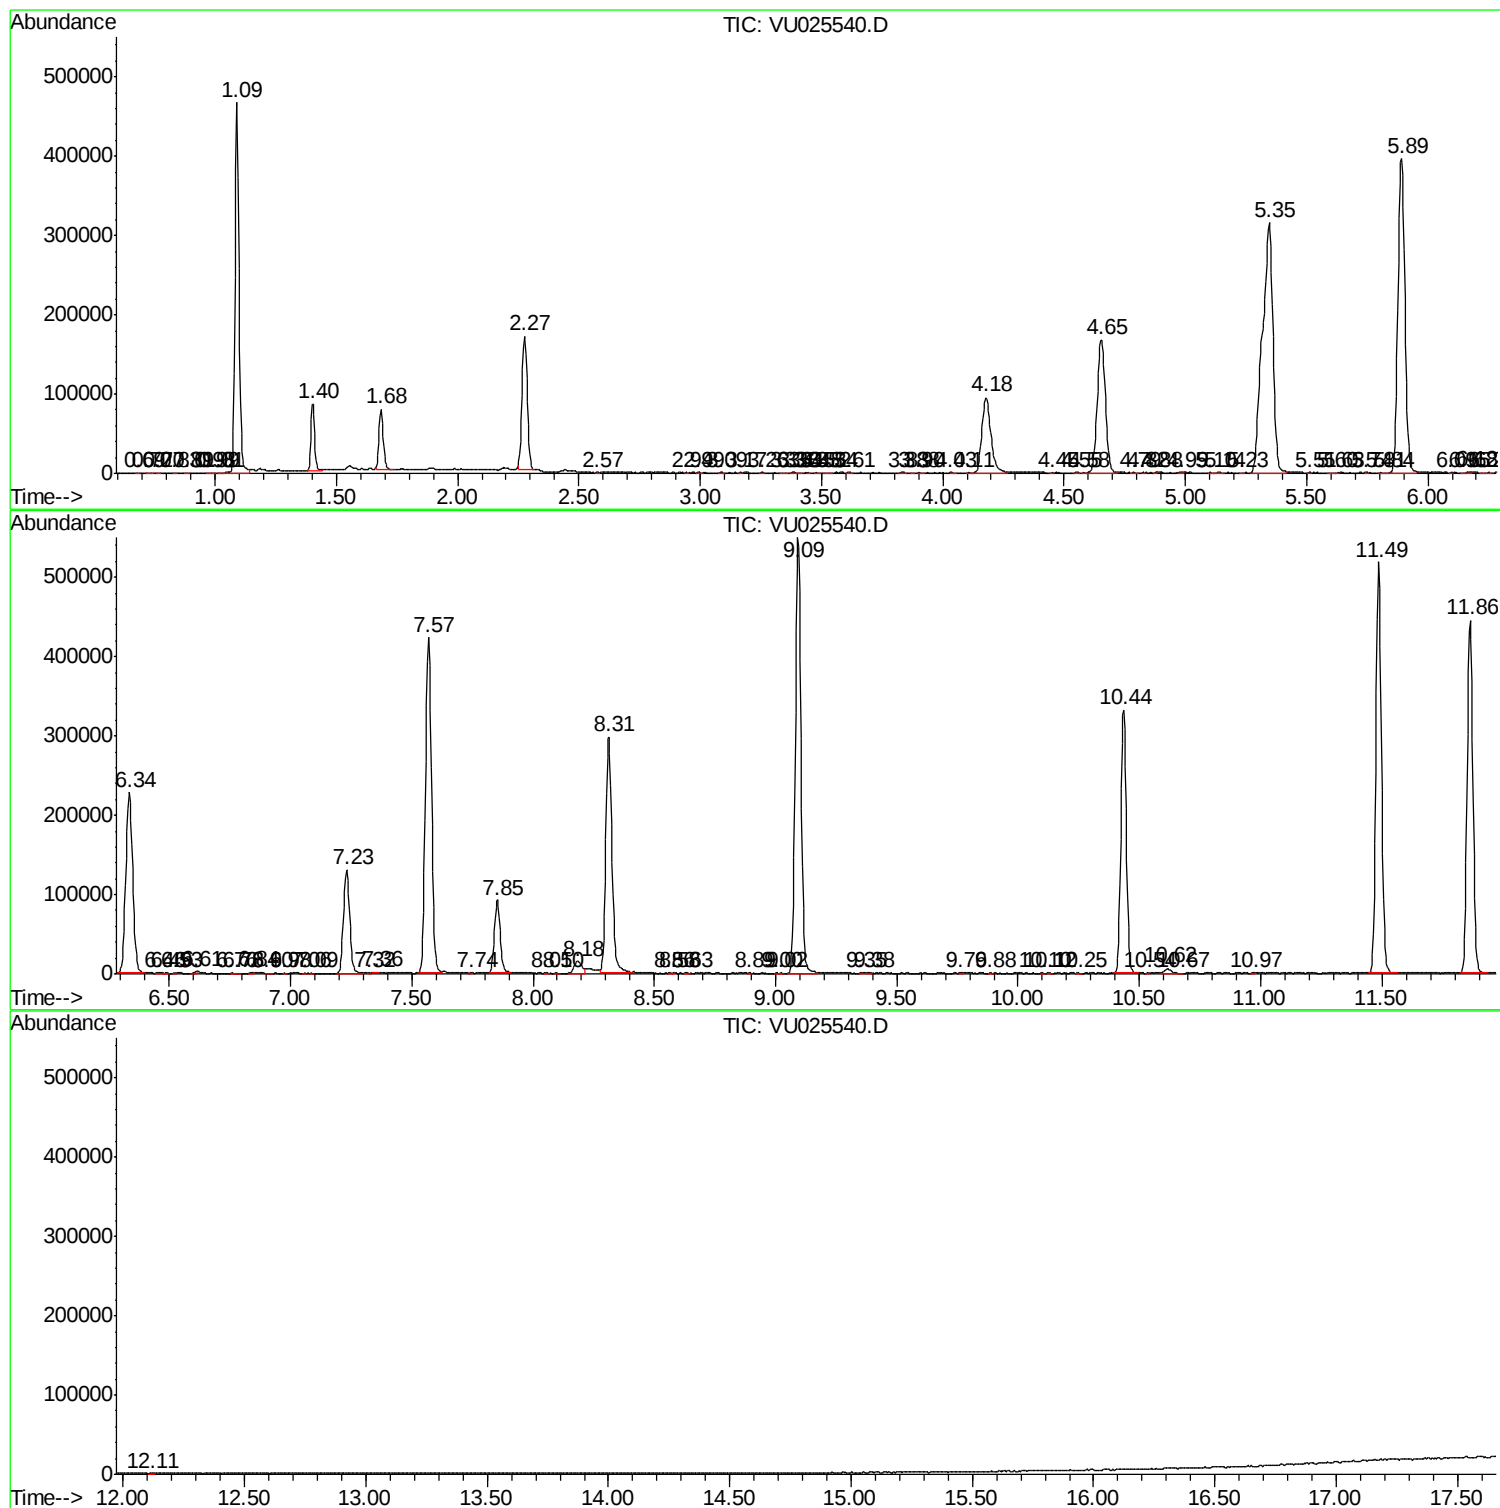

Data_Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU072018\
Data_File : VU025540.D
Acq_On : 20 Jul 2018 14:388
Operator : MD/SYY
Sample : J4039-088
Misc : 5.0mL/MSVOA_U/WATER
ALS_Vial : 14 Sample_Multiplier: 11

Instrument :
MSVOA_U
ClientSampleId :
DB1P6

Quant_Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.MM
Quant_Title : VOC_Analysis

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
