

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072018\
 Data File : VU025541.D
 Acq On : 20 Jul 2018 15:01
 Operator : MD/SY
 Sample : J4039-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB1P7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.622	7	10	12	rBV	258	141	0.002%	0.0002%
2	0.674	24	26	28	rBV2	201	123	0.001%	0.0002%
3	0.690	28	31	35	rVV2	309	248	0.003%	0.0003%
4	0.712	35	38	41	rVV3	274	185	0.002%	0.0002%
5	0.757	50	52	55	rBV	135	99	0.001%	0.0001%
6	0.792	60	63	65	rBV	112	76	0.001%	0.0001%
7	0.802	65	66	71	rVV2	209	137	0.001%	0.0002%
8	0.828	71	74	78	rVV	231	198	0.002%	0.0002%
9	0.850	78	81	86	rVB2	342	295	0.003%	0.0004%
10	0.870	86	87	88	rBV2	133	38	0.000%	0.0000%
11	0.931	100	106	108	rBV2	439	389	0.004%	0.0005%
12	0.985	121	123	124	rBV2	252	117	0.001%	0.0001%
13	1.088	147	155	171	rBV	285847	325058	34.60%	4.010%
14	1.403	246	253	263	rBV	87034	86808	9.24%	1.071%
15	1.683	333	340	353	rVB	76689	97201	10.35%	1.199%
16	2.275	515	524	535	rBV	168811	250710	26.68%	3.093%
17	2.712	658	660	663	rBV	382	251	0.003%	0.0003%
18	2.825	693	695	696	rBV2	464	186	0.002%	0.0002%
19	2.921	723	725	728	rBV2	387	253	0.003%	0.0003%
20	2.985	741	745	749	rBV3	469	402	0.004%	0.0005%
21	3.018	752	755	758	rBV4	420	283	0.003%	0.0003%
22	3.111	779	784	789	rBV3	532	511	0.005%	0.0006%
23	3.133	789	791	794	rBV	194	103	0.001%	0.0001%
24	3.345	855	857	862	rVB2	352	209	0.002%	0.0003%
25	3.381	866	868	869	rBV	357	144	0.002%	0.0002%
26	3.477	896	898	901	rBV	430	286	0.003%	0.0004%
27	3.493	901	903	907	rVV2	402	287	0.003%	0.0004%
28	3.689	962	964	966	rBV	219	89	0.001%	0.0001%
29	3.702	966	968	970	rBV	216	102	0.001%	0.0001%
30	3.786	991	994	997	rBV	223	151	0.002%	0.0002%
31	3.815	998	1003	1004	rBV2	378	294	0.003%	0.0004%
32	3.918	1032	1035	1036	rBV	325	167	0.002%	0.0002%
33	4.178	1100	1116	1143	rBV	95560	250326	26.64%	3.088%
34	4.423	1190	1192	1195	rBV2	393	253	0.003%	0.0003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072018\
 Data File : VU025541.D
 Acq On : 20 Jul 2018 15:01
 Operator : MD/SY
 Sample : J4039-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB1P7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

35	4.564	1233	1236	1239	rBV	223	120	0.01%	0.001%
36	4.587	1239	1243	1246	rBV3	600	542	0.06%	0.007%
37	4.654	1247	1264	1284	rVV	169312	394755	42.02%	4.869%
38	4.744	1289	1292	1294	rBV	464	307	0.03%	0.004%
39	4.792	1304	1307	1312	rBV3	270	174	0.02%	0.002%
40	4.879	1329	1334	1337	rBV3	803	949	0.10%	0.012%
41	4.966	1359	1361	1362	rBV2	281	101	0.01%	0.001%
42	5.017	1375	1377	1384	rVB2	452	367	0.04%	0.005%
43	5.050	1385	1387	1389	rBV	338	153	0.02%	0.002%
44	5.088	1397	1399	1401	rBV2	280	149	0.02%	0.002%
45	5.345	1455	1479	1499	rBV2	311792	939547	100.00%	11.590%
46	5.558	1543	1545	1547	rBV2	338	163	0.02%	0.002%
47	5.574	1547	1550	1556	rVB2	357	239	0.03%	0.003%
48	5.680	1581	1583	1587	rBV3	448	303	0.03%	0.004%
49	5.709	1587	1592	1596	rVB3	454	457	0.05%	0.006%
50	5.808	1621	1623	1625	rBV2	206	80	0.01%	0.001%
51	5.892	1634	1649	1672	rBV	391636	761266	81.02%	9.390%
52	6.172	1731	1736	1737	rBV	1006	687	0.07%	0.008%
53	6.336	1772	1787	1807	rBV	226079	445670	47.43%	5.497%
54	6.503	1837	1839	1842	rVB3	387	190	0.02%	0.002%
55	6.718	1902	1906	1907	rBV2	323	198	0.02%	0.002%
56	6.757	1914	1918	1919	rBV	419	226	0.02%	0.003%
57	6.850	1935	1947	1957	rBV5	2033	4214	0.45%	0.052%
58	6.905	1963	1964	1965	rBV5	227	49	0.01%	0.001%
59	7.178	2047	2049	2052	rBV	281	160	0.02%	0.002%
60	7.230	2053	2065	2084	rBV	128117	226985	24.16%	2.800%
61	7.355	2098	2104	2105	rBV4	1332	1069	0.11%	0.013%
62	7.426	2123	2126	2128	rBV	344	245	0.03%	0.003%
63	7.467	2136	2139	2141	rBV2	342	209	0.02%	0.003%
64	7.570	2156	2171	2188	rBV	420934	732806	78.00%	9.039%
65	7.734	2220	2222	2224	rBV2	402	199	0.02%	0.002%
66	7.853	2247	2259	2279	rBV	89214	153985	16.39%	1.899%
67	7.979	2295	2298	2300	rBV2	409	241	0.03%	0.003%
68	8.313	2392	2402	2428	rVB	294939	505251	53.78%	6.232%
69	9.091	2631	2644	2675	rBV	535205	881666	93.84%	10.876%
70	9.297	2705	2708	2709	rBV	415	240	0.03%	0.003%
71	9.673	2823	2825	2828	rVB2	396	222	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072018\
Data File : VU025541.D
Acq On : 20 Jul 2018 15:01
Operator : MD/SY
Sample : J4039-09
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB1P7

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Title : VOC Analysis

72	9.699	2828	2833	2836	rBV3	427	430	0.05%	0.005%
73	10.136	2965	2969	2972	rBV2	861	751	0.08%	0.009%
74	10.435	3050	3062	3083	rVB	330906	528743	56.28%	6.522%
75	10.750	3158	3160	3163	rBV	438	234	0.02%	0.003%
76	10.808	3175	3178	3181	rBV2	606	405	0.04%	0.005%
77	11.255	3315	3317	3319	rBV2	401	161	0.02%	0.002%
78	11.419	3365	3368	3374	rVB2	1273	981	0.10%	0.012%
79	11.487	3377	3389	3411	rVV	505575	795393	84.66%	9.811%
80	11.863	3494	3506	3526	rBV	442911	709446	75.51%	8.751%


Sum of corrected areas: 8106848

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU072018\
Data File : VU025541.D
Acq On : 20 Jul 2018 15:01
Operator : MD/SY
Sample : J4039-09
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB1P7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

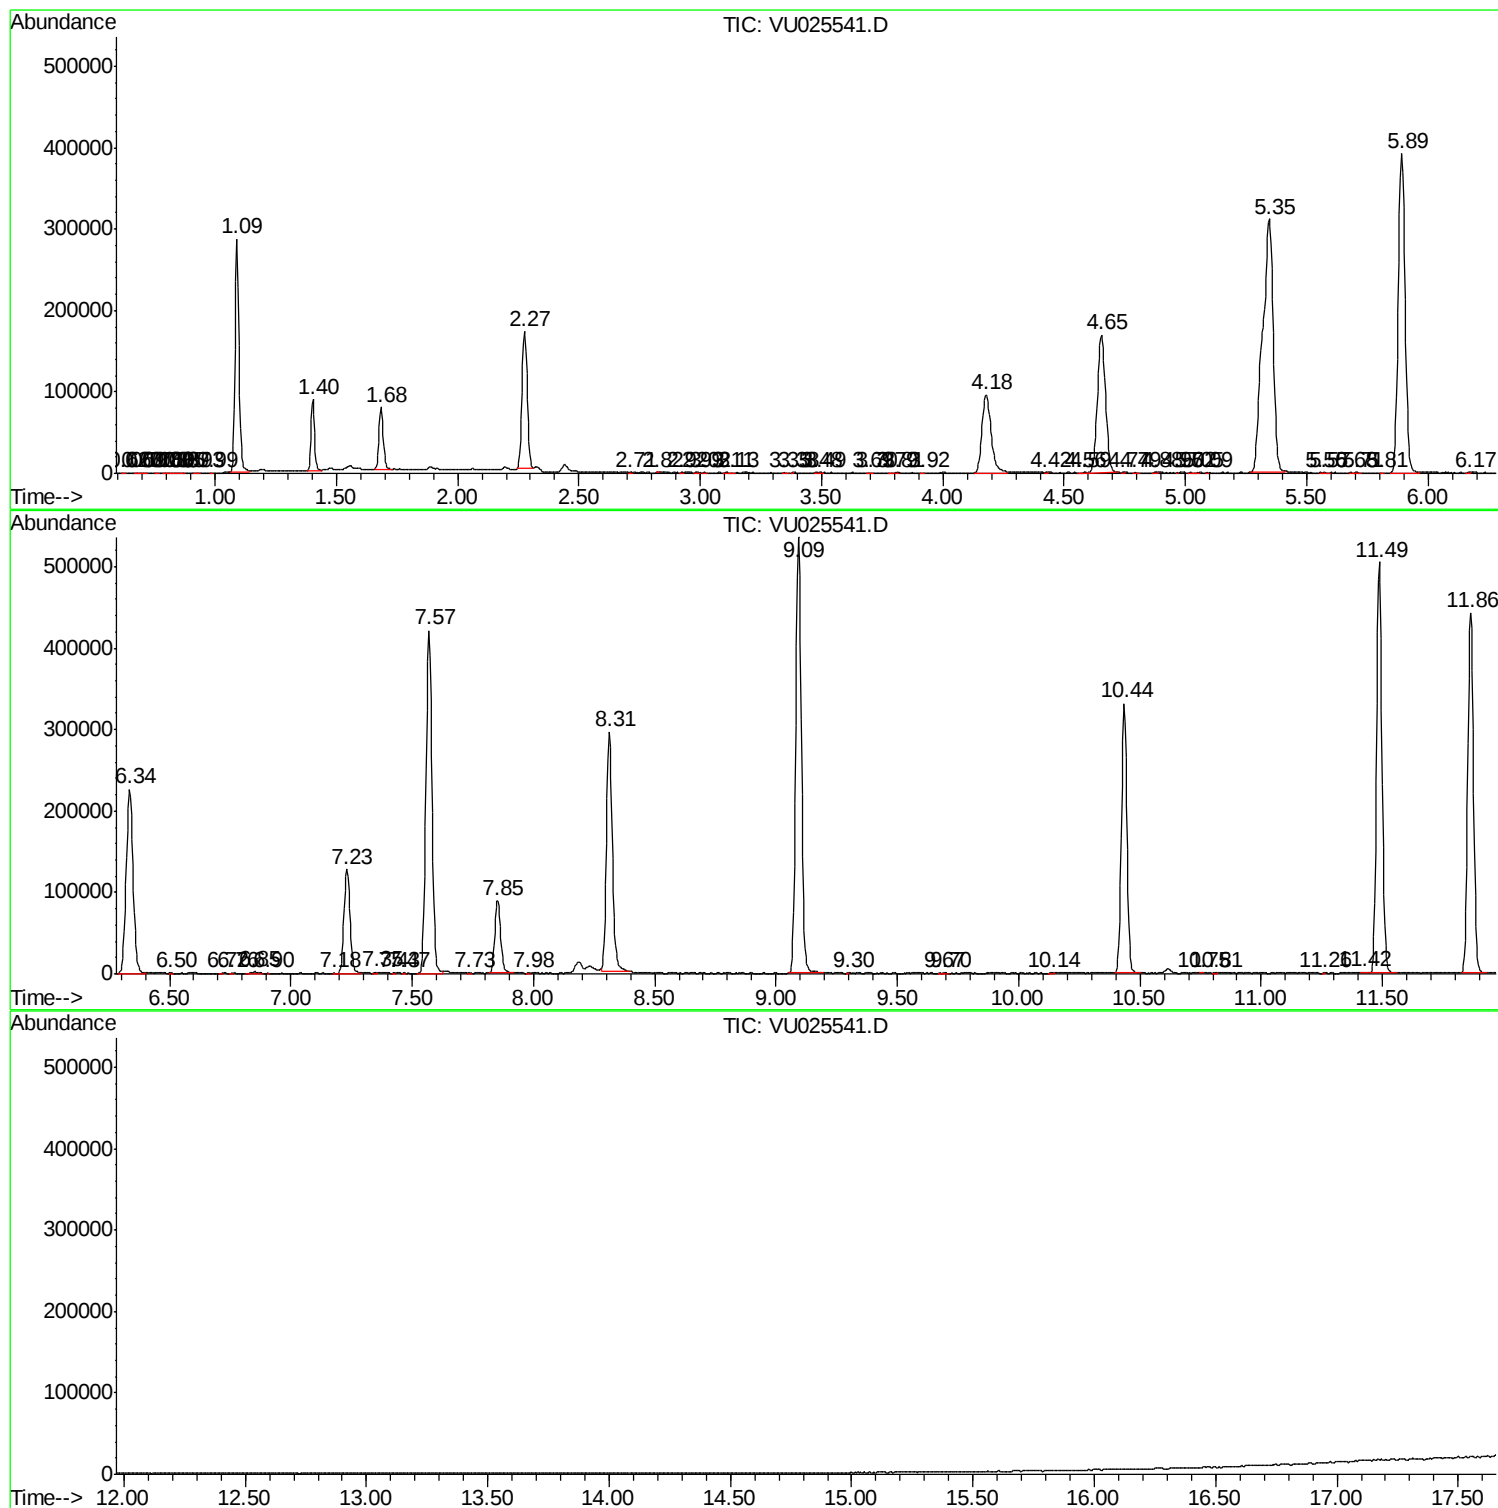

Data_Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU072018\
Data_File : VU025541.D
Acq_On : 20 Jul 2018 15:011
Operator : MD/SYY
Sample : J4039-099
Misc : 5.0mL/MSVOA_U/WATER
ALS_Vial : 15 Sample_Multiplier: 11

Instrument :
MSVOA_U
ClientSampleId :
DB1P7

Quant_Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.MM
Quant_Title : VOC_Analysis

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
