

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072018\
 Data File : VU025548.D
 Acq On : 20 Jul 2018 17:43
 Operator : MD/SY
 Sample : J4039-15
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB1R7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.645	15	17	19	rBV	260	95	0.01%	0.001%
2	0.680	26	28	31	rVB	306	135	0.01%	0.002%
3	0.748	48	49	53	rBV	271	142	0.01%	0.002%
4	0.767	53	55	58	rVB2	341	164	0.01%	0.002%
5	0.783	58	60	62	rVB	233	93	0.01%	0.001%
6	0.802	63	66	70	rVB2	172	124	0.01%	0.001%
7	0.825	70	73	76	rBV2	437	375	0.03%	0.004%
8	0.950	109	112	114	rBV2	229	178	0.02%	0.002%
9	0.995	123	126	130	rVB2	196	111	0.01%	0.001%
10	1.030	134	137	138	rBV2	266	153	0.01%	0.002%
11	1.088	142	155	173	rBV	236367	274295	24.30%	3.069%
12	1.403	246	253	268	rVB	135675	138479	12.27%	1.549%
13	1.683	333	340	354	rVB	106962	132650	11.75%	1.484%
14	2.275	515	524	536	rVB	244432	362978	32.15%	4.061%
15	2.526	600	602	606	rBV2	365	225	0.02%	0.003%
16	2.619	623	631	639	rBV4	853	1605	0.14%	0.018%
17	2.699	653	656	658	rBV2	578	402	0.04%	0.004%
18	2.735	665	667	668	rBV2	357	130	0.01%	0.001%
19	2.940	729	731	734	rVB2	283	154	0.01%	0.002%
20	2.969	737	740	741	rBV2	374	173	0.02%	0.002%
21	3.149	793	796	799	rVB2	454	282	0.02%	0.003%
22	3.317	844	848	850	rBV	285	202	0.02%	0.002%
23	3.374	863	866	869	rBV	421	313	0.03%	0.004%
24	3.407	874	876	880	rVB	276	122	0.01%	0.001%
25	3.432	880	884	889	rBV3	337	260	0.02%	0.003%
26	3.477	894	898	901	rBV2	250	232	0.02%	0.003%
27	3.493	901	903	905	rBV2	201	100	0.01%	0.001%
28	3.542	914	918	925	rVB2	461	460	0.04%	0.005%
29	3.583	925	931	934	rBV2	414	415	0.04%	0.005%
30	3.677	959	960	961	rBV2	218	76	0.01%	0.001%
31	3.722	973	974	976	rBV	207	61	0.01%	0.001%
32	3.747	979	982	983	rBV	183	95	0.01%	0.001%
33	3.789	992	995	1000	rVB2	398	355	0.03%	0.004%
34	3.860	1015	1017	1020	rVB2	235	126	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072018\
 Data File : VU025548.D
 Acq On : 20 Jul 2018 17:43
 Operator : MD/SY
 Sample : J4039-15
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB1R7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

35	4.001	1058	1061	1064	rBV2	262	200	0.02%	0.002%
36	4.050	1072	1076	1080	rBV2	207	198	0.02%	0.002%
37	4.178	1101	1116	1144	rBV	91075	236785	20.98%	2.649%
38	4.455	1199	1202	1205	rBV2	296	228	0.02%	0.003%
39	4.506	1214	1218	1224	rVB3	398	429	0.04%	0.005%
40	4.545	1227	1230	1231	rBV3	420	210	0.02%	0.002%
41	4.583	1240	1242	1244	rBV	147	95	0.01%	0.001%
42	4.654	1246	1264	1287	rVV	195148	457624	40.54%	5.119%
43	4.876	1329	1333	1335	rBV3	678	511	0.05%	0.006%
44	4.956	1356	1358	1360	rBV	174	77	0.01%	0.001%
45	5.043	1382	1385	1386	rBV	129	65	0.01%	0.001%
46	5.075	1392	1395	1397	rVB2	192	98	0.01%	0.001%
47	5.107	1400	1405	1406	rBV	236	179	0.02%	0.002%
48	5.185	1428	1429	1431	rBV	173	81	0.01%	0.001%
49	5.210	1435	1437	1439	rVB2	209	69	0.01%	0.001%
50	5.226	1439	1442	1444	rBV2	365	208	0.02%	0.002%
51	5.242	1445	1447	1449	rVB2	421	150	0.01%	0.002%
52	5.252	1449	1450	1452	rBV	221	88	0.01%	0.001%
53	5.345	1453	1479	1500	rBV2	382590	1128844	100.00%	12.628%
54	5.532	1535	1537	1538	rBV2	140	61	0.01%	0.001%
55	5.638	1565	1570	1573	rBV3	322	250	0.02%	0.003%
56	5.696	1586	1588	1592	rBV2	190	133	0.01%	0.001%
57	5.741	1599	1602	1608	rBV3	706	737	0.07%	0.008%
58	5.889	1629	1648	1666	rBV	373464	734083	65.03%	8.212%
59	6.098	1711	1713	1716	rVB2	456	291	0.03%	0.003%
60	6.123	1716	1721	1724	rBV2	457	396	0.04%	0.004%
61	6.146	1724	1728	1733	rVB3	389	366	0.03%	0.004%
62	6.172	1733	1736	1738	rBV	419	324	0.03%	0.004%
63	6.336	1772	1787	1805	rBV	255654	513958	45.53%	5.750%
64	6.541	1848	1851	1852	rBV	228	93	0.01%	0.001%
65	6.821	1936	1938	1940	rVB	209	64	0.01%	0.001%
66	6.853	1940	1948	1949	rBV5	1046	1217	0.11%	0.014%
67	6.979	1986	1987	1989	rVB5	320	89	0.01%	0.001%
68	6.998	1989	1993	1998	rBV2	369	380	0.03%	0.004%
69	7.021	1998	2000	2004	rVB	371	250	0.02%	0.003%
70	7.046	2005	2008	2014	rBV3	736	791	0.07%	0.009%
71	7.159	2039	2043	2047	rBV2	440	512	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072018\
 Data File : VU025548.D
 Acq On : 20 Jul 2018 17:43
 Operator : MD/SY
 Sample : J4039-15
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB1R7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

72	7.230	2053	2065	2081	rBV	150161	266284	23.59%	2.979%
73	7.519	2153	2155	2157	rBV3	348	156	0.01%	0.002%
74	7.570	2157	2171	2188	rBV	524021	910710	80.68%	10.188%
75	7.786	2237	2238	2239	rBV	210	61	0.01%	0.001%
76	7.799	2239	2242	2245	rVB3	521	298	0.03%	0.003%
77	7.853	2247	2259	2277	rBV	105612	179614	15.91%	2.009%
78	8.017	2308	2310	2311	rBV	315	130	0.01%	0.001%
79	8.088	2330	2332	2333	rBV	345	125	0.01%	0.001%
80	8.188	2354	2363	2372	rBV3	14613	28095	2.49%	0.314%
81	8.313	2391	2402	2426	rVB	297602	503125	44.57%	5.628%
82	8.686	2514	2518	2520	rBV	547	455	0.04%	0.005%
83	9.091	2632	2644	2673	rBV	524472	860829	76.26%	9.630%
84	9.246	2690	2692	2695	rBV3	502	316	0.03%	0.004%
85	9.313	2710	2713	2716	rBV	388	265	0.02%	0.003%
86	9.429	2745	2749	2752	rVB3	448	336	0.03%	0.004%
87	9.458	2752	2758	2762	rBV2	673	590	0.05%	0.007%
88	9.779	2855	2858	2860	rBV3	1009	653	0.06%	0.007%
89	9.879	2887	2889	2893	rBV	321	243	0.02%	0.003%
90	10.069	2944	2948	2952	rBV	494	388	0.03%	0.004%
91	10.278	3010	3013	3014	rBV	344	179	0.02%	0.002%
92	10.307	3019	3022	3025	rVB	419	289	0.03%	0.003%
93	10.435	3050	3062	3082	rBV	353058	554166	49.09%	6.199%
94	10.615	3109	3118	3128	rBV5	4596	8138	0.72%	0.091%
95	10.754	3159	3161	3163	rBV	288	127	0.01%	0.001%
96	11.419	3365	3368	3376	rVB5	1653	1899	0.17%	0.021%
97	11.487	3376	3389	3405	rBV	498842	793518	70.29%	8.877%
98	11.737	3464	3467	3474	rBV3	639	680	0.06%	0.008%
99	11.863	3493	3506	3526	rBV	516766	831203	73.63%	9.299%
100	12.586	3729	3731	3733	rBV	436	187	0.02%	0.002%


Sum of corrected areas: 8938953

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU072018\
Data File : VU025548.D
Acq On : 20 Jul 2018 17:43
Operator : MD/SY
Sample : J4039-15
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB1R7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

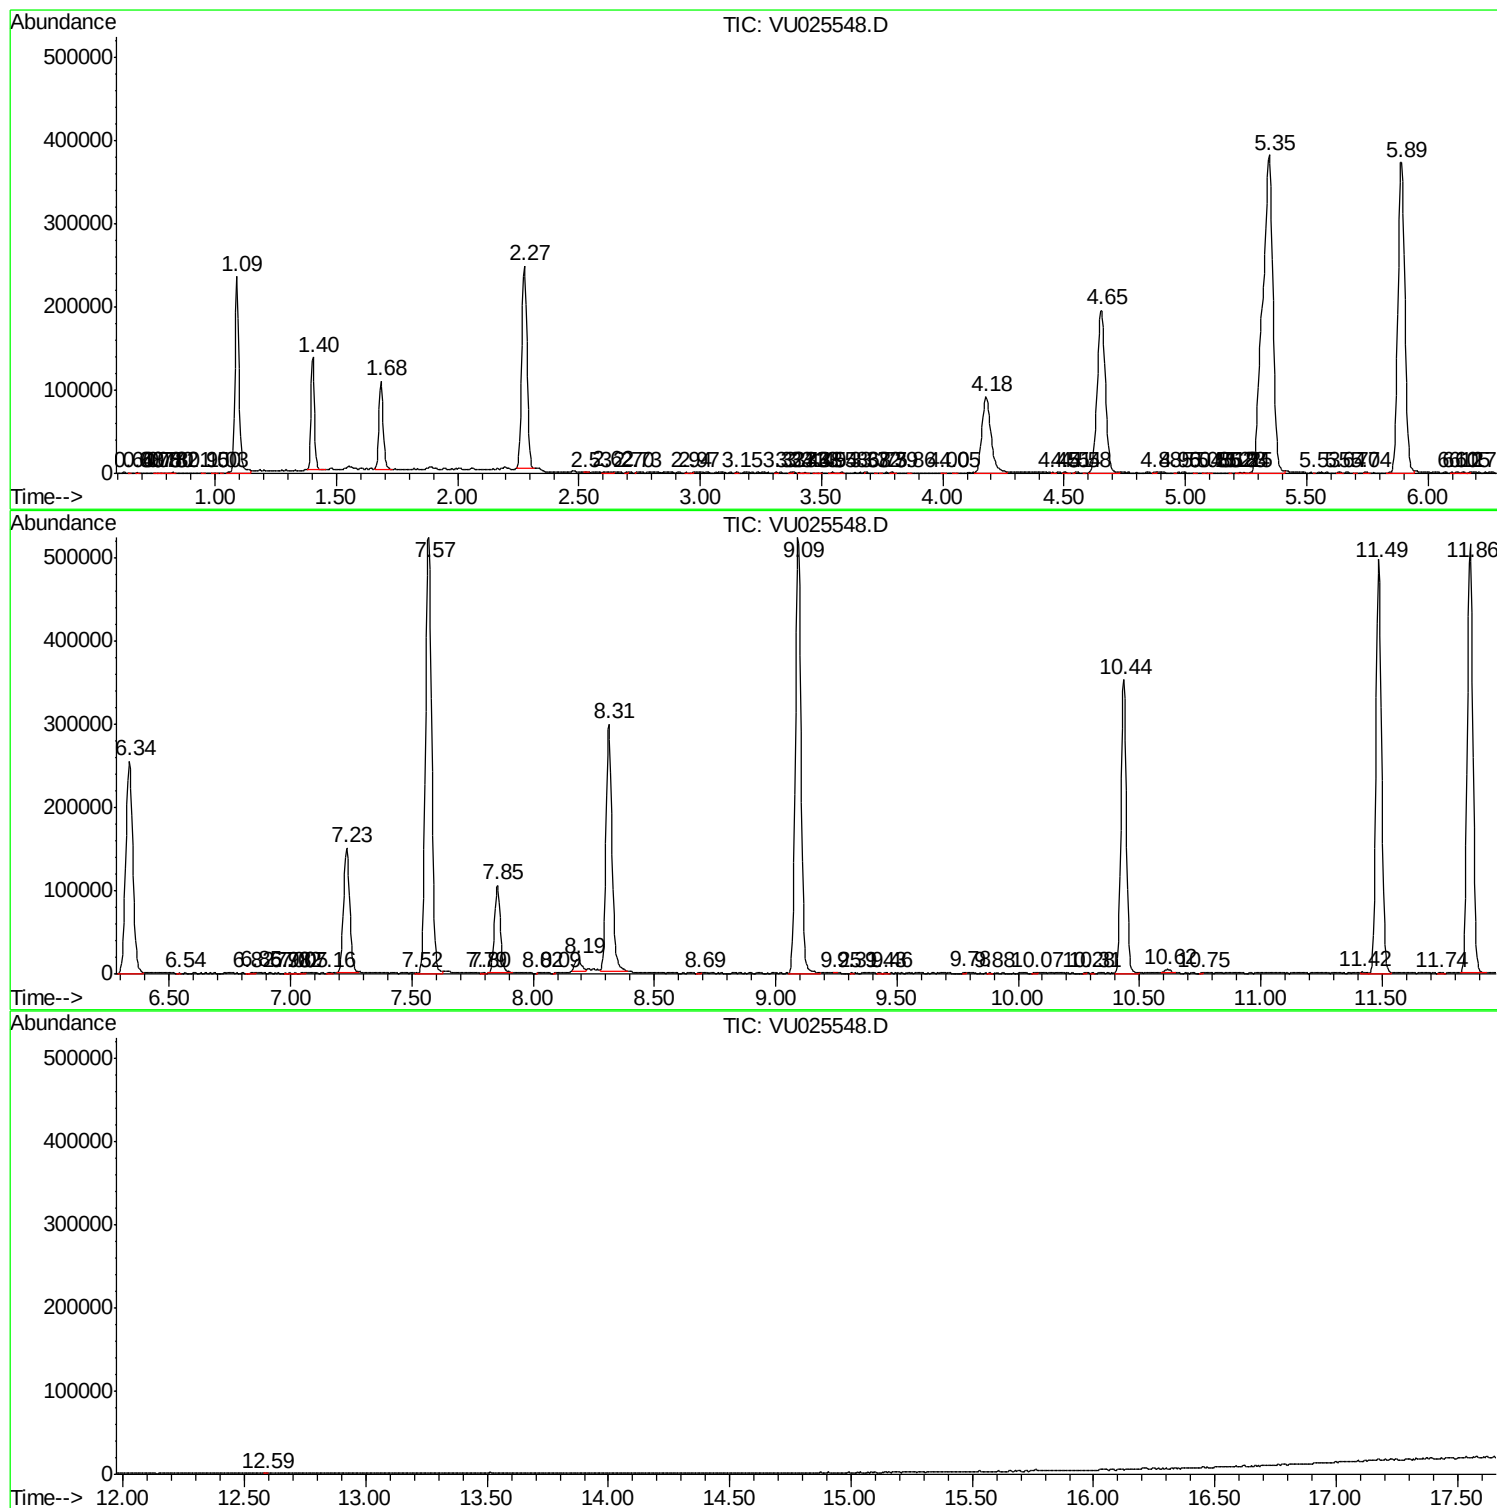

Data_Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU072018\
Data_File : VU025548.D
Acq_On : 20 Jul 2018 17:433
Operator : MD/SYY
Sample : J4039-155
Misc : 5.0mL/MSVOA_U/WATER
ALS_Vial : 22 Sample_Multiplier: 11

Instrument :
MSVOA_U
ClientSampleId :
DB1R7

Quant_Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.MM
Quant_Title : VOC_Analysis

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
