

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072018\
 Data File : VU025549.D
 Acq On : 20 Jul 2018 18:07
 Operator : MD/SY
 Sample : J4039-16
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB1S4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.625	8	11	14	rVB2	179	118	0.01%	0.001%
2	0.641	14	16	18	rVB2	183	81	0.01%	0.001%
3	0.658	18	21	29	rVB2	354	417	0.04%	0.005%
4	0.706	33	36	40	rBV2	156	165	0.01%	0.002%
5	0.818	68	71	75	rBV2	150	103	0.01%	0.001%
6	0.838	75	77	78	rBV2	153	71	0.01%	0.001%
7	0.873	86	88	90	rVB2	173	65	0.01%	0.001%
8	0.918	100	102	105	rBV	200	134	0.01%	0.002%
9	0.960	112	115	116	rBV	211	119	0.01%	0.001%
10	0.976	119	120	124	rVB2	216	104	0.01%	0.001%
11	1.008	127	130	135	rVB2	437	386	0.03%	0.004%
12	1.063	135	147	148	rBV2	1449	1837	0.16%	0.021%
13	1.092	148	156	179	rBV	163502	186480	16.58%	2.091%
14	1.403	246	253	263	rBV	133490	136048	12.10%	1.526%
15	1.683	333	340	354	rVB	104630	128856	11.46%	1.445%
16	2.275	514	524	536	rBV	244803	366490	32.59%	4.110%
17	2.899	714	718	720	rBV2	622	451	0.04%	0.005%
18	2.998	747	749	753	rBV	260	172	0.02%	0.002%
19	3.082	772	775	779	rBV	446	256	0.02%	0.003%
20	3.101	779	781	783	rBV	186	95	0.01%	0.001%
21	3.259	827	830	833	rBV2	338	234	0.02%	0.003%
22	3.294	839	841	842	rBV	210	110	0.01%	0.001%
23	3.384	865	869	878	rBV4	393	604	0.05%	0.007%
24	3.458	887	892	893	rBV	364	207	0.02%	0.002%
25	3.510	904	908	915	rVB3	531	600	0.05%	0.007%
26	3.545	916	919	922	rBV2	347	233	0.02%	0.003%
27	3.564	922	925	929	rBV3	503	365	0.03%	0.004%
28	3.616	938	941	947	rBV3	303	355	0.03%	0.004%
29	3.645	947	950	951	rBV	166	87	0.01%	0.001%
30	3.693	962	965	969	rBV3	274	308	0.03%	0.003%
31	3.802	997	999	1001	rVB2	331	161	0.01%	0.002%
32	3.825	1001	1006	1009	rBV3	456	395	0.04%	0.004%
33	3.886	1021	1025	1028	rVB3	383	306	0.03%	0.003%
34	3.918	1028	1035	1038	rBV3	416	410	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072018\
 Data File : VU025549.D
 Acq On : 20 Jul 2018 18:07
 Operator : MD/SY
 Sample : J4039-16
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB1S4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

35	3.940	1038	1042	1044	rBV2	429	224	0.02%	0.003%
36	3.973	1045	1052	1055	rBV2	497	618	0.05%	0.007%
37	4.088	1085	1088	1092	rBV	561	376	0.03%	0.004%
38	4.114	1092	1096	1100	rBV2	411	367	0.03%	0.004%
39	4.178	1100	1116	1147	rBV	93651	245085	21.80%	2.748%
40	4.374	1173	1177	1179	rBV3	777	652	0.06%	0.007%
41	4.487	1209	1212	1215	rBV3	302	212	0.02%	0.002%
42	4.506	1216	1218	1219	rBV	277	113	0.01%	0.001%
43	4.567	1236	1237	1239	rBV	218	75	0.01%	0.001%
44	4.654	1248	1264	1289	rVB	194809	452950	40.28%	5.079%
45	4.751	1289	1294	1297	rBV3	488	424	0.04%	0.005%
46	4.802	1308	1310	1313	rBV2	340	156	0.01%	0.002%
47	4.966	1359	1361	1362	rBV	178	74	0.01%	0.001%
48	4.982	1363	1366	1375	rVB3	728	852	0.08%	0.010%
49	5.024	1376	1379	1382	rBV	186	102	0.01%	0.001%
50	5.101	1400	1403	1406	rBV2	241	137	0.01%	0.002%
51	5.188	1428	1430	1431	rBV	168	73	0.01%	0.001%
52	5.345	1454	1479	1500	rBV2	378393	1124398	100.00%	12.609%
53	5.587	1548	1554	1556	rBV3	384	402	0.04%	0.005%
54	5.638	1568	1570	1571	rBV	155	70	0.01%	0.001%
55	5.648	1571	1573	1576	rBV2	154	98	0.01%	0.001%
56	5.664	1576	1578	1579	rBV	225	92	0.01%	0.001%
57	5.741	1598	1602	1605	rBV2	332	250	0.02%	0.003%
58	5.805	1619	1622	1625	rVB2	298	183	0.02%	0.002%
59	5.834	1629	1631	1634	rBV2	310	202	0.02%	0.002%
60	5.892	1634	1649	1669	rBV	391320	764882	68.03%	8.577%
61	6.172	1726	1736	1739	rBV2	613	692	0.06%	0.008%
62	6.226	1749	1753	1755	rBV2	401	239	0.02%	0.003%
63	6.239	1755	1757	1760	rBV	322	159	0.01%	0.002%
64	6.336	1771	1787	1804	rBV	255290	514563	45.76%	5.770%
65	6.455	1821	1824	1828	rBV3	808	675	0.06%	0.008%
66	6.603	1864	1870	1874	rBV3	426	405	0.04%	0.005%
67	6.841	1941	1944	1946	rBV3	691	468	0.04%	0.005%
68	6.931	1969	1972	1973	rBV	280	126	0.01%	0.001%
69	7.104	2023	2026	2028	rBV2	226	136	0.01%	0.002%
70	7.117	2028	2030	2032	rVV	282	127	0.01%	0.001%
71	7.133	2032	2035	2039	rVB	317	239	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072018\
 Data File : VU025549.D
 Acq On : 20 Jul 2018 18:07
 Operator : MD/SY
 Sample : J4039-16
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB1S4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

72	7.185	2048	2051	2053	rBV	205	136	0.01%	0.002%
73	7.230	2053	2065	2084	rBV	150474	265870	23.65%	2.981%
74	7.570	2157	2171	2191	rBV	518360	905168	80.50%	10.150%
75	7.853	2247	2259	2278	rBV	104103	177822	15.81%	1.994%
76	8.043	2315	2318	2321	rVB3	502	335	0.03%	0.004%
77	8.062	2321	2324	2325	rBV2	316	156	0.01%	0.002%
78	8.188	2350	2363	2372	rBV	15748	33733	3.00%	0.378%
79	8.313	2391	2402	2430	rVB	299322	517738	46.05%	5.806%
80	8.506	2459	2462	2464	rBV3	575	304	0.03%	0.003%
81	8.840	2563	2566	2567	rBV2	170	102	0.01%	0.001%
82	8.898	2580	2584	2586	rBV	397	343	0.03%	0.004%
83	9.091	2630	2644	2663	rBV	535752	883473	78.57%	9.907%
84	9.381	2728	2734	2739	rVB4	1052	1199	0.11%	0.013%
85	9.467	2758	2761	2764	rBV	664	334	0.03%	0.004%
86	9.599	2799	2802	2804	rBV2	260	172	0.02%	0.002%
87	9.824	2870	2872	2873	rBV2	258	114	0.01%	0.001%
88	10.011	2927	2930	2935	rBV2	285	312	0.03%	0.003%
89	10.165	2975	2978	2979	rBV2	575	277	0.02%	0.003%
90	10.239	2996	3001	3003	rBV2	504	421	0.04%	0.005%
91	10.339	3030	3032	3034	rBV	290	165	0.01%	0.002%
92	10.435	3050	3062	3083	rVB	350724	558183	49.64%	6.259%
93	10.683	3137	3139	3141	rBV	263	142	0.01%	0.002%
94	10.712	3146	3148	3150	rBV3	456	158	0.01%	0.002%
95	10.930	3214	3216	3220	rBV2	277	244	0.02%	0.003%
96	11.098	3266	3268	3271	rBV3	461	259	0.02%	0.003%
97	11.487	3376	3389	3410	rBV	514711	814752	72.46%	9.136%
98	11.863	3494	3506	3531	rVB	509802	817454	72.70%	9.167%
99	12.403	3672	3674	3677	rVB	419	161	0.01%	0.002%
100	12.934	3836	3839	3842	rBV2	631	451	0.04%	0.005%


Sum of corrected areas: 8917697

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU072018\
Data File : VU025549.D
Acq On : 20 Jul 2018 18:07
Operator : MD/SY
Sample : J4039-16
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB1S4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

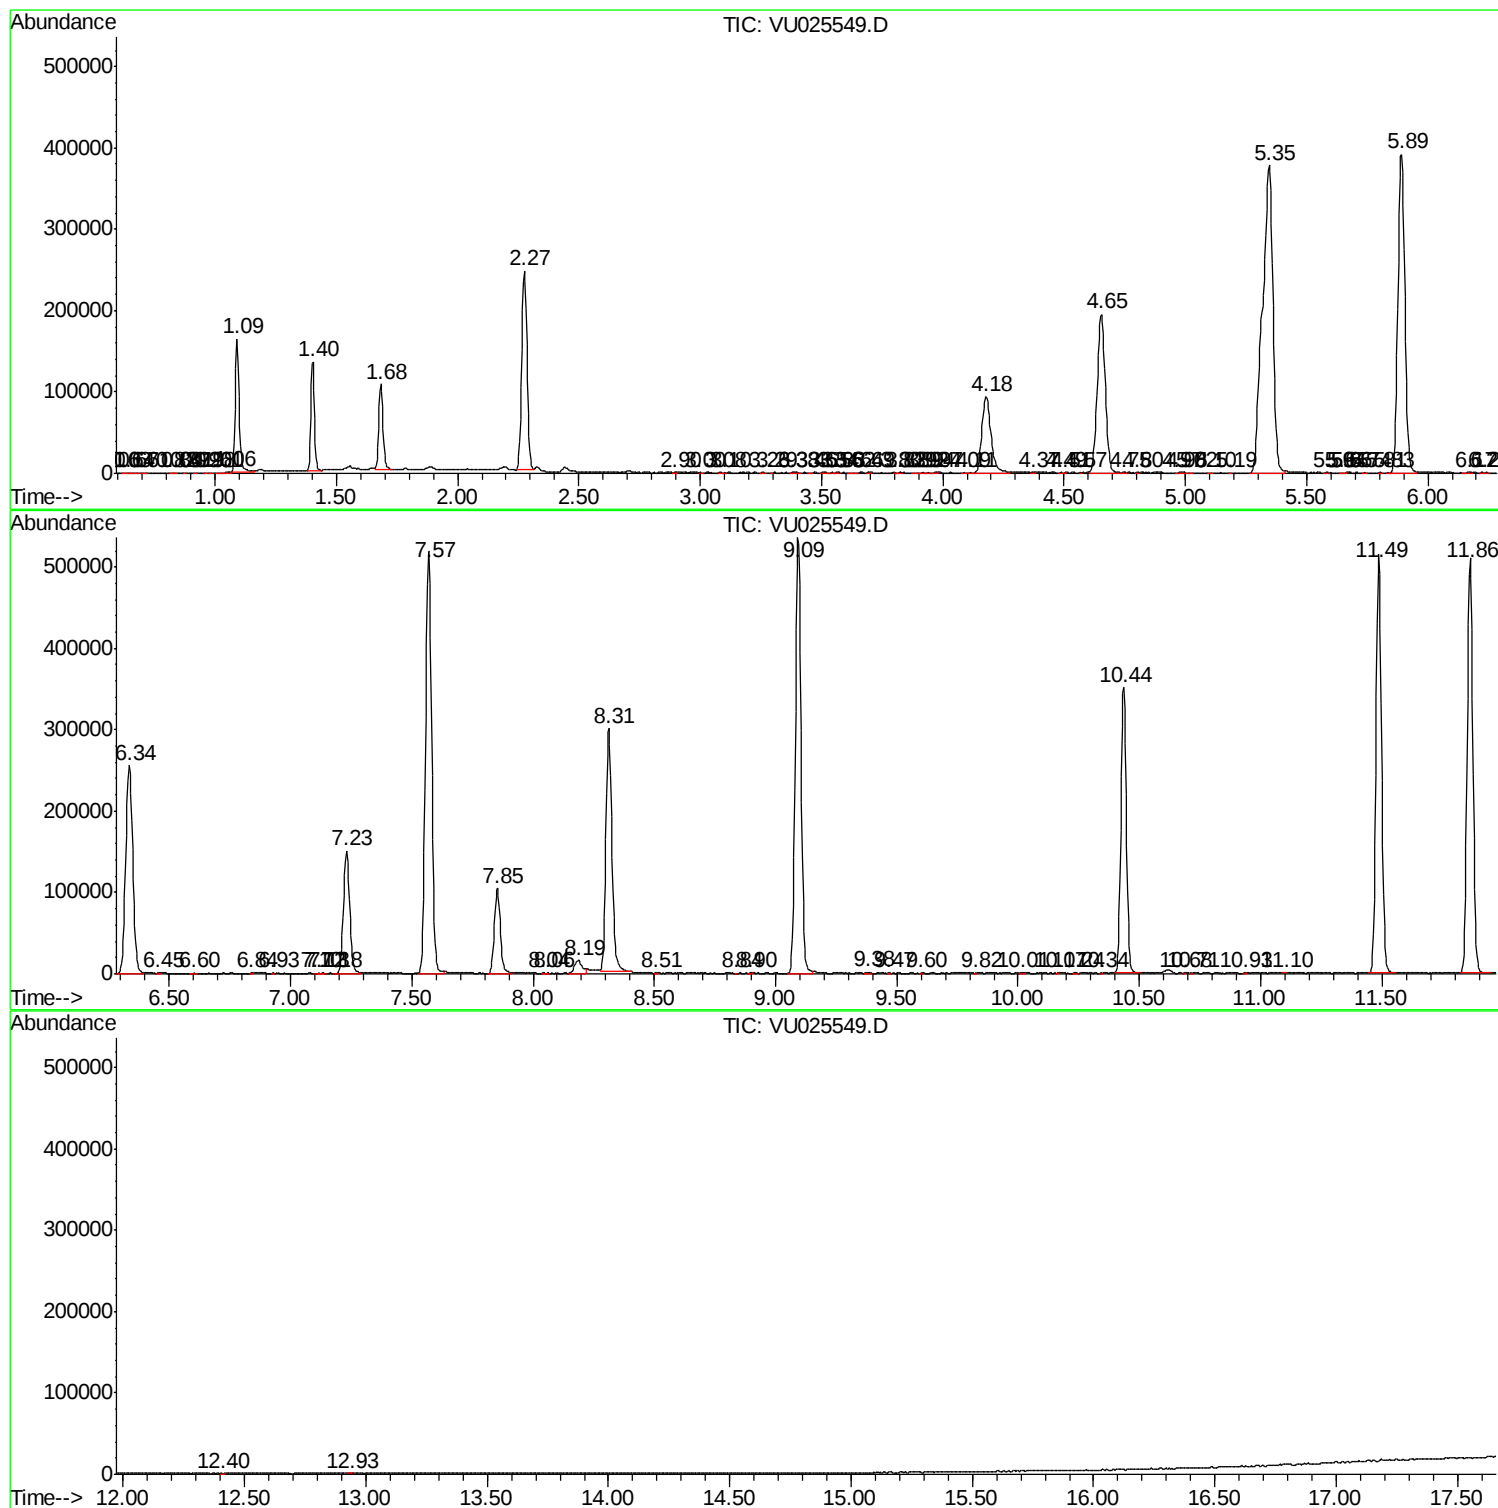

Data_Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU072018\
Data_File : VU025549.D
Acq_On : 20 Jul 2018 18:077
Operator : MD/SYY
Sample : J4039-166
Misc : 5.0mL/MSVOA_U/WATER
ALS_Vial : 23 Sample_Multiplier: 11

Instrument :
MSVOA_U
ClientSampleId :
DB1S4

Quant_Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.MM
Quant_Title : VOC_Analysis

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
