

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072018\
 Data File : VU025565.D
 Acq On : 21 Jul 2018 00:18
 Operator : MD/SY
 Sample : J4097-18
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AB5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.654	17	20	22	rBV	215	79	0.01%	0.001%
2	0.667	22	24	25	rBV	152	70	0.01%	0.001%
3	0.680	25	28	30	rBV	216	148	0.01%	0.002%
4	0.757	49	52	54	rBV2	215	130	0.01%	0.001%
5	0.863	81	85	89	rBV2	302	361	0.03%	0.004%
6	0.886	89	92	94	rVB2	291	171	0.02%	0.002%
7	0.915	99	101	104	rVV2	344	192	0.02%	0.002%
8	0.937	106	108	111	rVB2	195	71	0.01%	0.001%
9	0.960	112	115	117	rBV2	171	105	0.01%	0.001%
10	1.088	138	155	177	rBV	967903	1084673	100.00%	11.443%
11	1.403	246	253	268	rVB	124996	130230	12.01%	1.374%
12	1.683	333	340	354	rVB	98218	123751	11.41%	1.306%
13	2.275	515	524	539	rVB	225293	341016	31.44%	3.598%
14	2.609	625	628	630	rBV3	872	524	0.05%	0.006%
15	2.950	732	734	735	rBV	323	155	0.01%	0.002%
16	3.001	736	750	766	rVB	55997	121986	11.25%	1.287%
17	3.117	783	786	788	rBV	638	426	0.04%	0.004%
18	3.313	844	847	848	rBV	361	187	0.02%	0.002%
19	3.561	919	924	929	rVB3	448	502	0.05%	0.005%
20	3.603	934	937	938	rBV3	320	172	0.02%	0.002%
21	3.664	954	956	959	rBV	399	260	0.02%	0.003%
22	3.831	1006	1008	1009	rBV	263	104	0.01%	0.001%
23	3.876	1017	1022	1024	rBV3	364	264	0.02%	0.003%
24	4.075	1081	1084	1087	rBV3	282	225	0.02%	0.002%
25	4.178	1099	1116	1142	rBV	87895	229889	21.19%	2.425%
26	4.590	1241	1244	1246	rBV2	462	296	0.03%	0.003%
27	4.654	1246	1264	1287	rVV	184004	429699	39.62%	4.533%
28	4.776	1300	1302	1309	rVB2	661	614	0.06%	0.006%
29	4.866	1325	1330	1333	rBV5	716	646	0.06%	0.007%
30	4.982	1364	1366	1369	rBV2	341	219	0.02%	0.002%
31	5.043	1381	1385	1389	rBV3	486	426	0.04%	0.004%
32	5.140	1412	1415	1416	rBV	167	114	0.01%	0.001%
33	5.188	1425	1430	1433	rBV	360	414	0.04%	0.004%
34	5.233	1438	1444	1447	rBV2	404	395	0.04%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072018\
 Data File : VU025565.D
 Acq On : 21 Jul 2018 00:18
 Operator : MD/SY
 Sample : J4097-18
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AB5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

35	5.345	1454	1479	1505	rBV2	359255	1071855	98.82%	11.308%
36	5.577	1547	1551	1555	rBV	328	285	0.03%	0.003%
37	5.705	1589	1591	1593	rVB2	147	57	0.01%	0.001%
38	5.734	1597	1600	1603	rBV2	291	234	0.02%	0.002%
39	5.892	1634	1649	1667	rBV	372411	724388	66.78%	7.642%
40	6.069	1701	1704	1706	rBV2	280	164	0.02%	0.002%
41	6.172	1733	1736	1738	rBV3	457	305	0.03%	0.003%
42	6.210	1745	1748	1750	rBV3	277	191	0.02%	0.002%
43	6.278	1766	1769	1771	rBV	232	118	0.01%	0.001%
44	6.336	1771	1787	1806	rBV	245281	488726	45.06%	5.156%
45	6.435	1815	1818	1821	rBV2	463	266	0.02%	0.003%
46	6.574	1858	1861	1864	rBV	220	129	0.01%	0.001%
47	6.850	1944	1947	1949	rBV3	547	419	0.04%	0.004%
48	6.976	1984	1986	1990	rBV	216	113	0.01%	0.001%
49	7.230	2053	2065	2084	rBV	136433	241941	22.31%	2.553%
50	7.426	2122	2126	2129	rBV2	307	294	0.03%	0.003%
51	7.461	2136	2137	2140	rBV2	296	149	0.01%	0.002%
52	7.509	2150	2152	2153	rBV	472	204	0.02%	0.002%
53	7.570	2157	2171	2194	rBV	491115	852655	78.61%	8.996%
54	7.853	2247	2259	2278	rBV	95601	163578	15.08%	1.726%
55	7.988	2298	2301	2302	rBV	391	197	0.02%	0.002%
56	8.104	2334	2337	2341	rBV	330	252	0.02%	0.003%
57	8.184	2352	2362	2374	rBV3	11992	27088	2.50%	0.286%
58	8.313	2391	2402	2426	rVB	289914	495631	45.69%	5.229%
59	9.091	2632	2644	2667	rBV	507706	848461	78.22%	8.951%
60	9.548	2783	2786	2787	rBV	304	143	0.01%	0.002%
61	9.609	2802	2805	2809	rVB	577	389	0.04%	0.004%
62	9.686	2827	2829	2832	rBV	191	116	0.01%	0.001%
63	10.136	2967	2969	2972	rBV2	227	144	0.01%	0.002%
64	10.435	3050	3062	3080	rVB	337116	536247	49.44%	5.657%
65	10.612	3108	3117	3130	rVB3	9351	16822	1.55%	0.177%
66	11.078	3259	3262	3263	rBV2	432	248	0.02%	0.003%
67	11.487	3377	3389	3406	rBV	488481	764693	70.50%	8.068%
68	11.863	3494	3506	3526	rVB	485784	773502	71.31%	8.161%


Sum of corrected areas: 9478518

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU072018\
Data File : VU025565.D
Acq On : 21 Jul 2018 00:18
Operator : MD/SY
Sample : J4097-18
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AB5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

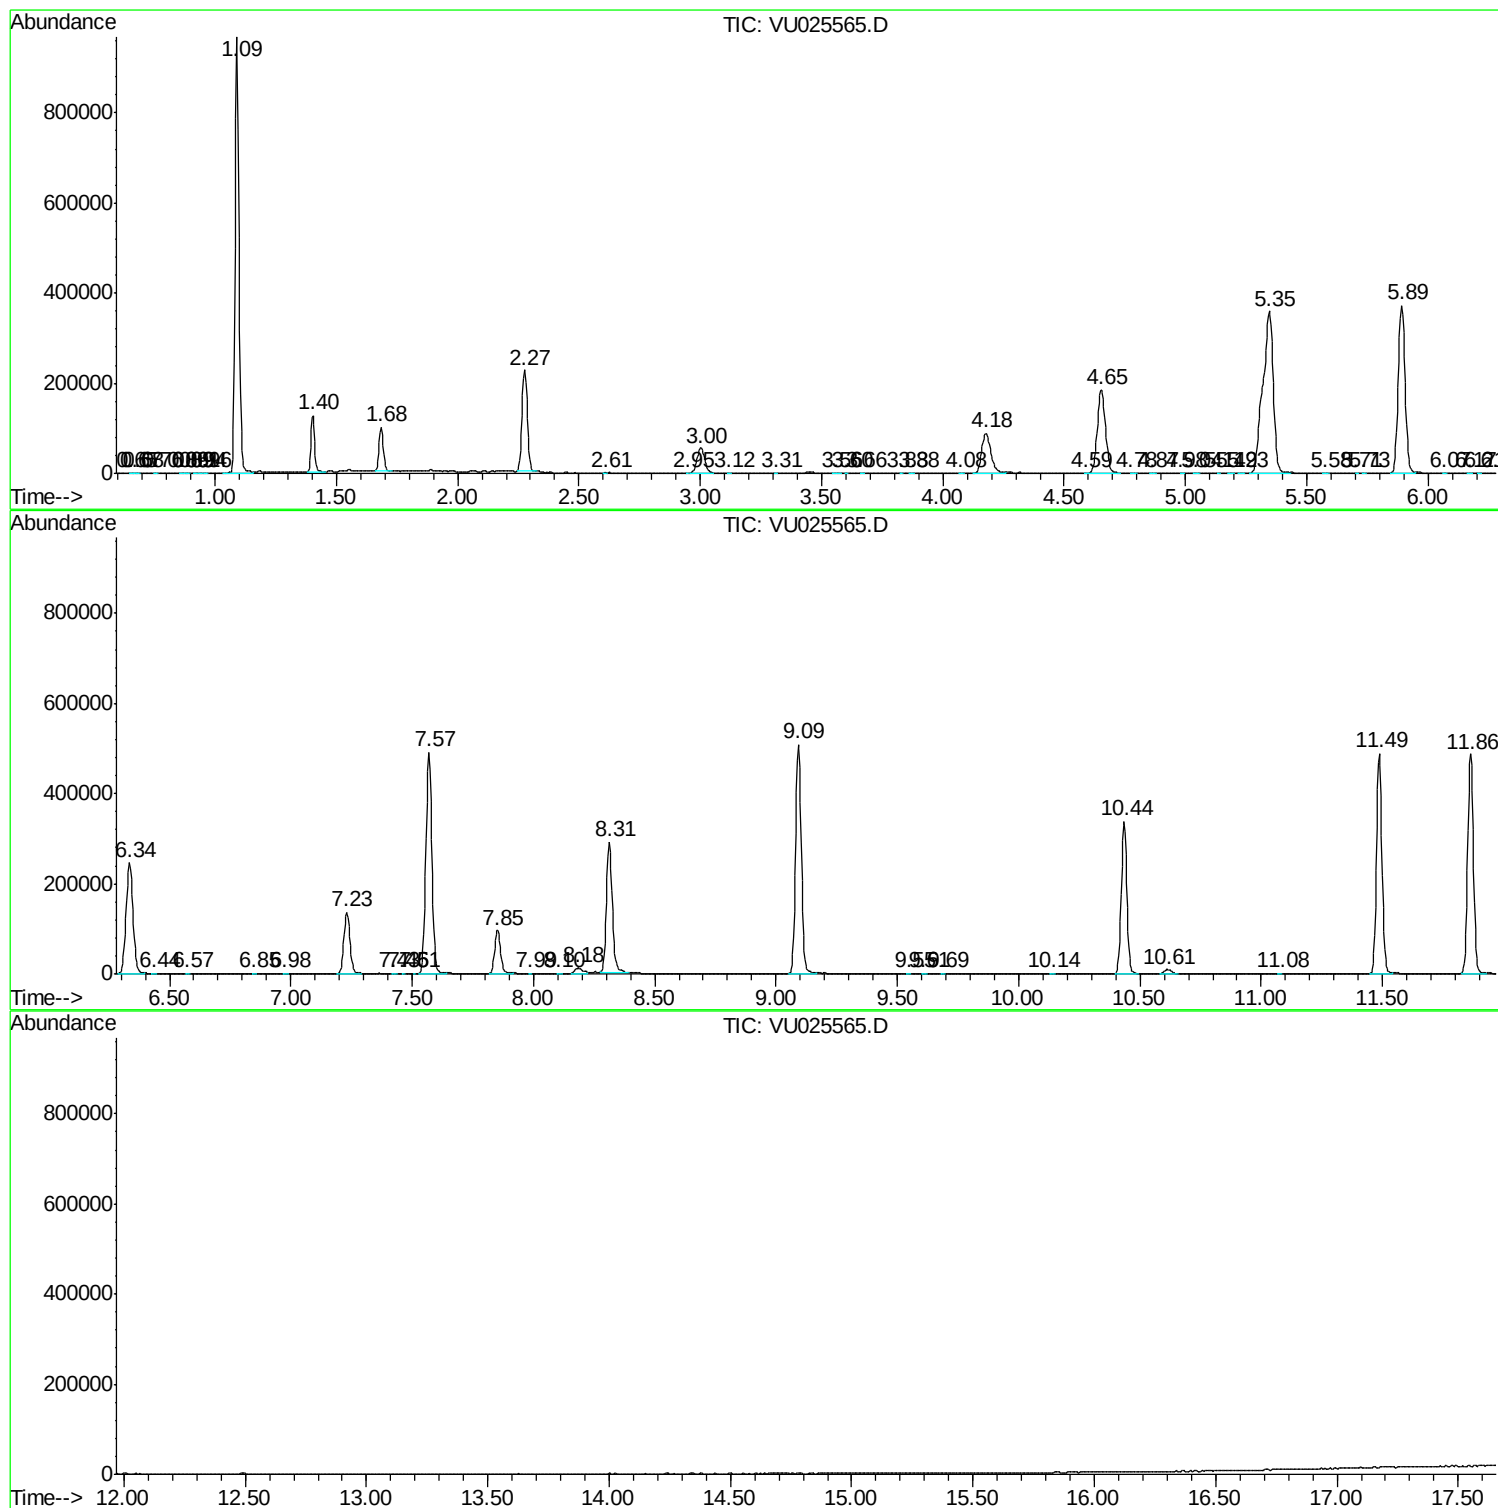

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU072018\
Data File : VU025565.D
Acq On : 21 Jul 2018 00:18
Operator : MD/SY
Sample : J4097-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AB5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU072018\
Data File : VU025565.D
Acq On : 21 Jul 2018 00:18
Operator : MD/SY
Sample : J4097-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AB5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc