


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072018\
 Data File : VU025527.D
 Acq On : 20 Jul 2018 07:56
 Operator : MD/SY
 Sample : BFB46
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB46

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis
 Last Update : Tue Jul 24 02:07:37 2018

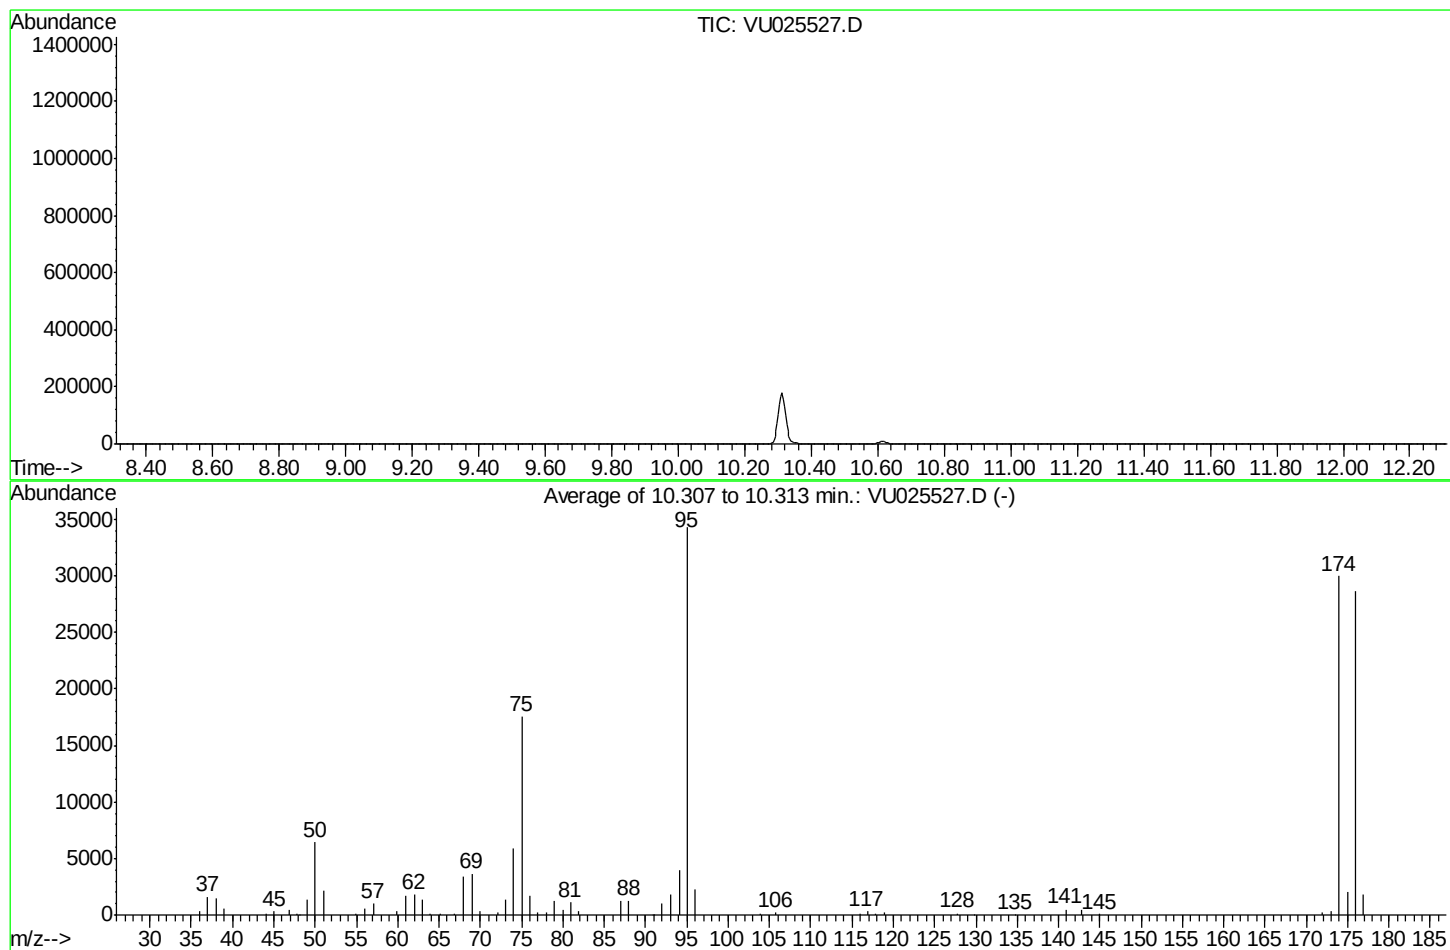

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3010

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	6419	PASS
75	95	30	80	51.2	17541	PASS
95	95	100	100	100.0	34282	PASS
96	95	5	9	6.7	2288	PASS
173	174	0.00	2	1.3	383	PASS
174	95	50	120	87.4	29957	PASS
175	174	5	9	6.9	2068	PASS
176	174	95	101	95.4	28589	PASS
177	176	5	9	6.3	1797	PASS

m/z	Abundance
44.00	432.0
207.00	419.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
35.90	240.0
37.00	1586.0
38.00	1431.0
38.90	607.0
44.00	510.0
45.10	312.0
46.90	494.0
47.80	209.0
49.00	1331.0
50.00	6321.0
51.00	2039.0
54.90	101.0
56.10	569.0
57.00	964.0
59.90	267.0
61.00	1666.0
62.00	1771.0
63.00	1432.0
65.10	199.0
68.00	3268.0
69.00	3452.0
69.90	295.0
72.00	197.0
73.00	1302.0
74.00	5808.0
75.00	16736.0
76.00	1677.0
77.00	208.0
78.00	215.0
78.90	1113.0
79.90	344.0
80.90	1152.0
81.90	253.0
87.00	1209.0
88.00	1249.0
90.80	104.0
92.00	979.0
93.00	1821.0
94.00	3793.0
95.00	33456.0
96.00	2294.0
103.90	188.0
105.80	170.0
116.00	117.0
116.90	276.0
117.80	132.0
118.90	237.0
127.80	134.0
134.80	103.0
140.90	458.0
142.80	493.0
145.00	101.0
171.90	249.0
173.00	411.0
174.00	28504.0
175.00	2007.0
176.00	26392.0
176.90	1684.0
206.90	293.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	304.0
37.00	1670.0
38.00	1519.0
39.00	619.0
44.00	496.0
45.10	342.0
46.90	484.0
47.80	182.0
49.00	1418.0
50.00	6609.0
51.00	2230.0
54.90	102.0
56.10	577.0
57.10	1050.0
59.90	336.0
61.00	1773.0
62.00	1820.0
63.00	1458.0
63.90	133.0
65.10	166.0
66.80	106.0
68.00	3468.0
69.00	3824.0
70.00	313.0
72.10	273.0
73.00	1384.0
74.00	6060.0
75.00	18088.0
76.00	1721.0
77.00	244.0
77.90	230.0
78.90	1270.0
79.90	417.0
80.90	1155.0
81.90	306.0
87.00	1252.0
88.00	1302.0
92.00	989.0
93.00	1941.0
94.00	4053.0
95.00	35264.0
96.00	2334.0
103.90	149.0
105.80	200.0
116.00	157.0
116.90	327.0
117.90	126.0
118.90	277.0
127.80	181.0
140.90	549.0
142.80	529.0
145.00	120.0
171.90	269.0
173.00	384.0
174.00	30832.0
175.00	2117.0
176.00	29568.0
176.90	1835.0
207.00	271.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	341.0
37.00	1587.0
38.10	1481.0
39.00	597.0
44.00	494.0
45.00	341.0
46.90	369.0
48.10	159.0
49.00	1391.0
50.00	6328.0
51.00	2053.0
54.80	110.0
56.00	518.0
57.10	1023.0
59.90	380.0
61.00	1729.0
62.00	1786.0
63.00	1351.0
63.90	210.0
65.10	107.0
66.80	118.0
68.00	3458.0
69.00	3679.0
70.00	297.0
72.10	276.0
73.00	1380.0
74.00	5693.0
75.00	17800.0
76.00	1570.0
77.00	255.0
77.90	249.0
78.90	1266.0
80.00	449.0
80.90	1082.0
81.90	347.0
87.00	1166.0
88.00	1271.0
91.00	107.0
92.00	1015.0
93.00	1745.0
94.10	3955.0
95.00	34128.0
96.00	2238.0
103.90	137.0
105.80	219.0
115.90	161.0
116.90	362.0
117.90	151.0
118.90	245.0
127.80	187.0
129.80	117.0
140.90	510.0
142.80	478.0
145.00	101.0
172.00	284.0
173.00	354.0
174.00	30536.0
175.00	2080.0
176.00	29808.0
177.00	1874.0
207.00	277.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46