


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072018\
 Data File : VU025534.D
 Acq On : 20 Jul 2018 12:01
 Operator : MD/SY
 Sample : VSTDCCC050
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 LabSampleId :
 VSTD05059

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis
 Last Update : Mon Jul 23 14:36:22 2018

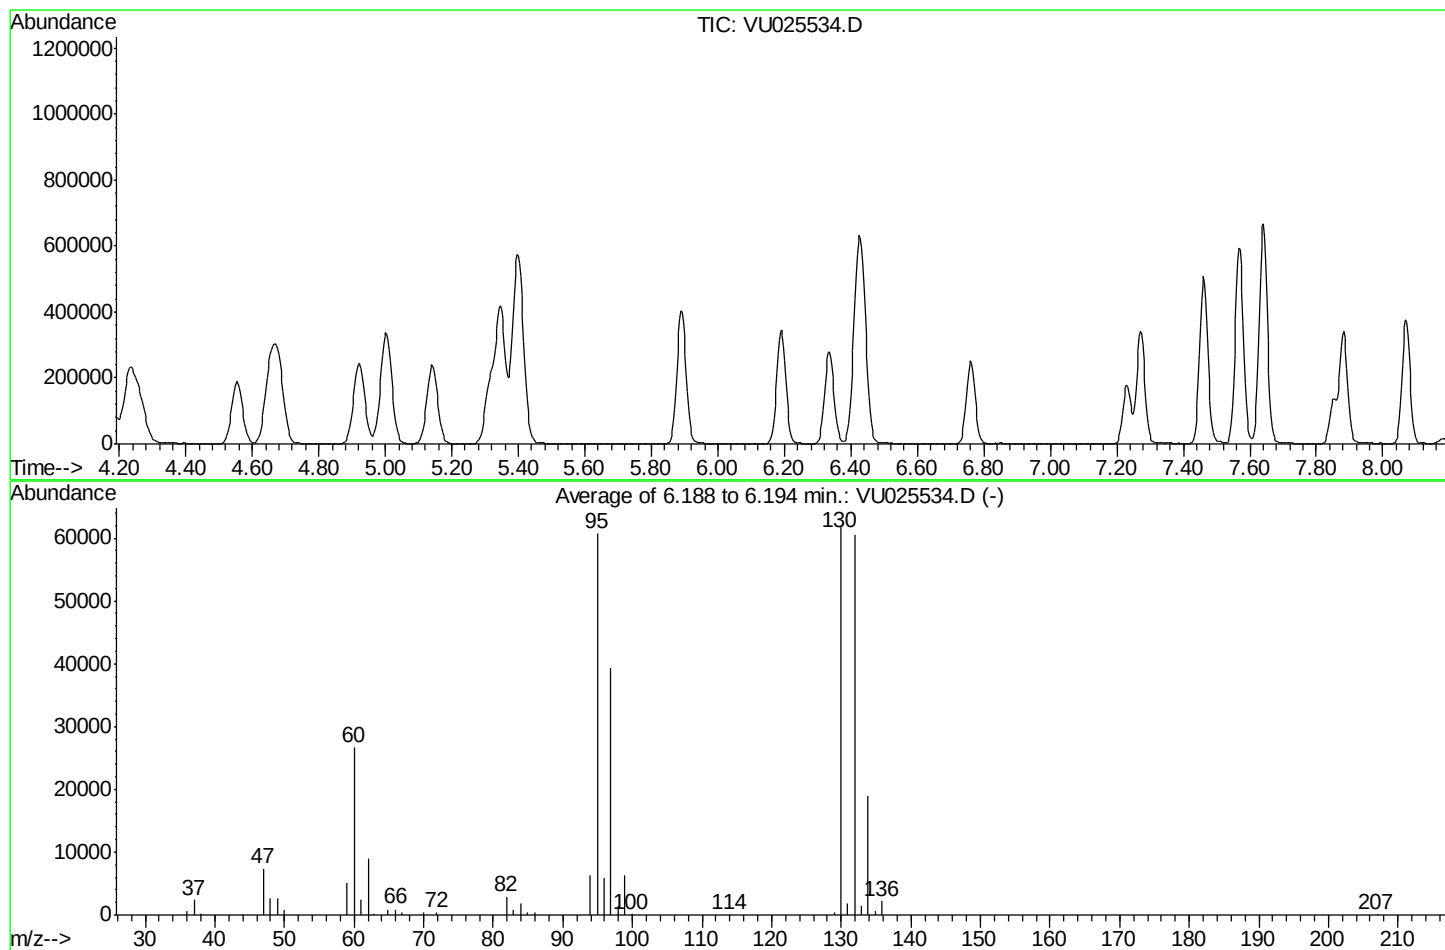

AutoFind: Scans 1741, 1742, 1743; Background Corrected with Scan 1727

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	1.5	923	FAIL*
75	95	30	80	0.0	0	FAIL*
95	95	100	100	100.0	60680	PASS
96	95	5	9	9.7	5901	FAIL*
173	174	COMPARISON MASS IS NOT PRESENT!!!				
174	95	50	120	0.0	0	FAIL*
175	174	COMPARISON MASS IS NOT PRESENT!!!				
176	174	COMPARISON MASS IS NOT PRESENT!!!				
177	176	COMPARISON MASS IS NOT PRESENT!!!				