

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072019\
 Data File : VU033356.D
 Acq On : 20 Jul 2019 02:44
 Operator : JC/SP
 Sample : K3890-09
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A52J4

Quant Time: Jul 20 06:01:40 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR071619WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jul 20 05:21:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	101038	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	107527	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.47	152	44983	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	41482	4.08	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.60%
7) Chloroethane-d5	1.67	69	39571	4.67	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.40%
11) 1,1-Dichloroethene-d2	2.26	63	69392	3.53	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.60%
20) 2-Butanone-d5	4.17	46	109801	57.26	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.52%
24) Chloroform-d	4.62	84	70070	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.40%
26) 1,2-Dichloroethane-d4	5.29	65	41931	5.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.40%
32) Benzene-d6	5.32	84	132059	4.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.20%
36) 1,2-Dichloropropane-d6	6.31	67	45820	4.81	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.20%
41) Toluene-d8	7.55	98	108024	3.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.20%
43) trans-1,3-Dichloropropene-	7.83	79	16503	4.32	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.40%
46) 2-Hexanone-d5	8.30	63	83214	53.06	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	106.12%
57) 1,1,2,2-Tetrachloroethane-	10.41	84	40815	5.16	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.20%
64) 1,2-Dichlorobenzene-d4	11.85	152	43382	4.95	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.00%


Target Compounds					Ovalue
13) Acetone	2.31	43	10694	6.370 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072019\
Data File : VU033356.D
Acq On : 20 Jul 2019 02:44
Operator : JC/SP
Sample : K3890-09
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A52J4

Quant Time: Jul 20 06:01:40 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR071619WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jul 20 05:21:55 2019
Response via : Initial Calibration

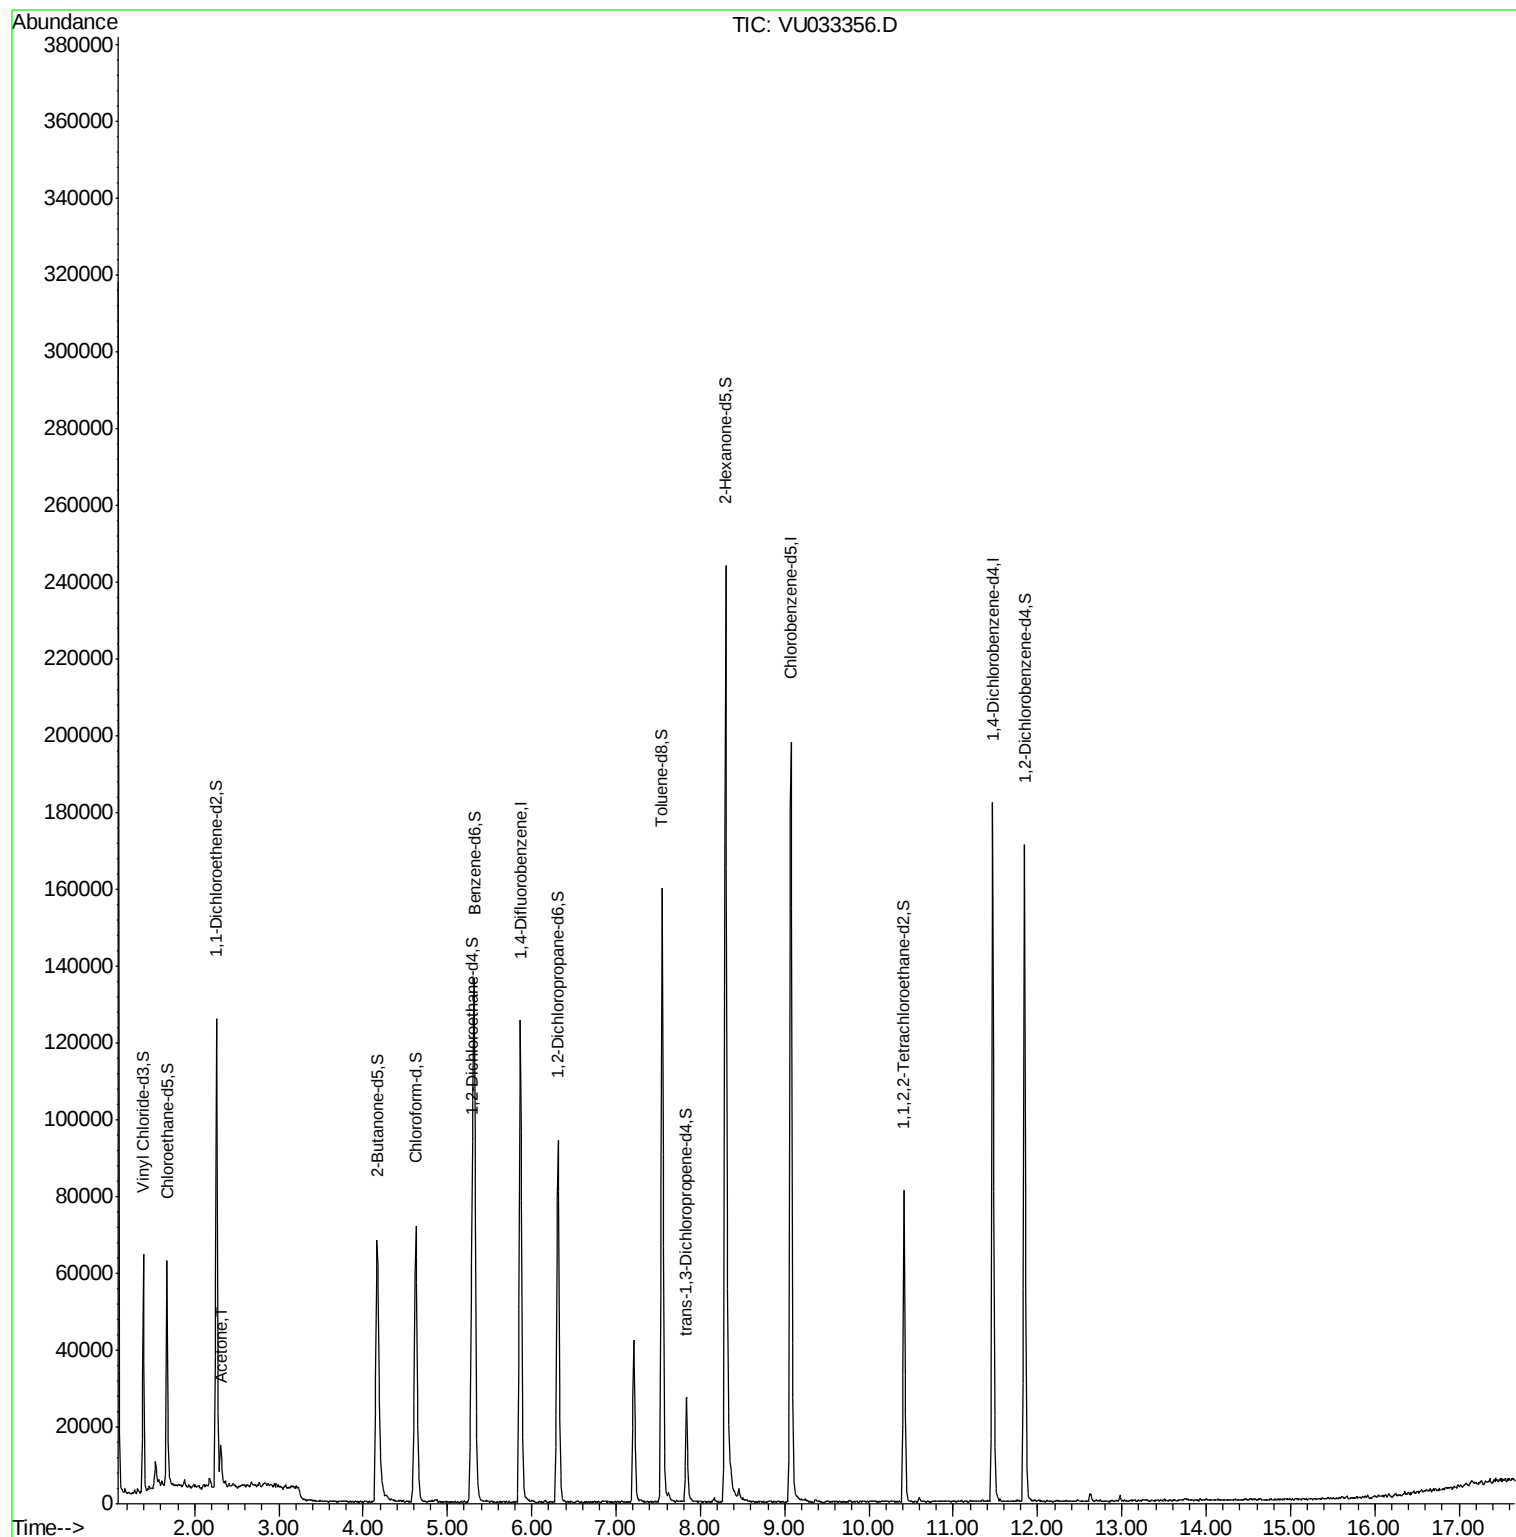

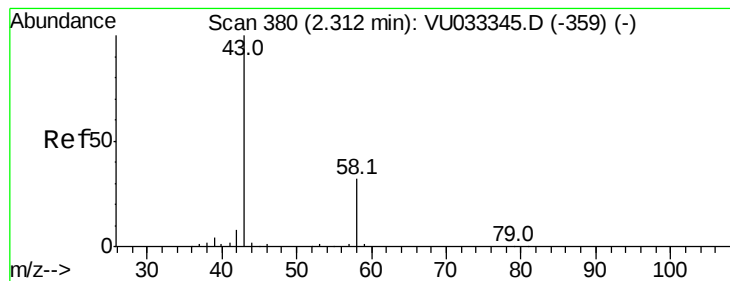

#13

Acetone

Concen: 6.370 ug/L

RT: 2.31 min Scan# 379

Delta R.T. -0.00 min

Lab File: VU033356.D

Acq: 20 Jul 2019 02:44

Instrument :

MSVOA_U

ClientSampleId :

A52J4

Tot Ion: 43 Resp: 10694

Ion Ratio Lower Upper

43 100

58 33.7 0.0 66.6

