

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072019\
 Data File : VU033357.D
 Acq On : 20 Jul 2019 03:09
 Operator : JC/SP
 Sample : K3890-10
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A52Q6

Quant Time: Jul 20 06:04:03 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR071619WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jul 20 05:21:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	101114	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	104463	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.47	152	44145	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	40727	4.00	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.00%
7) Chloroethane-d5	1.67	69	39186	4.62	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.40%
11) 1,1-Dichloroethene-d2	2.26	63	66780	3.39	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.80%
20) 2-Butanone-d5	4.17	46	96224	50.15	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.30%
24) Chloroform-d	4.62	84	63534	4.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.60%
26) 1,2-Dichloroethane-d4	5.29	65	41297	5.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.80%
32) Benzene-d6	5.32	84	131079	4.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.20%
36) 1,2-Dichloropropane-d6	6.31	67	45095	4.87	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.40%
41) Toluene-d8	7.55	98	106503	3.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.40%
43) trans-1,3-Dichloropropene-	7.83	79	15681	4.23	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.60%
46) 2-Hexanone-d5	8.30	63	77542	50.89	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.78%
57) 1,1,2,2-Tetrachloroethane-	10.42	84	40064	5.21	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.20%
64) 1,2-Dichlorobenzene-d4	11.85	152	41533	4.83	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.60%


Target Compounds					Ovalue
13) Acetone	2.31	43	9138	5.439 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU072019\
Data File : VU033357.D
Acq On : 20 Jul 2019 03:09
Operator : JC/SP
Sample : K3890-10
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A52Q6

Quant Time: Jul 20 06:04:03 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR071619WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jul 20 05:21:55 2019
Response via : Initial Calibration

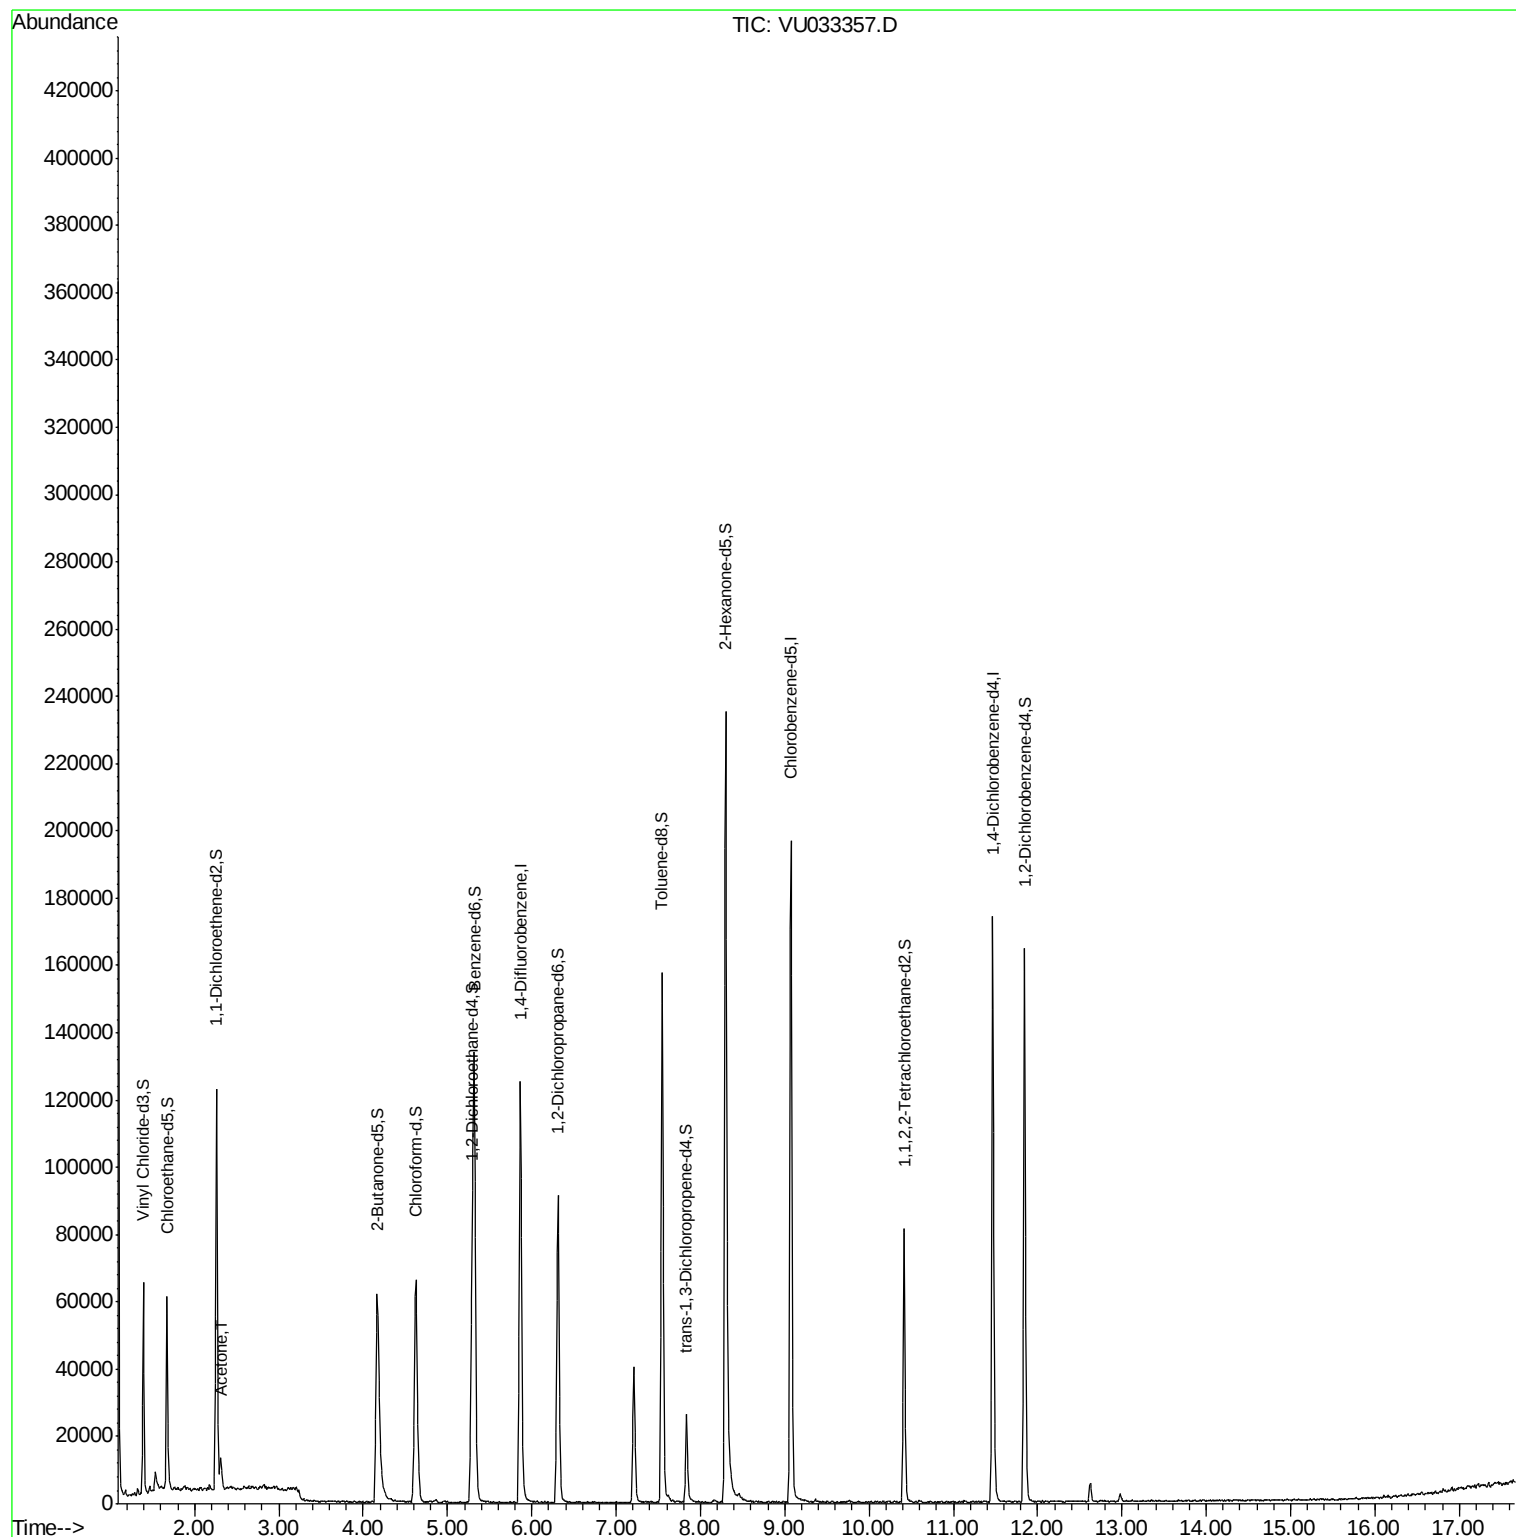

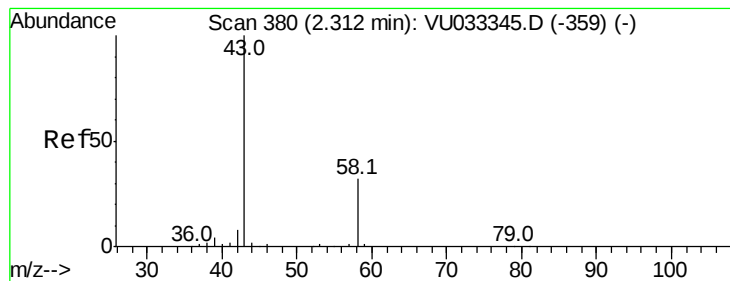

#13

Acetone

Concen: 5.439 ug/L

RT: 2.31 min Scan# 379

Delta R.T. -0.00 min

Lab File: VU033357.D

Acq: 20 Jul 2019 03:09

Instrument :

MSVOA_U

ClientSampleId :

A52Q6

Tot Ion: 43 Resp: 9138

Ion Ratio Lower Upper

43 100

58 29.0 0.0 66.6

