


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU072019\
 Data File : VU033344.D
 Acq On : 19 Jul 2019 21:04
 Operator : JC/SP
 Sample : BFB27
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB27

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR071619WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Jul 18 08:01:21 2019

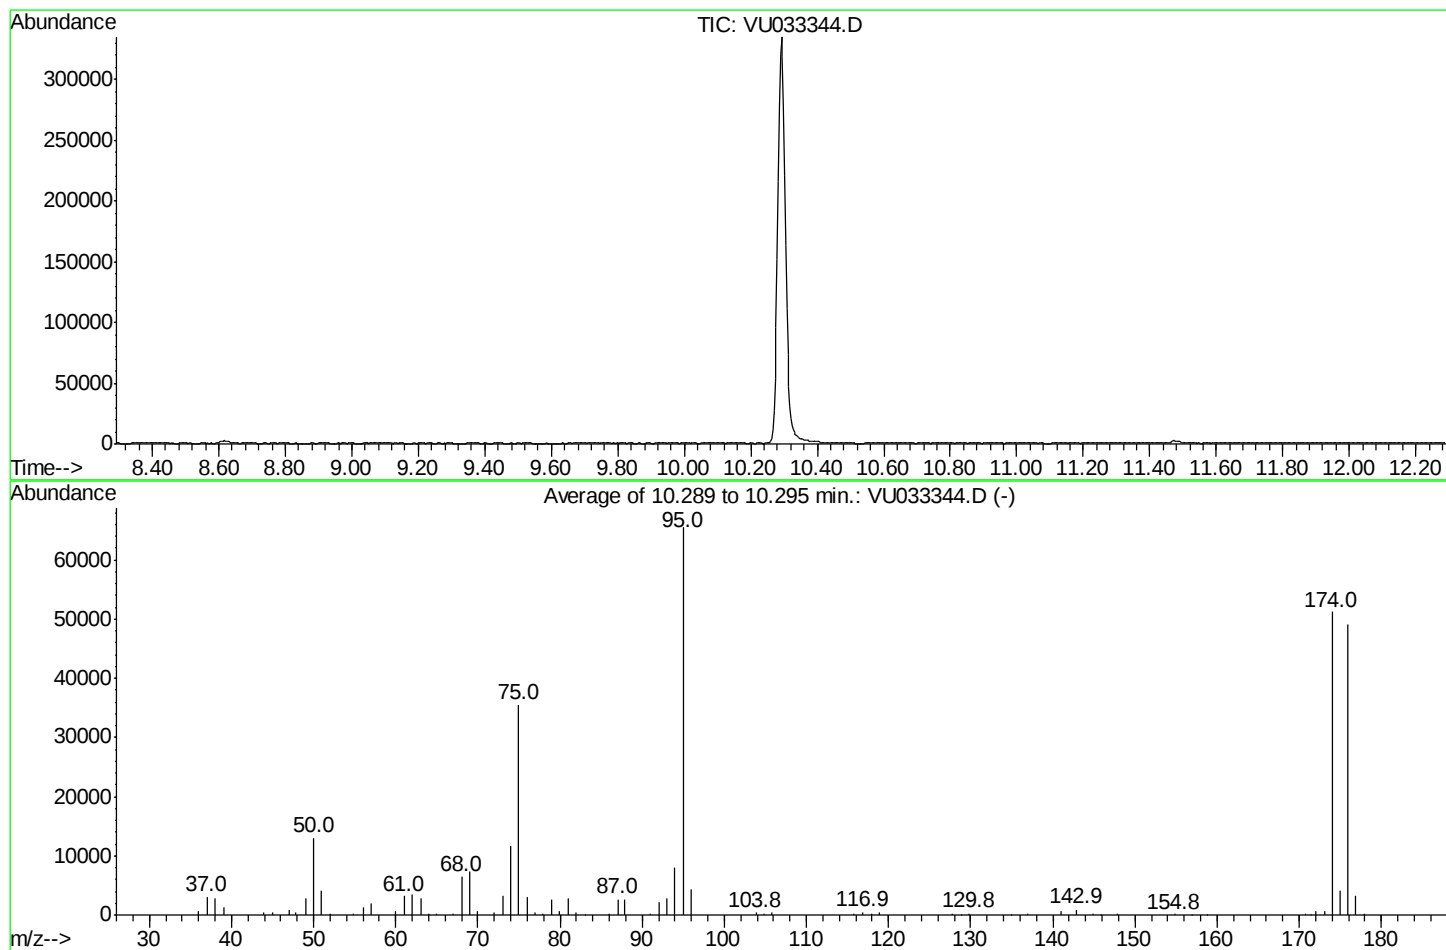

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2849

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	13072	PASS
75	95	30	80	54.2	35501	PASS
95	95	100	100	100.0	65490	PASS
96	95	5	9	6.7	4363	PASS
173	174	0.00	2	1.3	659	PASS
174	95	50	120	78.2	51200	PASS
175	174	5	9	8.2	4195	PASS
176	174	95	101	96.0	49160	PASS
177	176	5	9	6.7	3273	PASS

Scan 2849 (10.250 min): VU033344.D
BFB27

m/z	Abundance
40.00	252.0
43.90	455.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

m/z	Abundance
36.00	626.0
37.00	3053.0
38.00	2716.0
39.10	1348.0
40.00	240.0
44.00	878.0
45.00	592.0
47.00	844.0
47.80	360.0
49.00	2847.0
50.00	13113.0
51.00	4283.0
52.00	190.0
54.80	177.0
56.00	1289.0
57.00	1997.0
60.00	671.0
61.00	3249.0
62.00	3481.0
63.00	2718.0
64.00	325.0
65.00	324.0
67.00	191.0
68.00	6397.0
69.00	7315.0
70.00	571.0
72.00	383.0
73.00	3496.0
74.00	12060.0
75.00	35312.0
76.00	3166.0
77.00	400.0
77.90	256.0
78.90	2813.0
79.90	752.0
81.00	2812.0
81.90	590.0
86.00	140.0
87.00	2624.0
87.90	2401.0
90.90	274.0
92.00	2187.0
93.00	2675.0
94.00	7825.0
95.00	65272.0
96.00	4408.0
103.80	401.0
104.90	136.0
105.80	368.0
115.90	253.0
116.90	469.0
117.90	247.0
118.80	351.0
127.80	192.0
129.90	318.0
134.90	150.0
137.00	120.0
140.90	516.0
142.90	835.0
144.80	214.0
147.80	144.0
154.80	121.0
158.70	115.0
170.70	128.0
171.30	116.0
172.00	538.0
173.10	990.0
174.00	49232.0
175.00	4163.0
175.90	46840.0
176.90	3298.0
177.90	113.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

m/z	Abundance
36.00	620.0
37.00	3194.0
38.00	2966.0
39.10	1293.0
39.90	218.0
44.00	954.0
45.00	526.0
47.10	829.0
47.90	418.0
49.00	2915.0
50.00	13469.0
51.00	4230.0
52.00	226.0
54.80	175.0
56.00	1279.0
57.00	2121.0
60.00	706.0
61.00	3227.0
62.00	3558.0
63.00	2832.0
64.00	331.0
65.00	308.0
67.00	213.0
68.00	6574.0
69.00	7647.0
70.00	570.0
72.00	373.0
73.00	3463.0
74.00	12028.0
75.00	36736.0
76.00	3203.0
77.00	405.0
77.90	306.0
78.90	2786.0
79.90	766.0
80.90	2864.0
81.90	523.0
83.00	113.0
86.00	206.0
87.00	2682.0
87.90	2735.0
91.00	306.0
92.00	2348.0
93.00	2826.0
94.00	8314.0
95.00	67288.0
96.00	4521.0
103.90	427.0
104.80	126.0
105.80	340.0
115.80	235.0
116.90	456.0
117.90	293.0
118.80	394.0
127.80	227.0
128.80	134.0
129.90	314.0
134.90	141.0
136.90	148.0
140.90	604.0
142.90	873.0
144.90	202.0
145.90	109.0
147.80	142.0
154.80	183.0
156.80	118.0
158.70	119.0
170.80	148.0
171.30	103.0
172.00	608.0
173.10	988.0
174.00	52800.0
175.00	4306.0
176.00	50680.0
176.90	3327.0
177.90	117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

m/z	Abundance
36.00	554.0
37.00	3127.0
38.00	2894.0
39.00	1141.0
39.90	180.0
44.00	966.0
45.00	492.0
47.10	762.0
47.90	398.0
49.00	2806.0
50.00	12636.0
51.00	3902.0
52.00	215.0
54.90	146.0
56.00	1225.0
57.00	1920.0
60.00	594.0
61.00	3017.0
62.00	3284.0
63.10	2661.0
64.00	330.0
65.00	284.0
67.00	208.0
68.00	6248.0
69.00	7271.0
70.00	534.0
72.00	336.0
73.00	3110.0
74.00	11203.0
75.00	34456.0
76.00	2937.0
77.00	429.0
77.90	305.0
78.90	2474.0
80.00	685.0
80.90	2544.0
81.90	446.0
83.00	108.0
86.00	210.0
87.00	2629.0
87.90	2789.0
91.00	322.0
92.00	2168.0
93.00	2872.0
94.00	8020.0
95.00	63912.0
96.00	4161.0
103.80	342.0
104.80	102.0
105.90	310.0
115.70	239.0
116.90	428.0
117.90	293.0
118.80	368.0
127.80	231.0
128.80	153.0
129.80	299.0
136.90	155.0
141.00	631.0
142.90	898.0
145.00	180.0
145.90	114.0
147.80	131.0
154.90	239.0
156.90	114.0
170.90	144.0
172.00	604.0
174.00	51568.0
175.00	4116.0
176.00	49960.0
176.90	3196.0
177.90	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27