

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072021\
 Data File : VU044368.D
 Acq On : 20 Jul 2021 11:12
 Operator : SY/MD
 Sample : VU0720WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0720WBL01

Quant Time: Jul 21 01:24:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Jul 16 14:36:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.115	96	50530	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.639	95	18044	0.885	ug/l	0.00
Spiked Amount 1.000			Recovery	=	88.000%	
68) 1,2-Dichlorobenzene-d4	12.198	152	17671	0.889	ug/l	0.00
Spiked Amount 1.000			Recovery	=	89.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072021\
Data File : VU044368.D
Acq On : 20 Jul 2021 11:12
Operator : SY/MD
Sample : VU0720WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0720WBL01

Quant Time: Jul 21 01:24:47 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Jul 16 14:36:39 2021
Response via : Initial Calibration

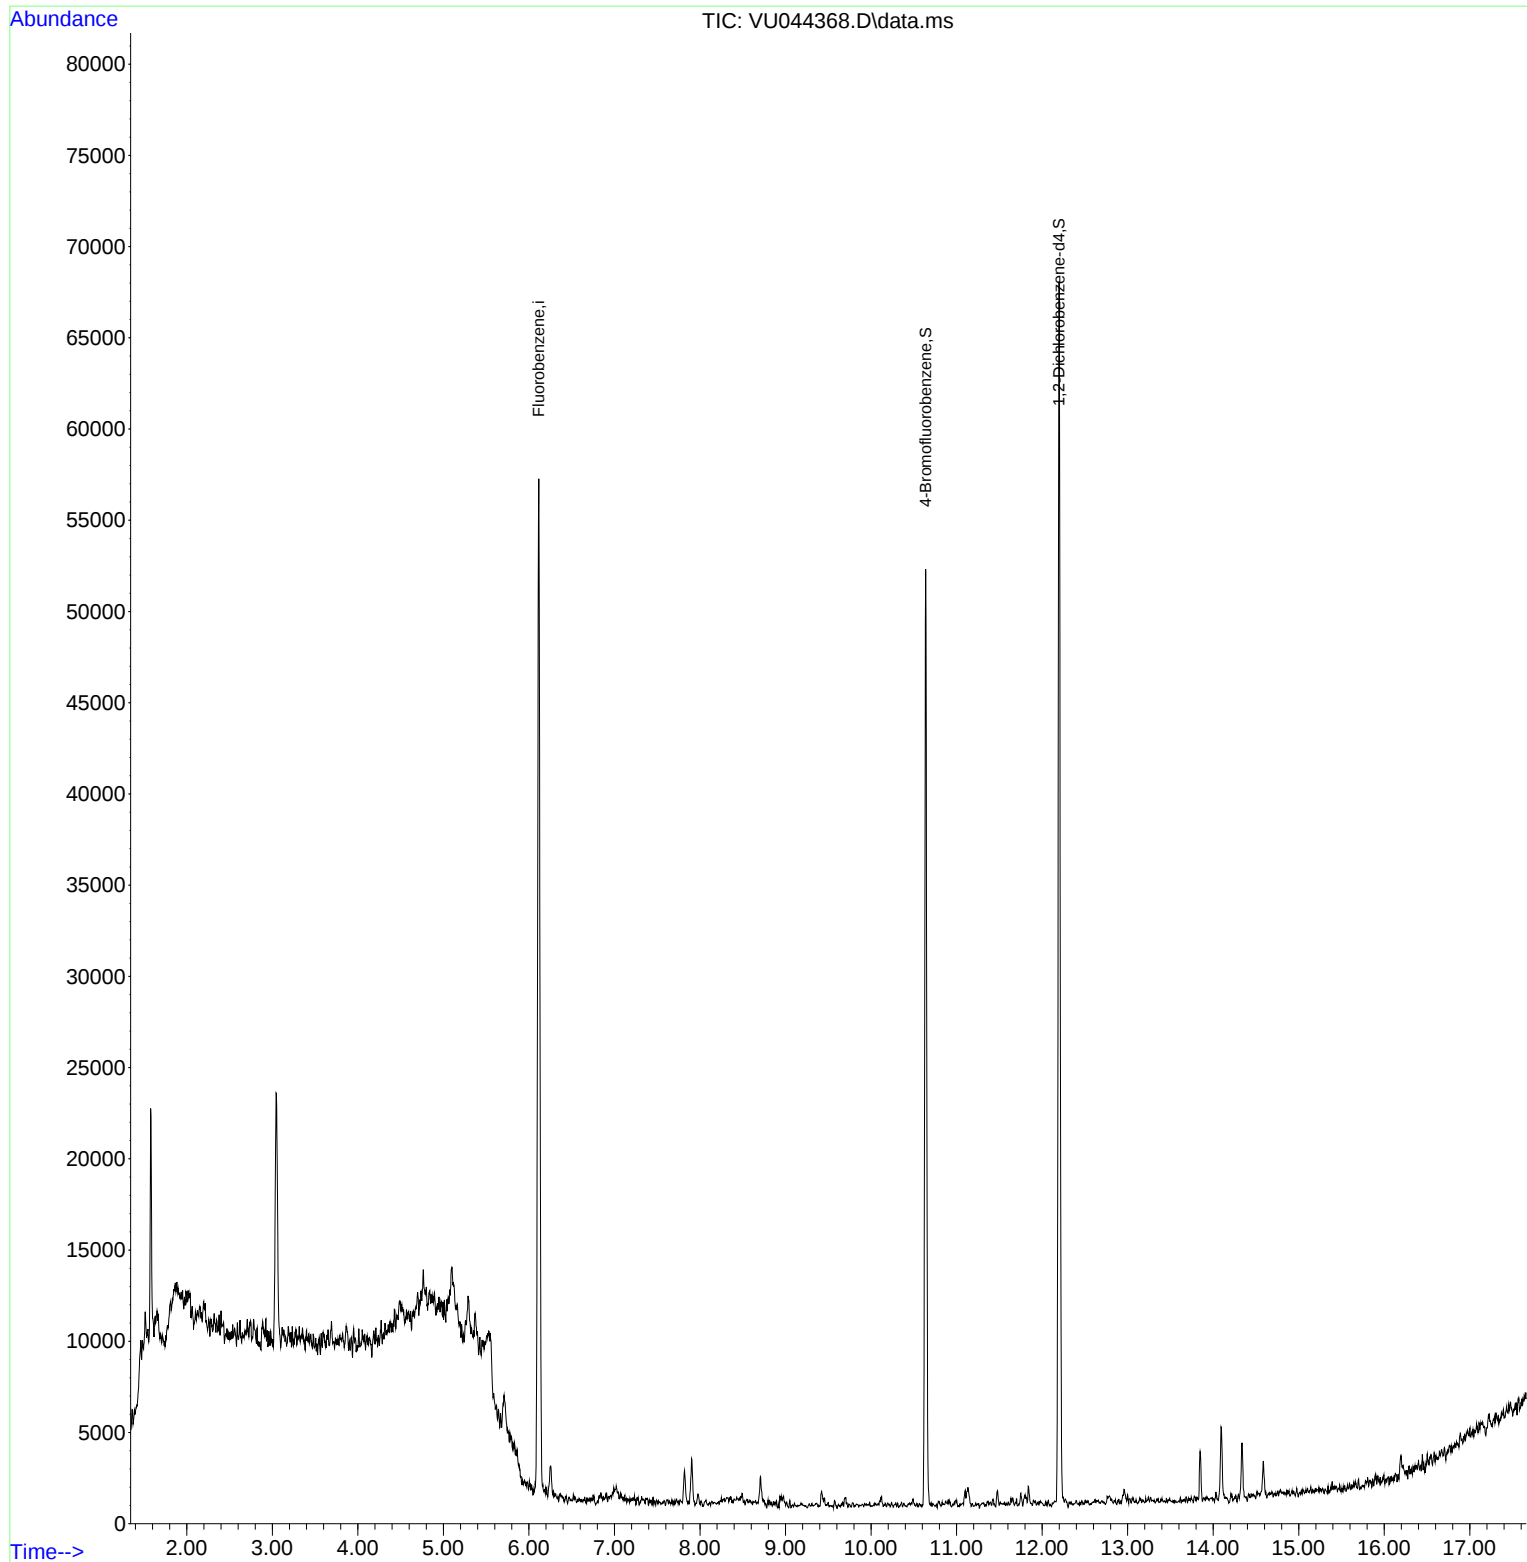




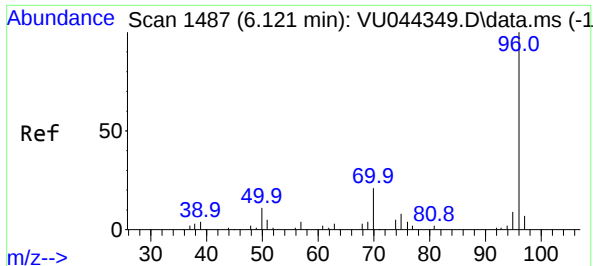


#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.115 min Scan# 1485
Delta R.T. -0.006 min
Lab File: VU044368.D
Acq: 20 Jul 2021 11:12

Instrument :
MSVOA_U
ClientSampleId :
VU0720WBL01

Tgt Ion: 96 Resp: 50530




Ion	Ratio	Lower	Upper
96	100		
70	20.6	16.2	24.2
95	9.3	7.3	10.9
97	6.7	0.0	0.0

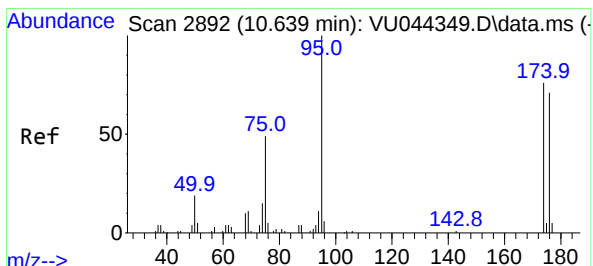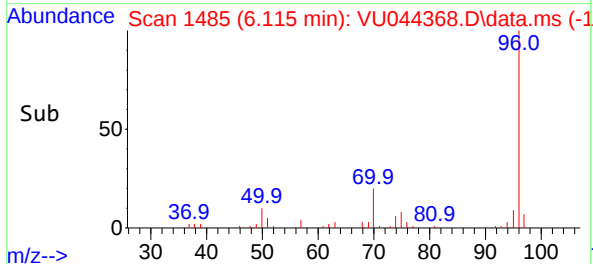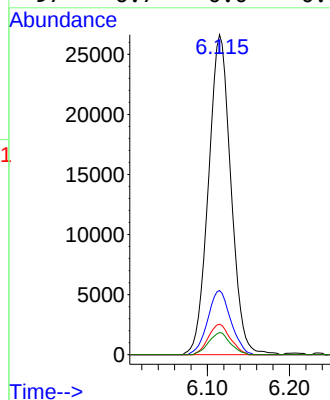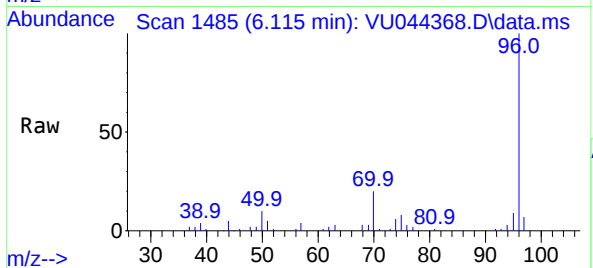


#57
4-Bromofluorobenzene
Concen: 0.885 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. -0.000 min
Lab File: VU044368.D
Acq: 20 Jul 2021 11:12

Tgt Ion: 95 Resp: 18044

Ion	Ratio	Lower	Upper
95	100		
174	73.1	62.2	93.2
176	69.9	60.3	90.5

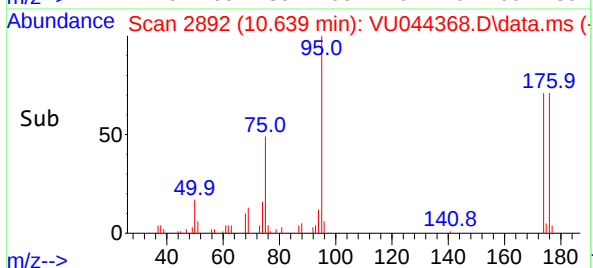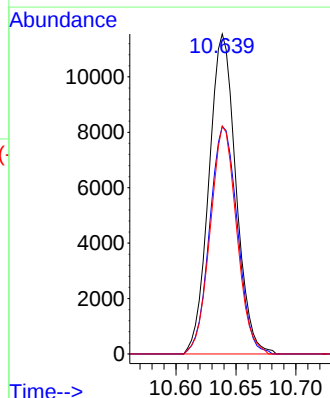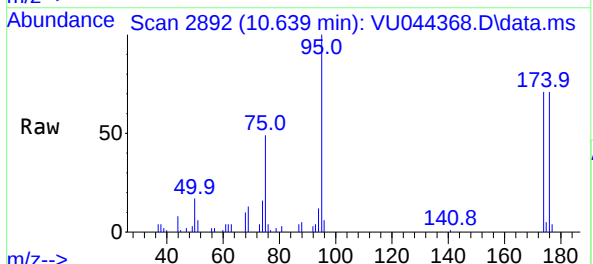

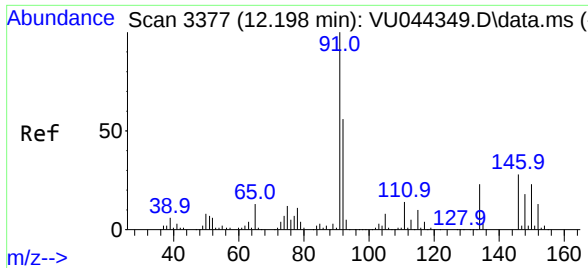

#68
1,2-Dichlorobenzene-d4
Concen: 0.889 ug/l
RT: 12.198 min Scan# 3377
Delta R.T. -0.000 min
Lab File: VU044368.D
Acq: 20 Jul 2021 11:12

Instrument :
MSVOA_U
ClientSampleId :
VU0720WBL01

Tgt Ion:152 Resp: 17671
Ion Ratio Lower Upper
152 100
115 64.4 0.0 257.0
150 152.3 0.0 630.2

