

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072021\
 Data File : VU044368.D
 Acq On : 20 Jul 2021 11:12
 Operator : SY/MD
 Sample : VU0720WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0720WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU044368.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.044	522	530	547	rVB2	13958	26963	25.46%	7.729%
2	6.115	1470	1485	1499	rBV	55387	103502	97.73%	29.669%
3	6.253	1518	1528	1535	rBV5	1688	3015	2.85%	0.864%
4	7.819	2007	2015	2026	rVB4	1805	2740	2.59%	0.785%
5	7.902	2032	2041	2050	rBV5	2473	3752	3.54%	1.076%
6	8.706	2283	2291	2299	rBV3	1459	2179	2.06%	0.625%
7	9.423	2507	2514	2520	rBV4	813	1252	1.18%	0.359%
8	10.639	2882	2892	2906	rBV	51280	78423	74.05%	22.480%
9	11.131	3043	3045	3054	rVB4	887	1094	1.03%	0.314%
10	11.478	3147	3153	3159	rBV3	894	1208	1.14%	0.346%
11	12.198	3366	3377	3391	rBV	66884	105907	100.00%	30.358%
12	13.848	3884	3890	3898	rVB3	2730	3564	3.37%	1.022%
13	14.092	3956	3966	3976	rBV	4043	6410	6.05%	1.837%
14	14.336	4032	4042	4050	rBV4	3079	4350	4.11%	1.247%
15	14.587	4113	4120	4127	rVB3	1773	2321	2.19%	0.665%
16	16.198	4613	4621	4626	rBV4	1282	2177	2.06%	0.624%




Sum of corrected areas: 348857

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072021\
Data File : VU044368.D
Acq On : 20 Jul 2021 11:12
Operator : SY/MD
Sample : VU0720WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0720WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

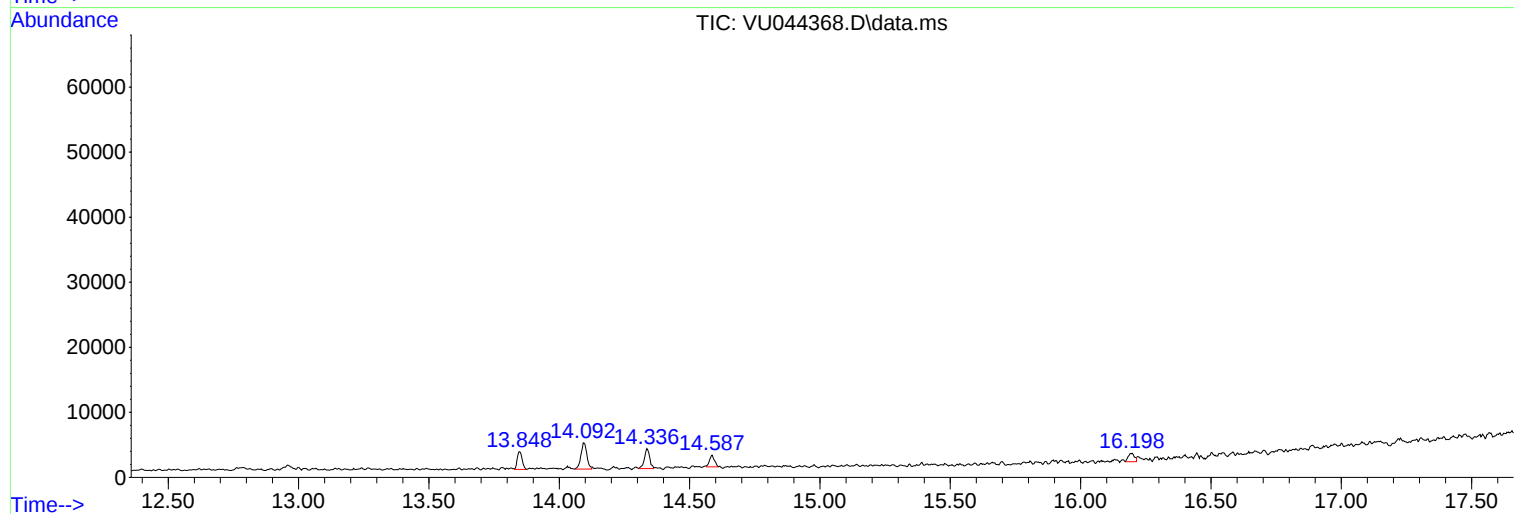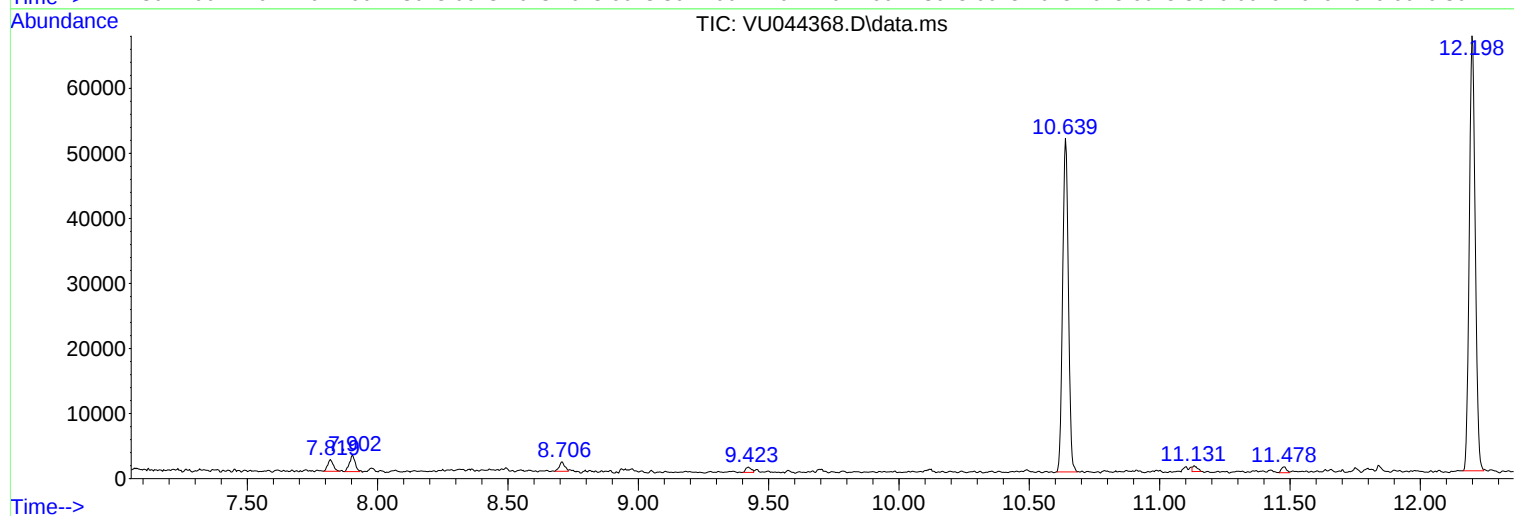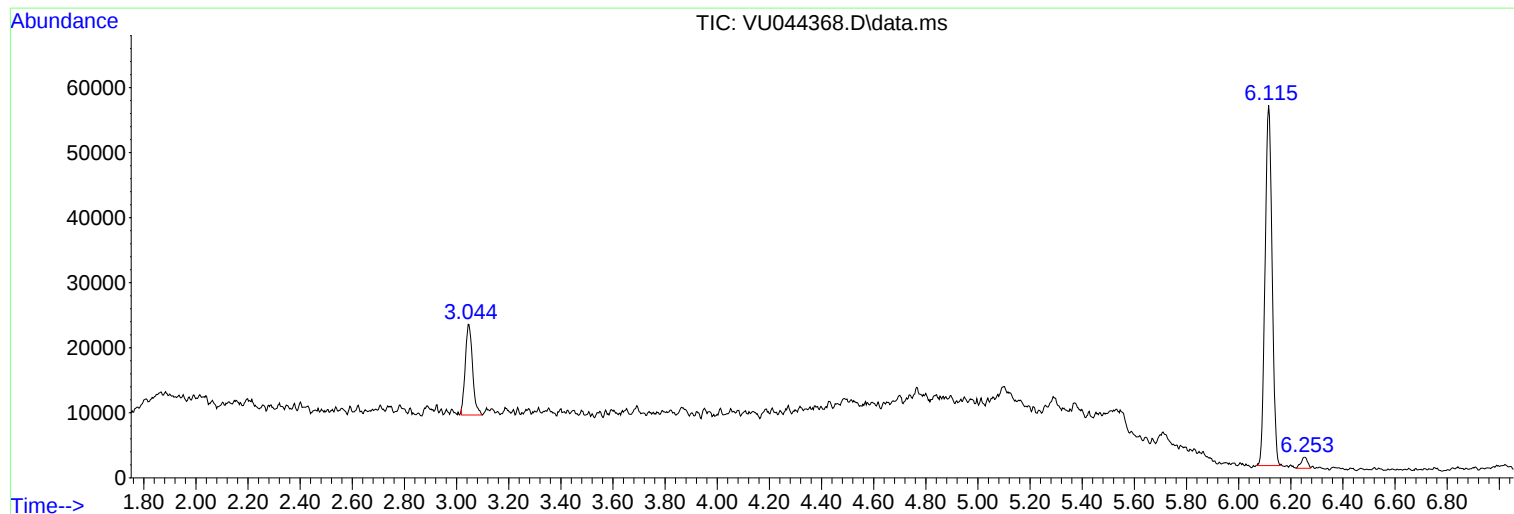

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072021\
Data File : VU044368.D
Acq On : 20 Jul 2021 11:12
Operator : SY/MD
Sample : VU0720WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0720WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072021\
Data File : VU044368.D
Acq On : 20 Jul 2021 11:12
Operator : SY/MD
Sample : VU0720WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0720WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
