




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
 Data File : VU049810.D
 Acq On : 20 Jul 2022 18:01
 Operator : SY/MD
 Sample : N3743-15ME
 Misc : 6.17g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5D13ME

Manual IntegrationsAPPROVED

Quant Time: Jul 21 04:25:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 21 04:19:56 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 07/21/2022
 Supervised By :Mahesh Dadoda 07/21/2022

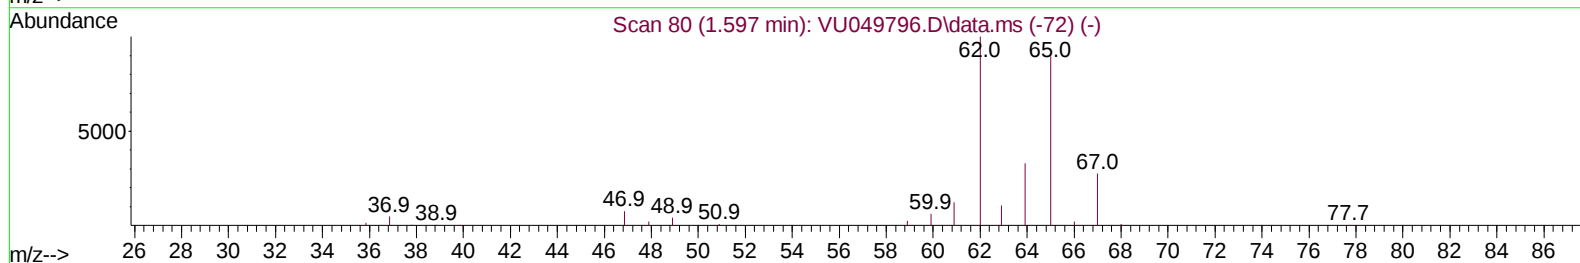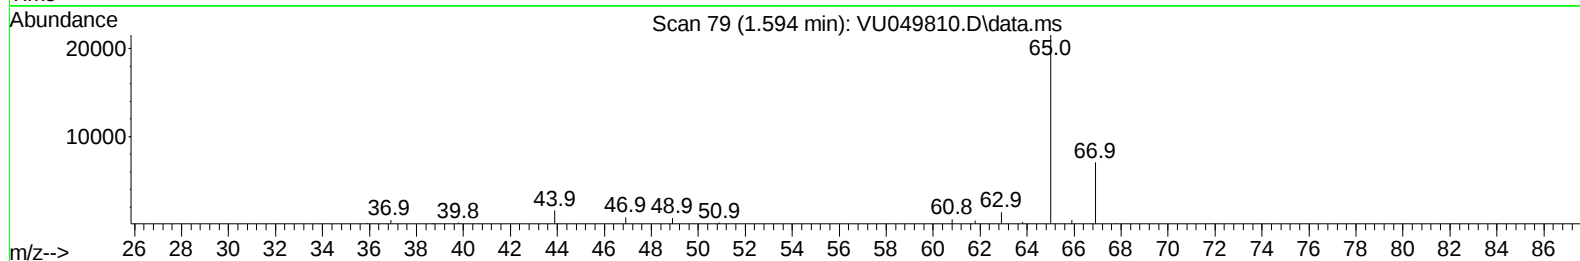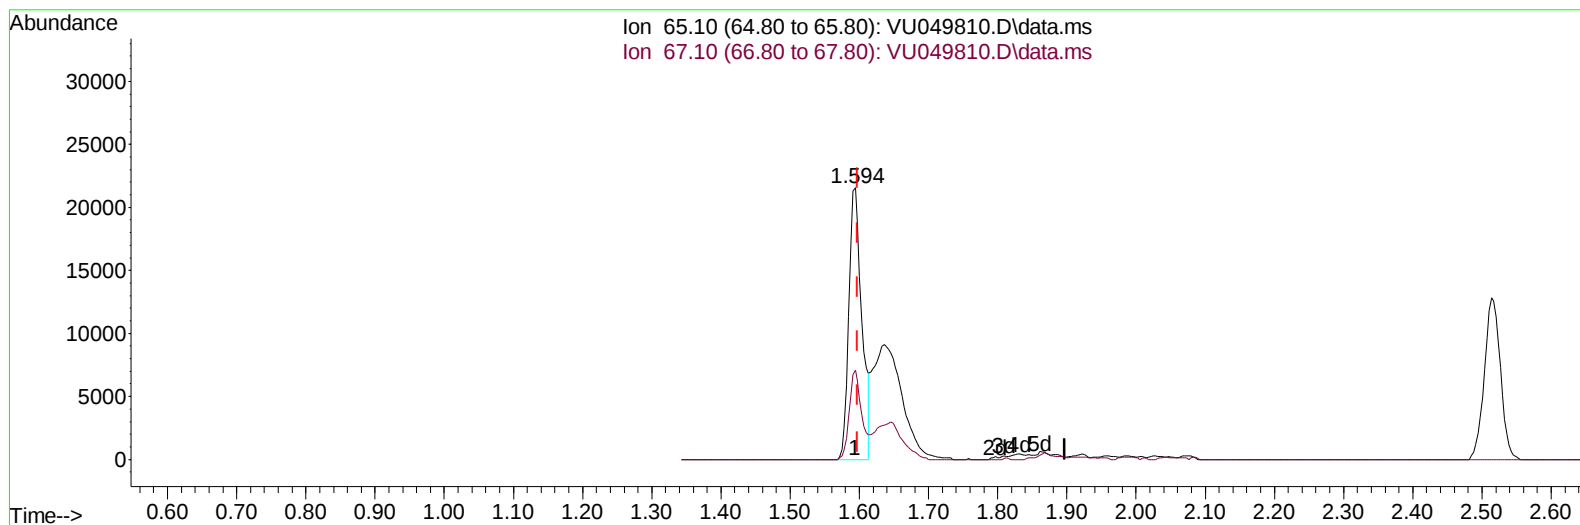

TIC: VU049810.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.594min (-0.003) 17.47 ug/L

response 28466

Ion	Exp%	Act%
65.10	100.00	100.00
67.10	31.10	32.77
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
 Data File : VU049810.D
 Acq On : 20 Jul 2022 18:01
 Operator : SY/MD
 Sample : N3743-15ME
 Misc : 6.17g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5D13ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 07/21/2022
 Supervised By :Mahesh Dadoda 07/21/2022

Quant Time: Jul 21 04:25:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 21 04:19:56 2022
 Response via : Initial Calibration

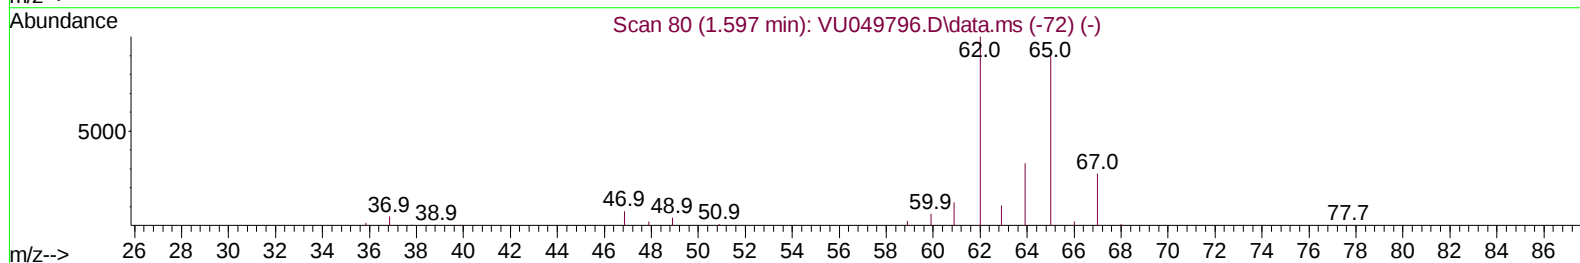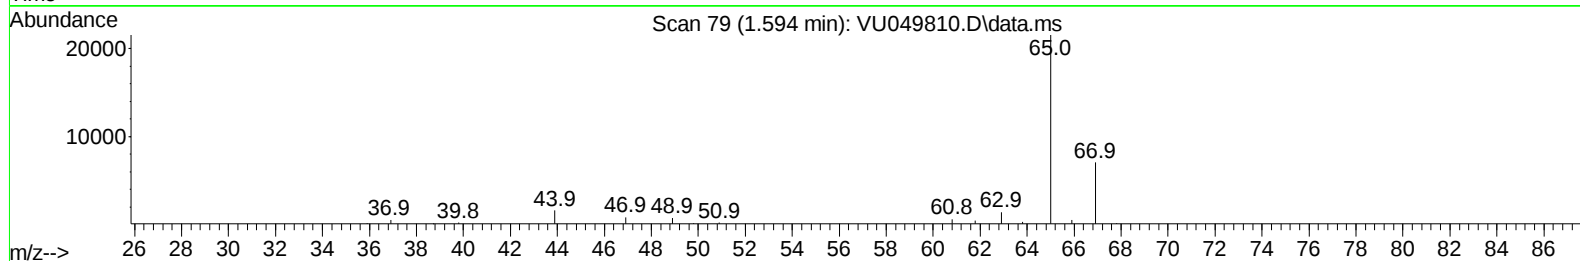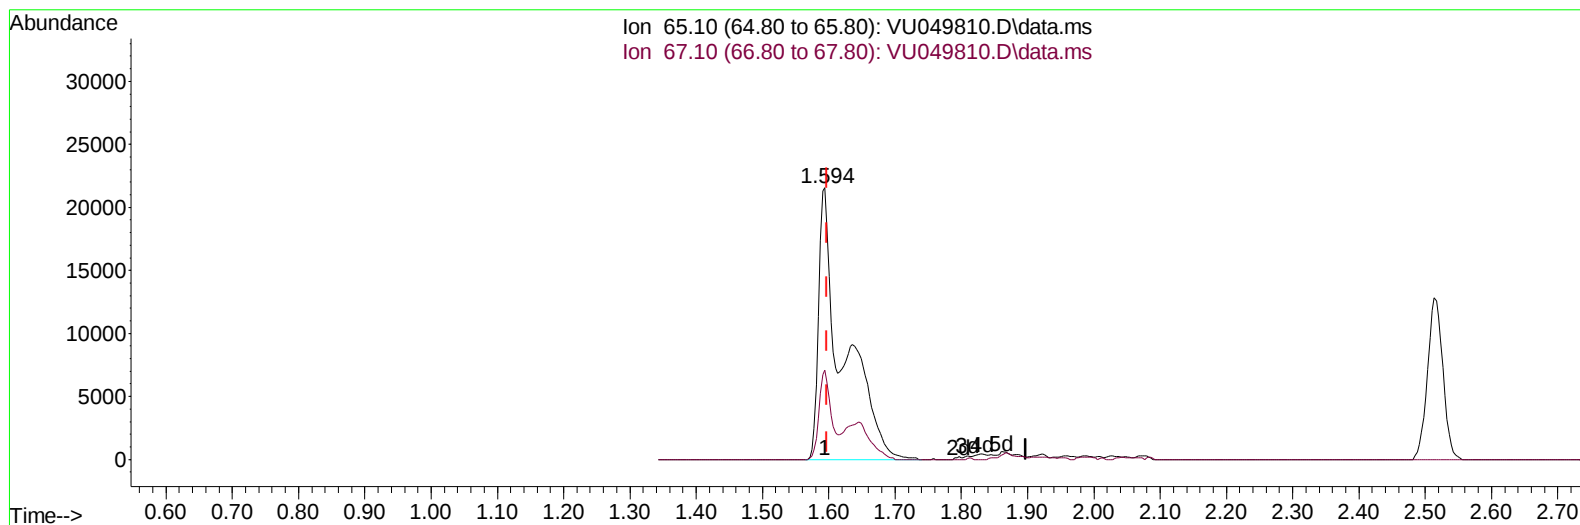

TIC: VU049810.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.594min (-0.003) 33.81 ug/L m

response 55086

Ion	Exp%	Act%
65.10	100.00	100.00
67.10	31.10	16.94#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
Data File : VU049810.D
Acq On : 20 Jul 2022 18:01
Operator : SY/MD
Sample : N3743-15ME
Misc : 6.17g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5D13ME

Manual IntegrationsAPPROVED

Quant Time: Jul 21 04:25:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 21 04:19:56 2022
Response via : Initial Calibration

Reviewed By :John Carlone 07/21/2022
Supervised By :Mahesh Dadoda 07/21/2022

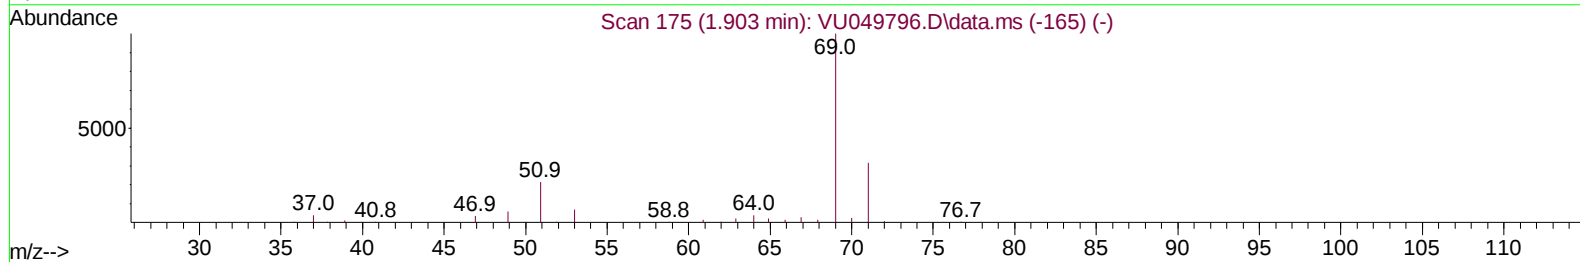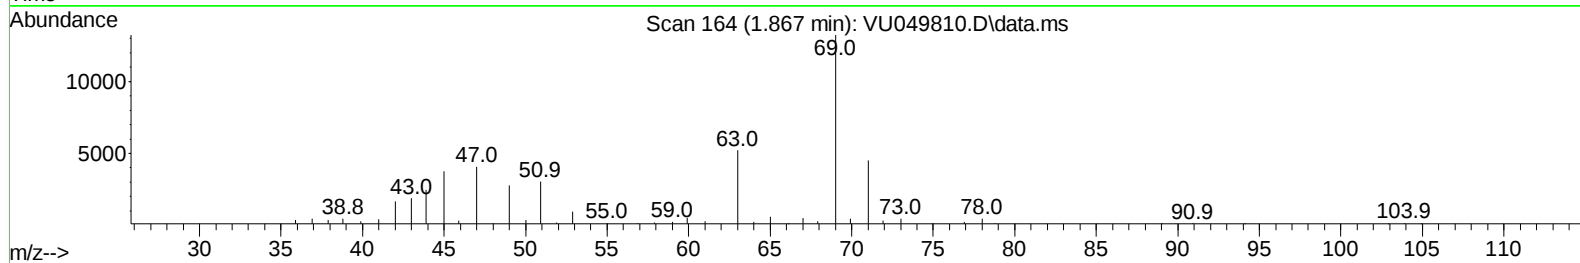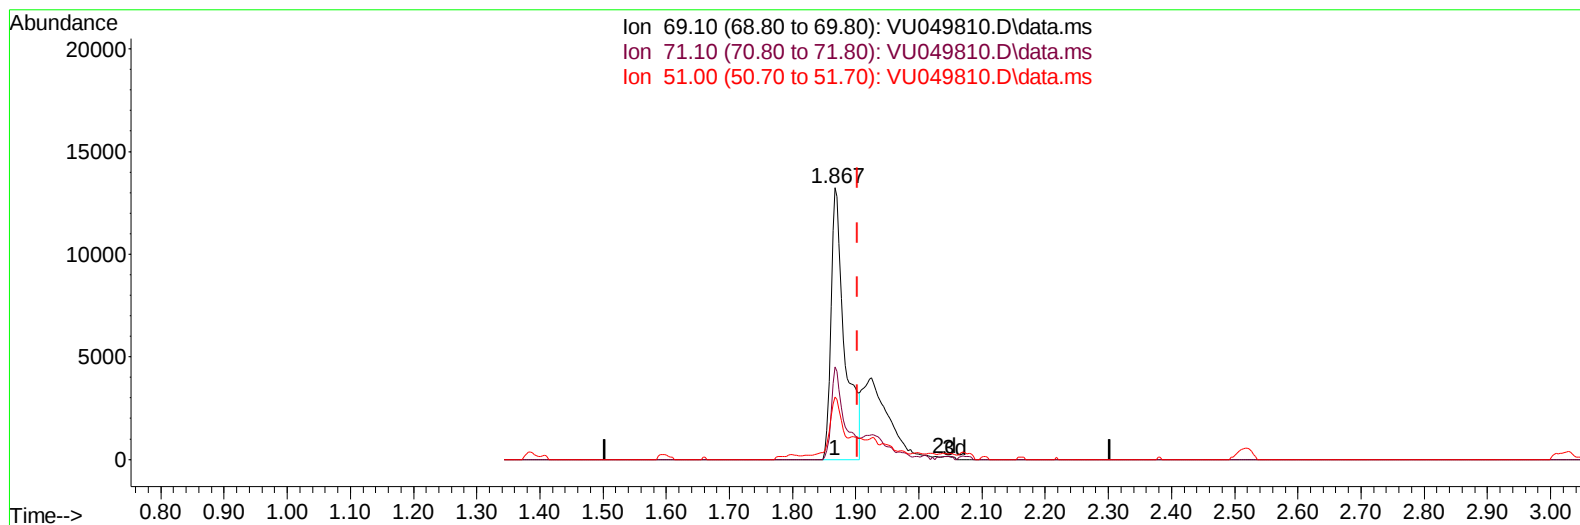

TIC: VU049810.D\data.ms

(7) Chloroethane-d5 (S)

1.867min (-0.035) 17.02 ug/L

response 20047

Ion	Exp%	Act%
69.10	100.00	100.00
71.10	31.70	33.10
51.00	23.40	18.47
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
Data File : VU049810.D
Acq On : 20 Jul 2022 18:01
Operator : SY/MD
Sample : N3743-15ME
Misc : 6.17g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5D13ME

Manual IntegrationsAPPROVED

Quant Time: Jul 21 04:25:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 21 04:19:56 2022
Response via : Initial Calibration

Reviewed By :John Carlone 07/21/2022
Supervised By :Mahesh Dadoda 07/21/2022

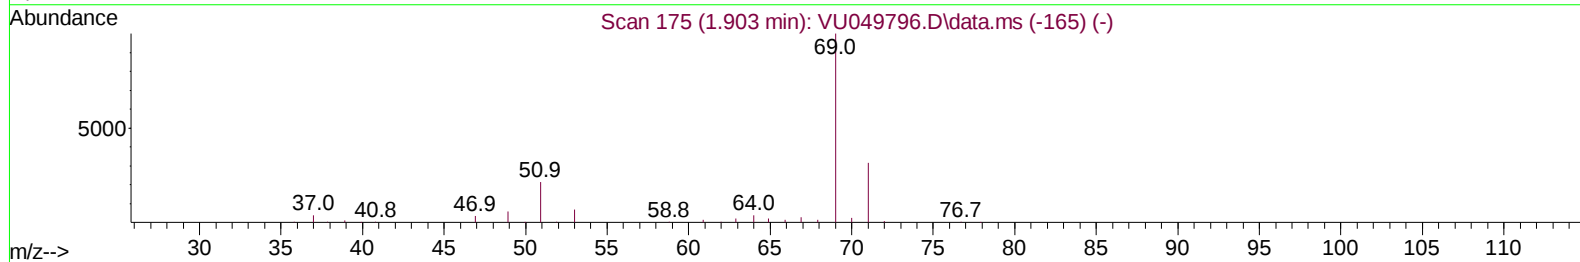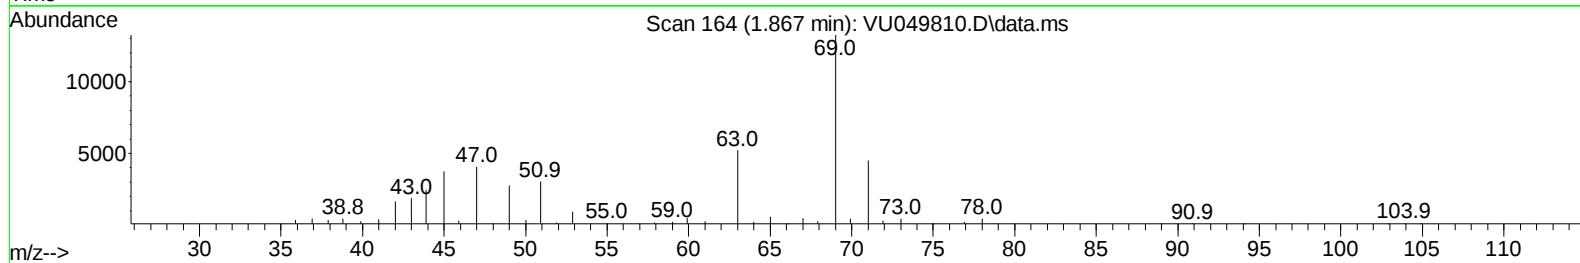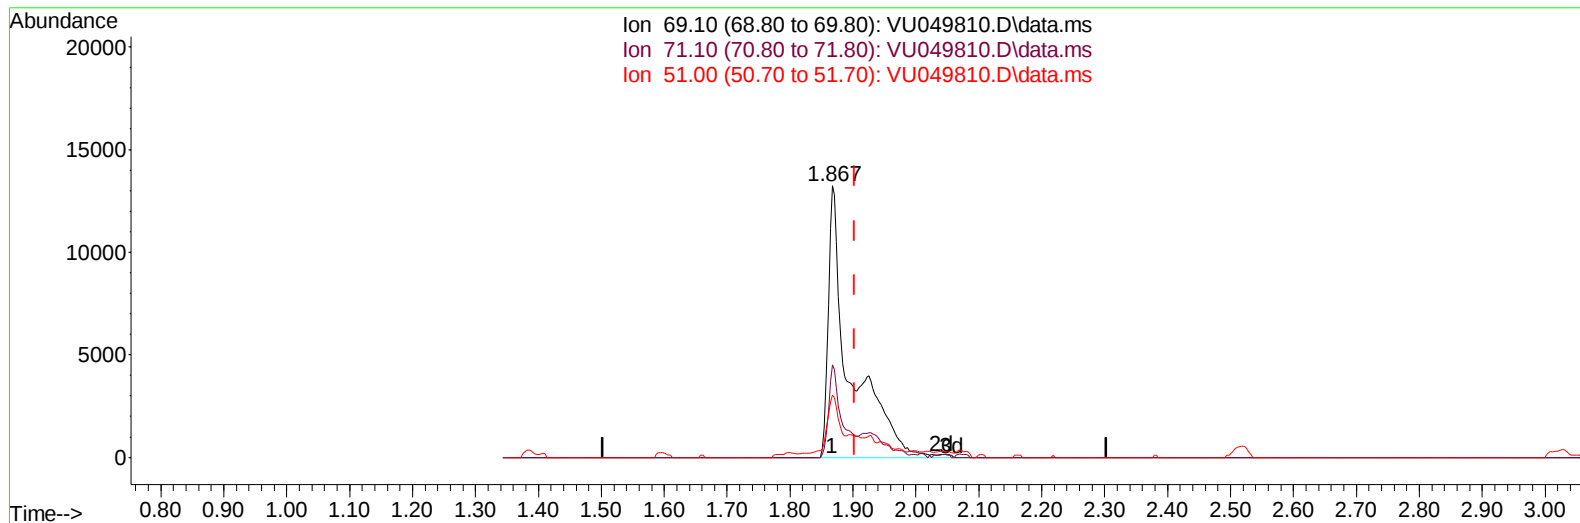

TIC: VU049810.D\data.ms

(7) Chloroethane-d5 (S)

1.867min (-0.035) 26.97 ug/L m

response 31760

Ion	Exp%	Act%
69.10	100.00	100.00
71.10	31.70	20.89#
51.00	23.40	11.66#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
 Data File : VU049810.D
 Acq On : 20 Jul 2022 18:01
 Operator : SY/MD
 Sample : N3743-15ME
 Misc : 6.17g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5D13ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 07/21/2022
 Supervised By :Mahesh Dadoda 07/21/2022

Quant Time: Jul 21 04:25:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 21 04:19:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	193073	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	184868	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.815	152	83651	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	55086m	33.815	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	67.620%	
7) Chloroethane-d5	1.867	69	31760m	26.972	ug/L	-0.04
Spiked Amount 50.000	Range 70	- 130	Recovery	=	53.940%#	
11) 1,1-Dichloroethene-d2	2.514	63	64774	22.510	ug/L	-0.05
Spiked Amount 50.000	Range 60	- 125	Recovery	=	45.020%#	
21) 2-Butanone-d5	4.642	46	122121	87.815	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130	Recovery	=	87.820%	
24) Chloroform-d	5.060	84	104931	36.367	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	72.740%	
26) 1,2-Dichloroethane-d4	5.700	65	77928	39.906	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	79.820%	
32) Benzene-d6	5.716	84	195037	34.727	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	69.460%#	
36) 1,2-Dichloropropane-d6	6.687	67	70585	37.365	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	74.740%	
41) Toluene-d8	7.896	98	159604	32.633	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	65.260%#	
43) trans-1,3-Dichloroprop...	8.182	79	28410	35.695	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	71.400%	
47) 2-Hexanone-d5	8.652	63	73960	87.037	ug/L	0.02
Spiked Amount 100.000	Range 45	- 130	Recovery	=	87.040%	
56) 1,1,2,2-Tetrachloroeth...	10.764	84	109620	41.472	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	82.940%	
66) 1,2-Dichlorobenzene-d4	12.198	152	59037	37.432	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	74.860%#	
Target Compounds					Qvalue	
20) cis-1,2-Dichloroethene	4.655	96	3674	2.165	ug/L	70
46) Tetrachloroethene	8.552	164	9959	8.549	ug/L	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
Data File : VU049810.D
Acq On : 20 Jul 2022 18:01
Operator : SY/MD
Sample : N3743-15ME
Misc : 6.17g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5D13ME

Manual IntegrationsAPPROVED

Quant Time: Jul 21 04:25:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 21 04:19:56 2022
Response via : Initial Calibration

Reviewed By :John Carlone 07/21/2022
Supervised By :Mahesh Dadoda 07/21/2022

