

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
 Data File : VU049808.D
 Acq On : 20 Jul 2022 17:13
 Operator : SY/MD
 Sample : N3743-05ME
 Misc : 6.03g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5C91ME

Manual Integrations
 APPROVED


Reviewed By : John Carlone 07/21/2022
 Supervised By : Mahesh Dadoda 07/21/2022

Quant Time: Jul 21 04:25:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 21 04:19:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	178080	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	172976	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.815	152	80708	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	57912m	38.543	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	77.080%		
7) Chloroethane-d5	1.867	69	33553m	30.893	ug/L	-0.04
Spiked Amount 50.000	Range 70 - 130		Recovery =	61.780%#		
11) 1,1-Dichloroethene-d2	2.514	63	70134	26.425	ug/L	-0.05
Spiked Amount 50.000	Range 60 - 125		Recovery =	52.860%#		
21) 2-Butanone-d5	4.642	46	125307	97.692	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	97.690%		
24) Chloroform-d	5.060	84	107591	40.429	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	80.860%		
26) 1,2-Dichloroethane-d4	5.697	65	79594	44.191	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.380%		
32) Benzene-d6	5.716	84	204587	38.932	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	77.860%		
36) 1,2-Dichloropropane-d6	6.687	67	74194	41.976	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	83.960%		
41) Toluene-d8	7.896	98	166840	36.458	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	72.920%#		
43) trans-1,3-Dichloroprop...	8.182	79	29139	39.128	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	78.260%		
47) 2-Hexanone-d5	8.648	63	78333	98.521	ug/L	0.02
Spiked Amount 100.000	Range 45 - 130		Recovery =	98.520%		
56) 1,1,2,2-Tetrachloroeth...	10.764	84	114973	46.488	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	92.980%		
66) 1,2-Dichlorobenzene-d4	12.198	152	65788	43.233	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.460%		
Target Compounds						Qvalue
16) Methylene chloride	3.025	84	2288	1.427	ug/L	96
20) cis-1,2-Dichloroethene	4.655	96	4001	2.556	ug/L	94
34) Trichloroethene	6.542	95	4409	2.805	ug/L	83
46) Tetrachloroethene	8.552	164	9627	8.832	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

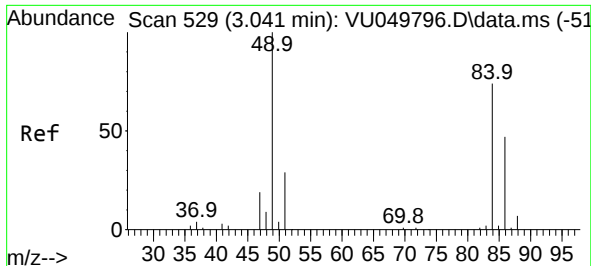

#16
Methylene chloride
Concen: 1.427 ug/L
RT: 3.025 min Scan# 51
Delta R.T. -0.016 min
Lab File: VU049808.D
Acq: 20 Jul 2022 17:13




Instrument :
MSVOA_U
ClientSampleId :
F5C91ME

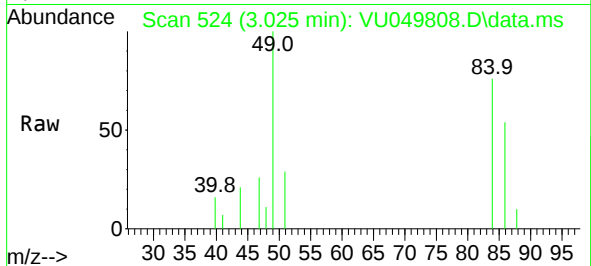


Tgt Ion: 84 Resp: 228
Ion Ratio Lower Upper
84 100
86 71.3 45.6 84.6
49 131.5 94.4 175.4

Manual Integrations
APPROVED



Reviewed By :John Carlone 07/21/2022
Supervised By :Mahesh Dadoda 07/21/2022

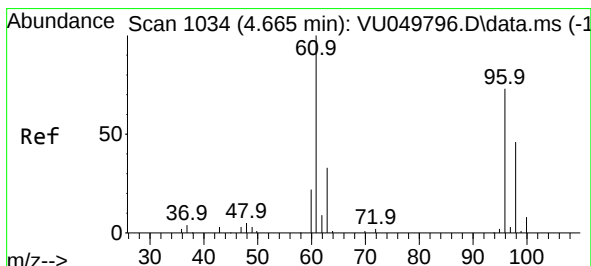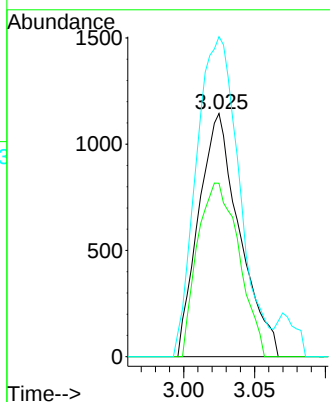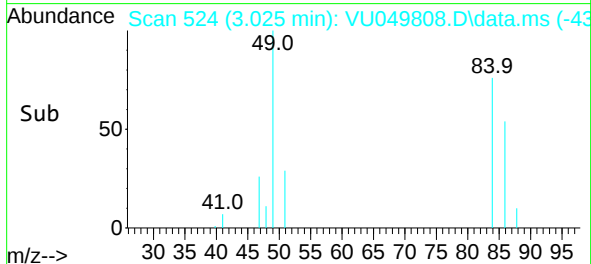


#20
cis-1,2-Dichloroethene
Concen: 2.556 ug/L
RT: 4.655 min Scan# 1031
Delta R.T. -0.010 min
Lab File: VU049808.D
Acq: 20 Jul 2022 17:13

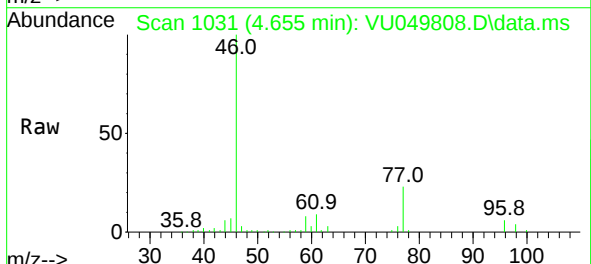


Tgt Ion: 96 Resp: 4001
Ion Ratio Lower Upper
96 100
61 151.5 101.1 187.7
68 0.0 0.0 0.0

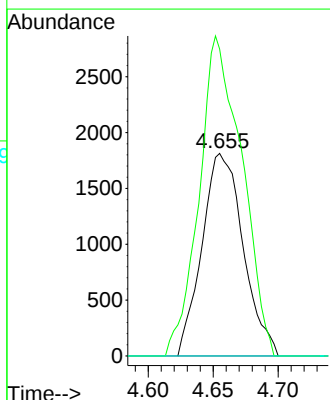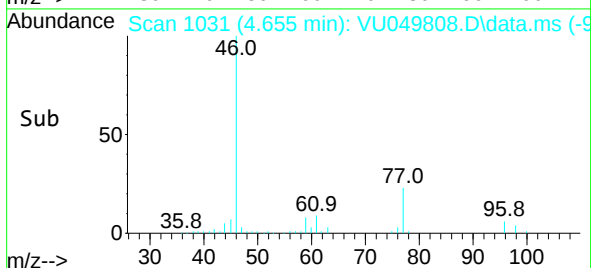

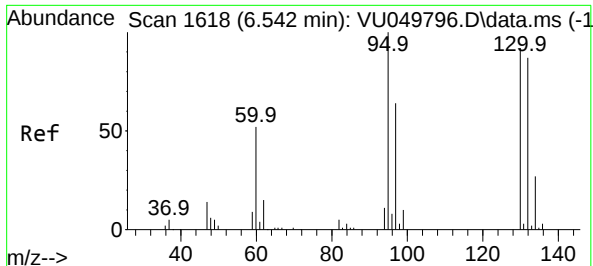

#34
Trichloroethene
Concen: 2.805 ug/L
RT: 6.542 min Scan# 1618
Delta R.T. 0.000 min
Lab File: VU049808.D
Acq: 20 Jul 2022 17:13




Instrument :
MSVOA_U
ClientSampleId :
F5C91ME

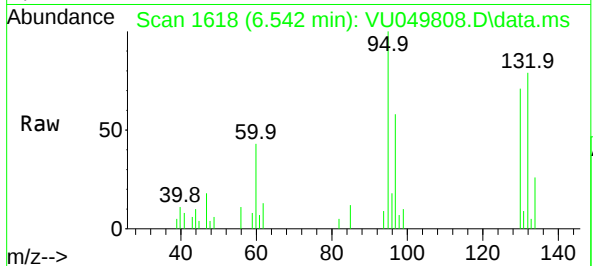


Tgt Ion: 95 Resp: 4409
Ion Ratio Lower Upper
95 100
97 58.3 46.9 87.1
132 78.5 62.7 116.5
130 70.7 66.4 123.4

Manual Integrations
APPROVED

Reviewed By :John Carlone 07/21/2022
Supervised By :Mahesh Dadoda 07/21/2022

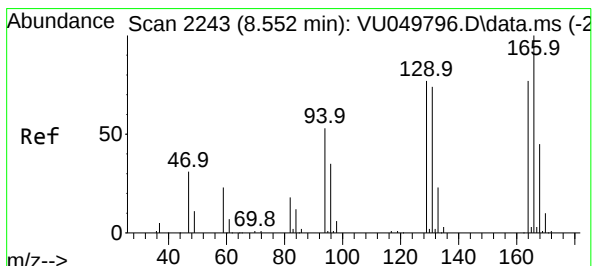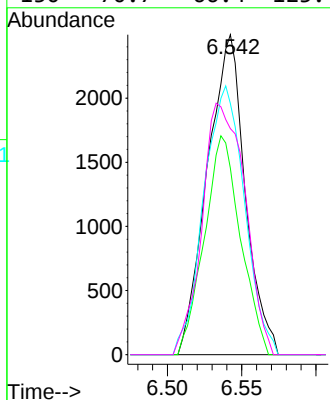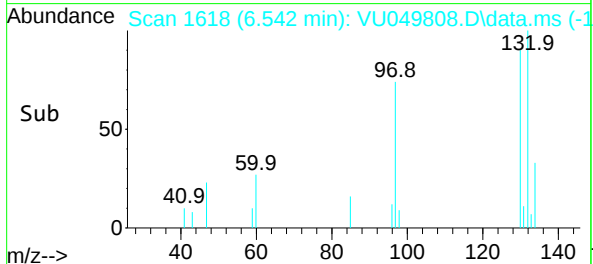

#46
Tetrachloroethene
Concen: 8.832 ug/L
RT: 8.552 min Scan# 2243
Delta R.T. 0.000 min
Lab File: VU049808.D
Acq: 20 Jul 2022 17:13

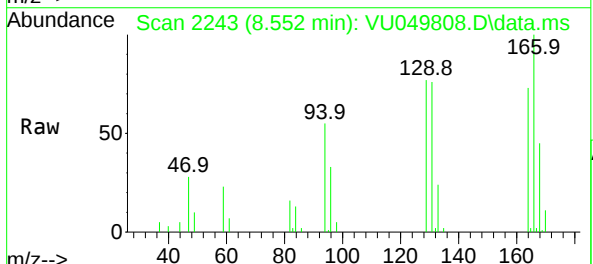

Tgt Ion:164 Resp: 9627
Ion Ratio Lower Upper
164 100
129 105.5 72.0 133.8
131 103.7 69.0 128.1
166 136.8 91.1 169.3

