

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
 Data File : VU049811.D
 Acq On : 20 Jul 2022 18:49
 Operator : SY/MD
 Sample : N3792-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUL2

Quant Time: Jul 21 04:26:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 21 04:19:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	175150	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	167372	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	68029	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	63193	42.761	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	85.520%
7) Chloroethane-d5	1.900	69	50946	47.692	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	95.380%
11) 1,1-Dichloroethene-d2	2.562	63	79254	30.361	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	60.720%
21) 2-Butanone-d5	4.620	46	151695	120.243	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	120.240%
24) Chloroform-d	5.063	84	129723	49.561	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.120%
26) 1,2-Dichloroethane-d4	5.700	65	93936	53.026	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.060%
32) Benzene-d6	5.726	84	237799	46.767	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.540%
36) 1,2-Dichloropropane-d6	6.690	67	86409	50.523	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.040%
41) Toluene-d8	7.896	98	190381	42.995	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.980%
43) trans-1,3-Dichloroprop...	8.179	79	33542	46.549	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.100%
47) 2-Hexanone-d5	8.632	63	74825	97.260	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	97.260%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	123399	51.565	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	103.140%
66) 1,2-Dichlorobenzene-d4	12.195	152	64894	50.594	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.180%
Target Compounds						
13) Acetone	2.626	43	11135	9.287	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
Data File : VU049811.D
Acq On : 20 Jul 2022 18:49
Operator : SY/MD
Sample : N3792-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUL2

Quant Time: Jul 21 04:26:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 21 04:19:56 2022
Response via : Initial Calibration

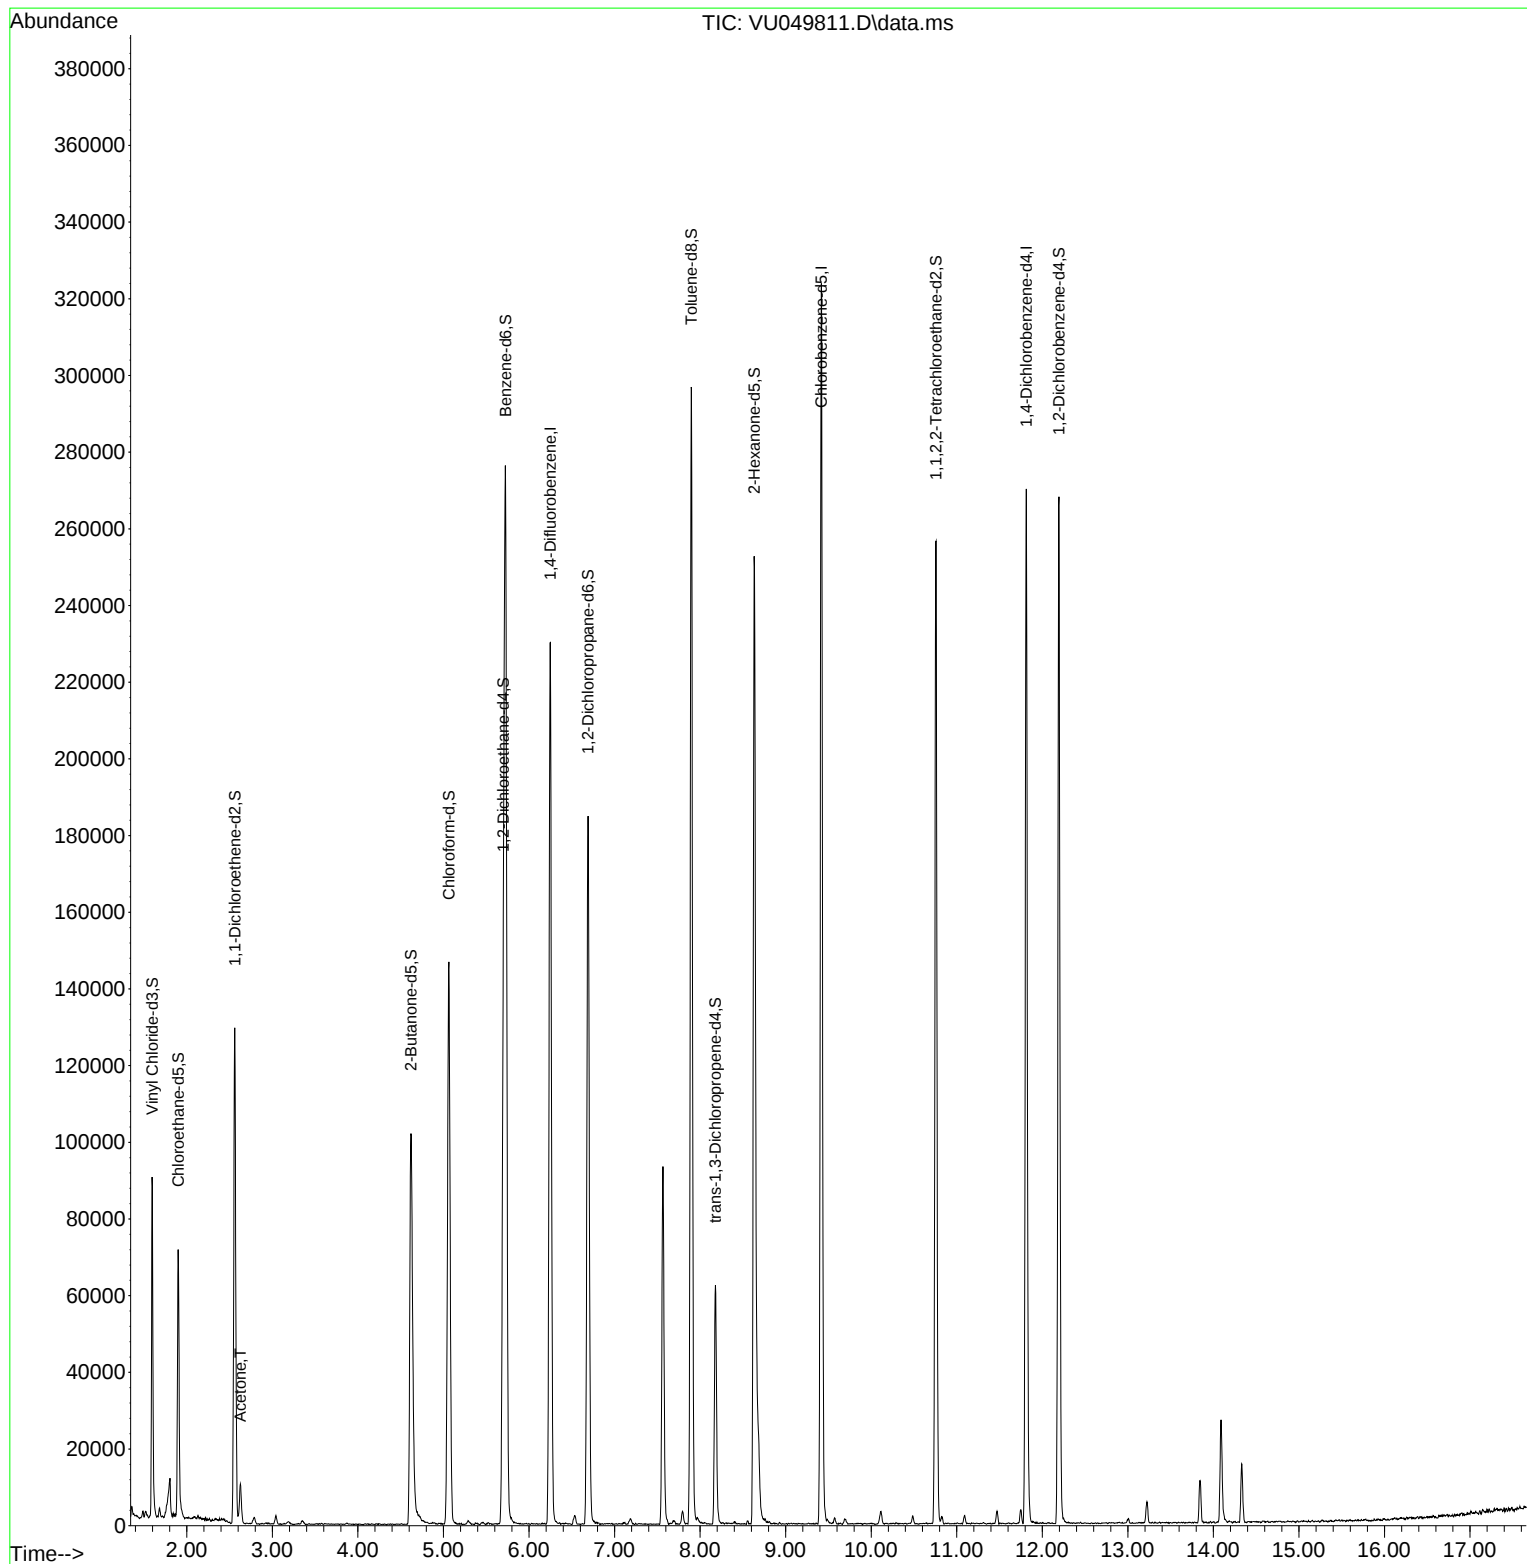

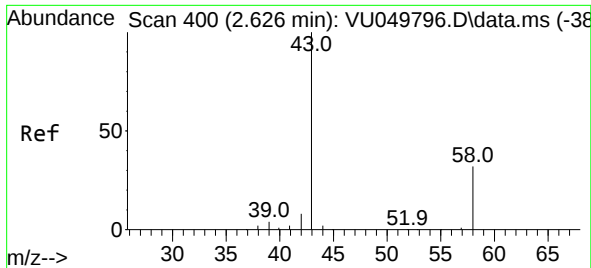

#13

Acetone

Concen: 9.287 ug/L

RT: 2.626 min Scan# 40

Delta R.T. 0.000 min

Lab File: VU049811.D


Acq: 20 Jul 2022 18:49

Instrument :

MSVOA_U

ClientSampleId :

DBUL2

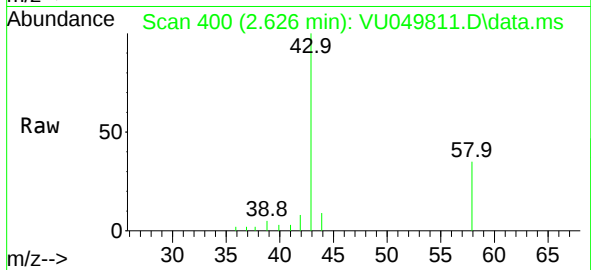

Tgt Ion: 43 Resp: 11135

Ion Ratio Lower Upper

43 100

58 31.9 0.0 61.4

