

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
 Data File : VU049813.D
 Acq On : 20 Jul 2022 19:36
 Operator : SY/MD
 Sample : N3792-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUM6

Quant Time: Jul 21 04:26:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 21 04:19:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	176446	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	164822	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	67202	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	63276	42.503	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	85.000%
7) Chloroethane-d5	1.903	69	50364	46.801	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	93.600%
11) 1,1-Dichloroethene-d2	2.562	63	80103	30.461	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	60.920%
21) 2-Butanone-d5	4.620	46	142679	112.266	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	112.270%
24) Chloroform-d	5.063	84	127556	48.375	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.740%
26) 1,2-Dichloroethane-d4	5.700	65	90729	50.840	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.680%
32) Benzene-d6	5.726	84	234634	46.859	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.720%
36) 1,2-Dichloropropane-d6	6.690	67	85327	50.663	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.320%
41) Toluene-d8	7.899	98	187934	43.099	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.200%
43) trans-1,3-Dichloroprop...	8.179	79	32292	45.507	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.020%
47) 2-Hexanone-d5	8.632	63	69082	91.184	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	91.180%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	121680	51.634	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	103.260%
66) 1,2-Dichlorobenzene-d4	12.195	152	63984	50.498	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.000%
Target Compounds						
13) Acetone	2.626	43	6748	5.587	ug/L	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
Data File : VU049813.D
Acq On : 20 Jul 2022 19:36
Operator : SY/MD
Sample : N3792-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUM6

Quant Time: Jul 21 04:26:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 21 04:19:56 2022
Response via : Initial Calibration

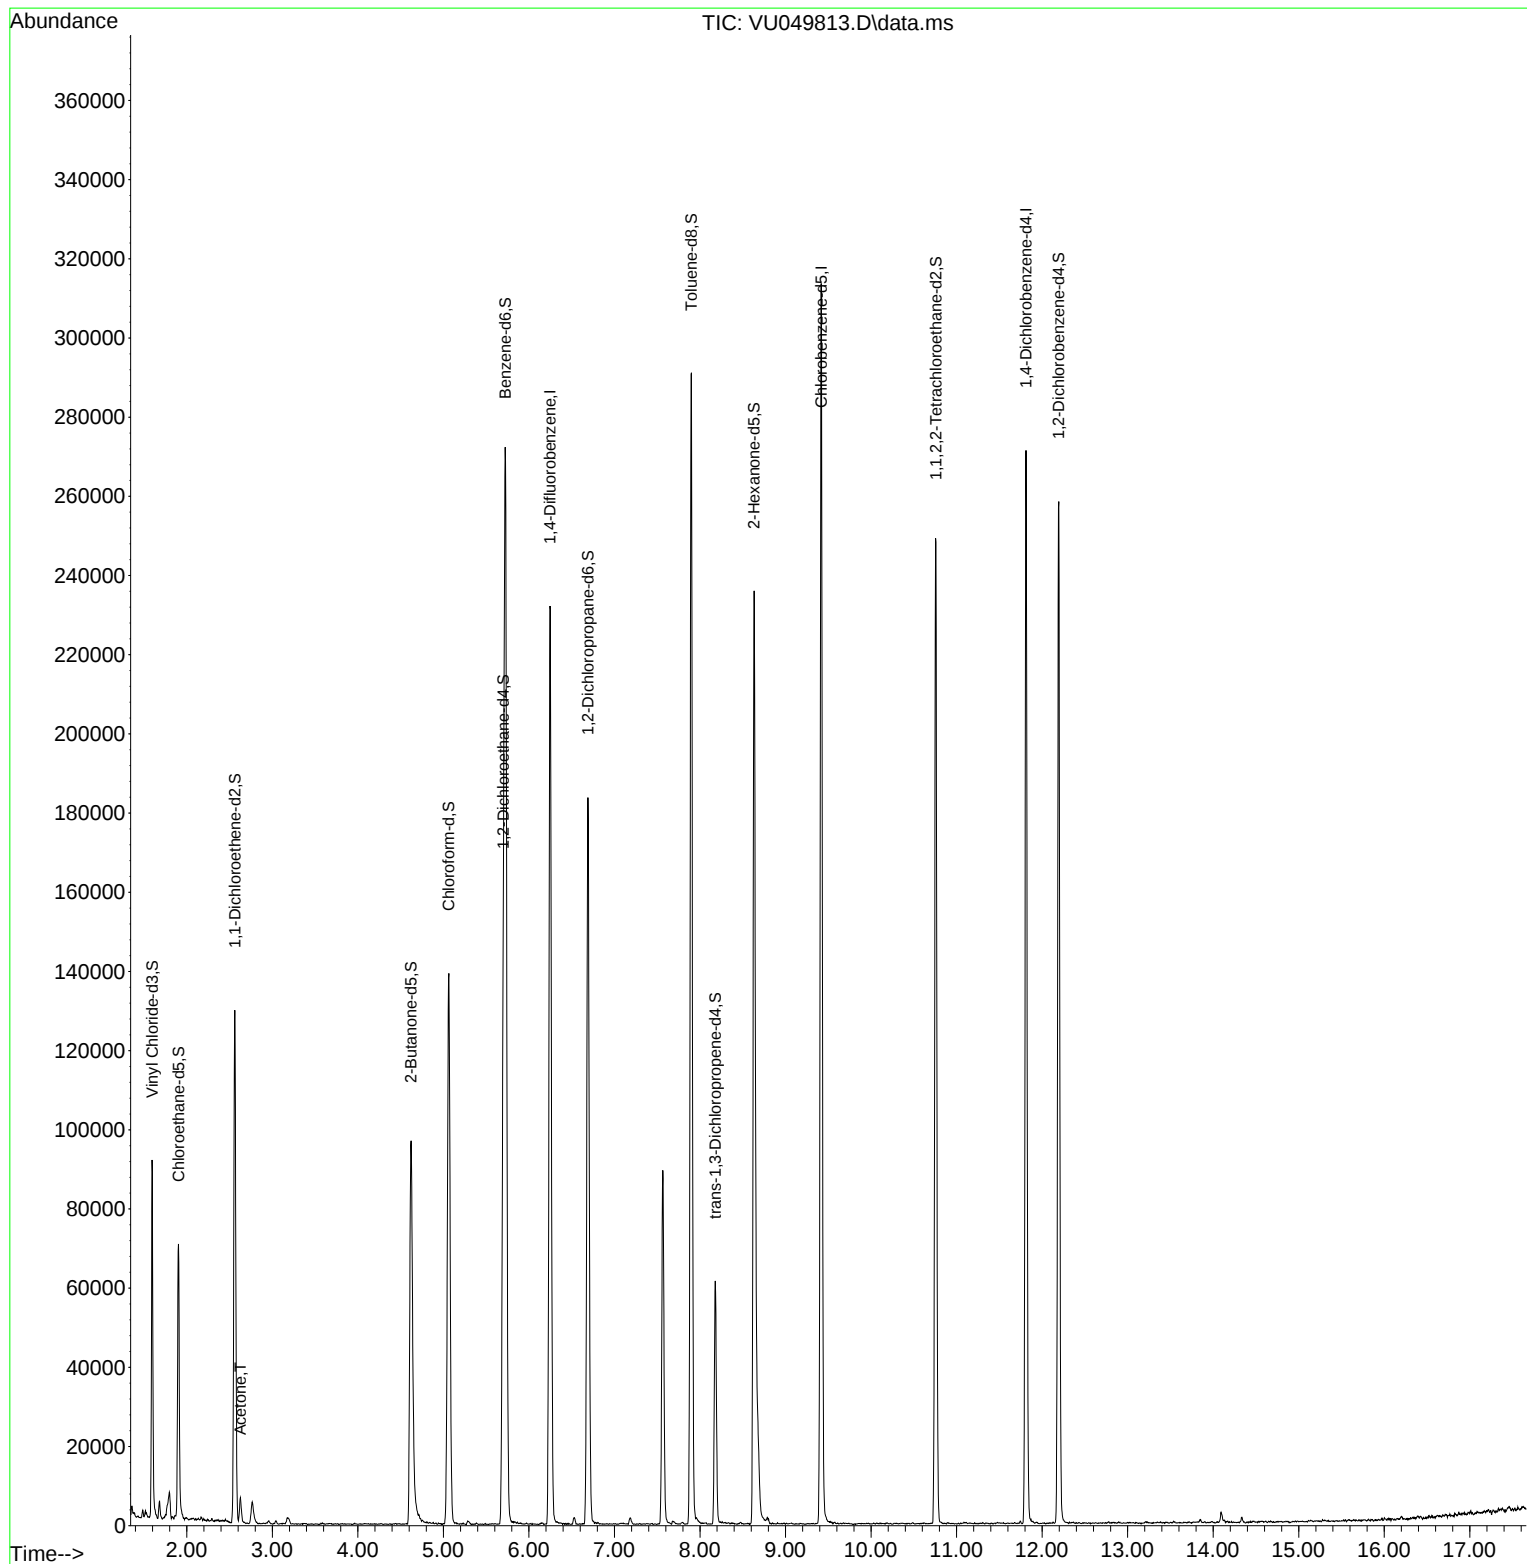

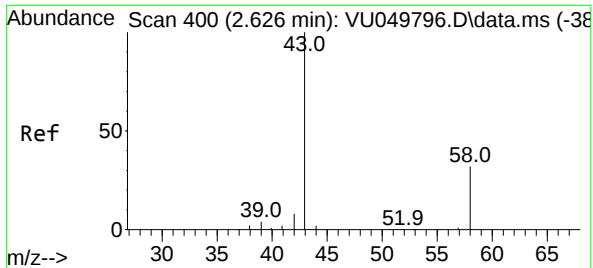

#13
 Acetone
 Concen: 5.587 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. 0.000 min
 Lab File: VU049813.D
 Acq: 20 Jul 2022 19:36

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUM6

Tgt Ion:	43	Resp:	6748
Ion	Ratio	Lower	Upper
43	100		
58	35.0	0.0	61.4

