

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
 Data File : VU049814.D
 Acq On : 20 Jul 2022 20:00
 Operator : SY/MD
 Sample : N3792-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUM7

Quant Time: Jul 21 04:26:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 21 04:19:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	175097	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	165666	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	67335	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	64179	43.441	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.880%
7) Chloroethane-d5	1.899	69	50098	46.913	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	93.820%
11) 1,1-Dichloroethene-d2	2.562	63	80674	30.914	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	61.820%
21) 2-Butanone-d5	4.620	46	141443	112.151	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	112.150%
24) Chloroform-d	5.063	84	126595	48.380	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.760%
26) 1,2-Dichloroethane-d4	5.700	65	91558	51.700	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.400%
32) Benzene-d6	5.726	84	233401	46.375	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.760%
36) 1,2-Dichloropropane-d6	6.690	67	86970	51.375	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.760%
41) Toluene-d8	7.899	98	187729	42.832	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.660%
43) trans-1,3-Dichloroprop...	8.179	79	33701	47.251	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.500%
47) 2-Hexanone-d5	8.632	63	69543	91.325	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	91.330%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	123314	52.061	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	104.120%
66) 1,2-Dichlorobenzene-d4	12.195	152	65056	51.243	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.480%
Target Compounds						
13) Acetone	2.626	43	8104	6.761	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
Data File : VU049814.D
Acq On : 20 Jul 2022 20:00
Operator : SY/MD
Sample : N3792-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUM7

Quant Time: Jul 21 04:26:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 21 04:19:56 2022
Response via : Initial Calibration

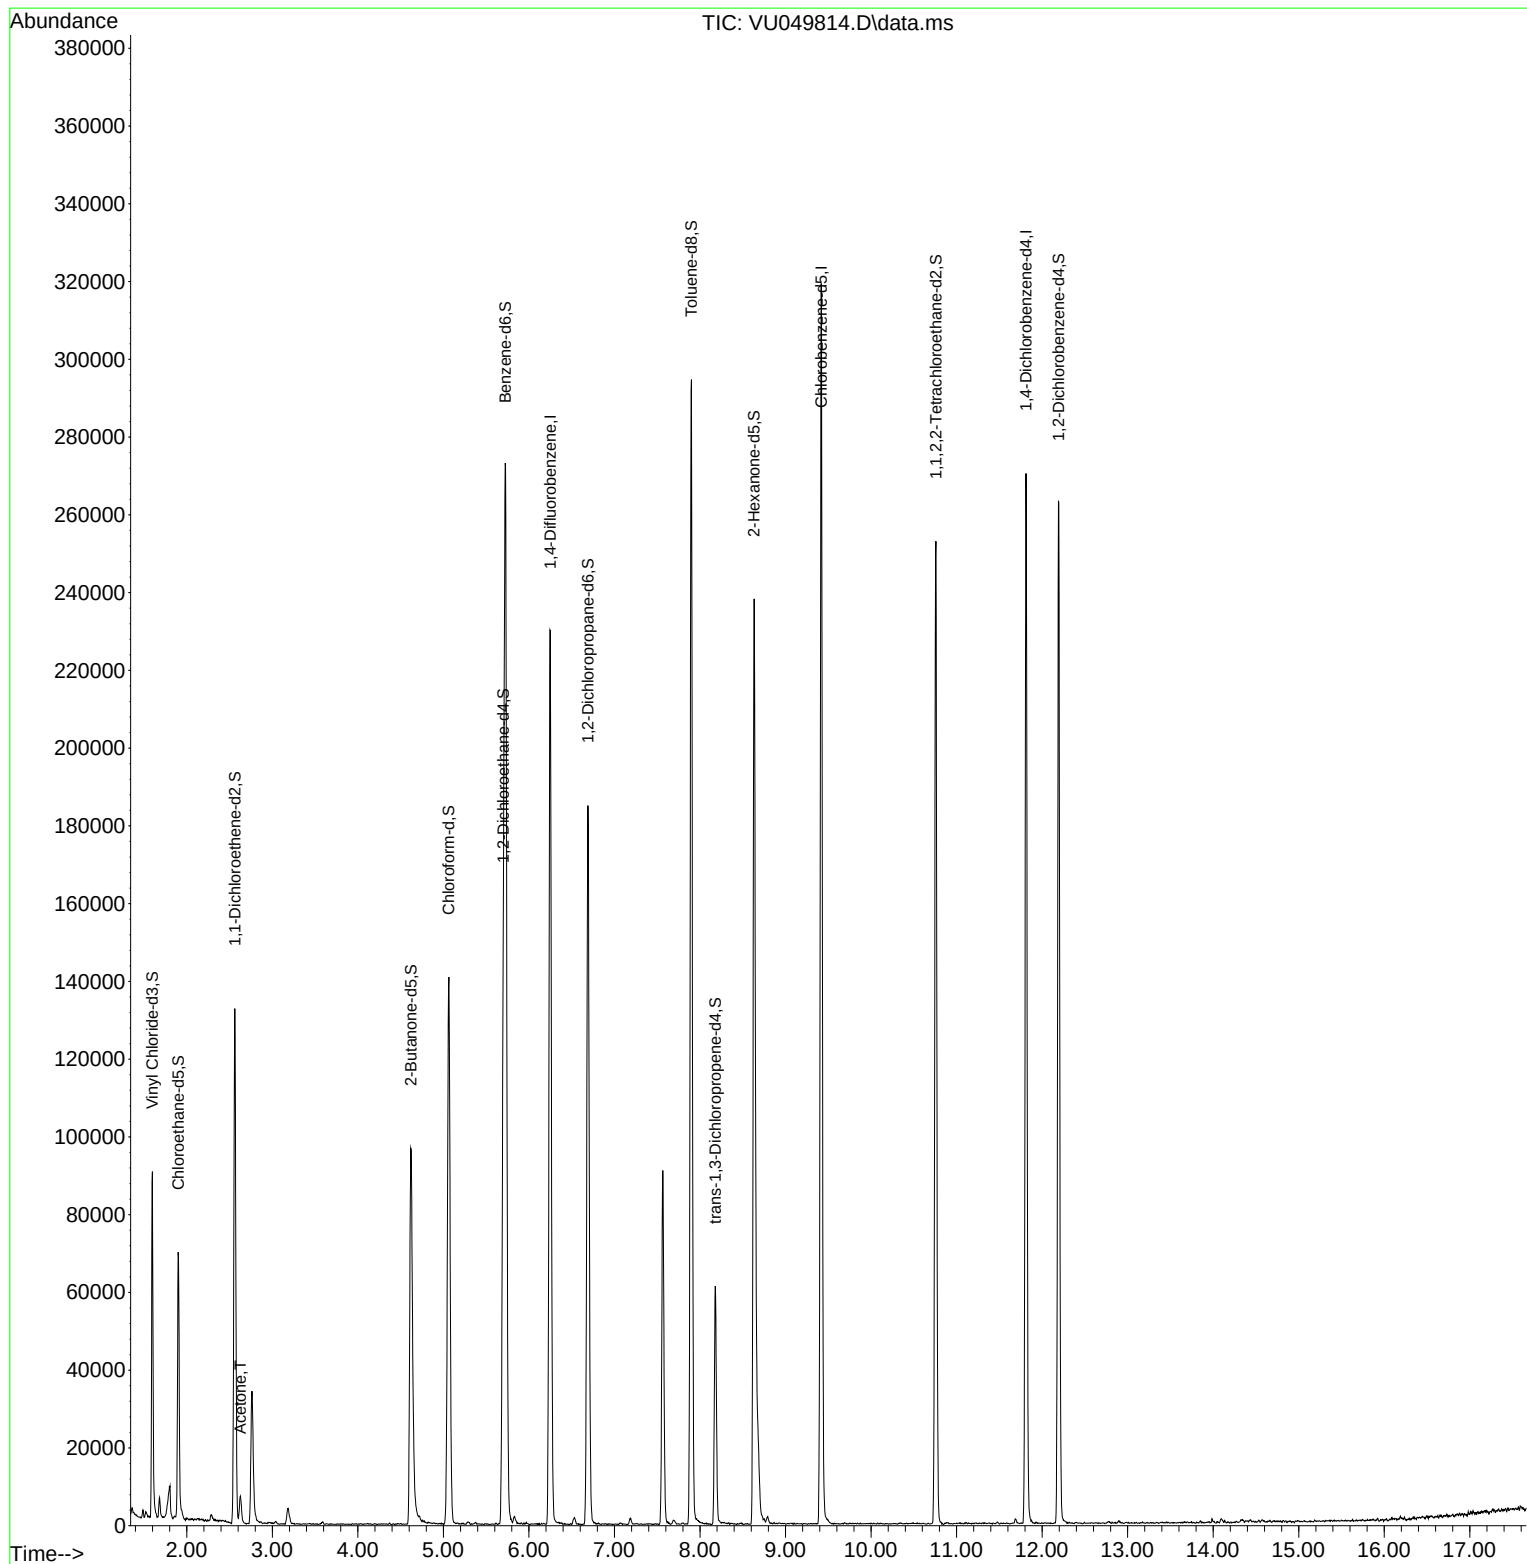

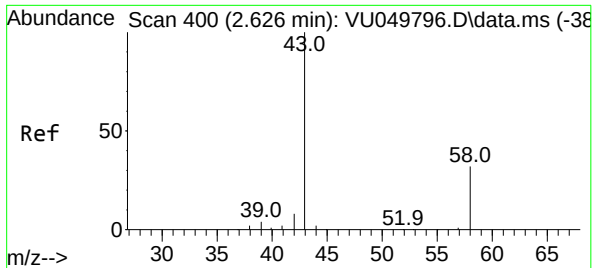

#13
 Acetone
 Concen: 6.761 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. 0.000 min
 Lab File: VU049814.D
 Acq: 20 Jul 2022 20:00

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUM7

Tgt Ion: 43 Resp: 8104
 Ion Ratio Lower Upper
 43 100
 58 30.0 0.0 61.4

