

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
 Data File : VU049815.D
 Acq On : 20 Jul 2022 20:24
 Operator : SY/MD
 Sample : N3792-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUN1

Quant Time: Jul 21 04:26:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 21 04:19:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	170993	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	160219	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	63786	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	61410	42.565	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	85.120%
7) Chloroethane-d5	1.900	69	48556	46.560	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	93.120%
11) 1,1-Dichloroethene-d2	2.559	63	78025	30.617	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	61.240%
21) 2-Butanone-d5	4.623	46	136376	110.729	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	110.730%
24) Chloroform-d	5.063	84	126576	49.534	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.060%
26) 1,2-Dichloroethane-d4	5.700	65	90819	52.513	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.020%
32) Benzene-d6	5.726	84	230957	47.450	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.900%
36) 1,2-Dichloropropane-d6	6.690	67	85826	52.423	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	104.840%
41) Toluene-d8	7.899	98	183006	43.174	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.340%
43) trans-1,3-Dichloroprop...	8.179	79	32362	46.916	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.840%
47) 2-Hexanone-d5	8.632	63	66898	90.838	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.840%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	118954	51.927	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	103.860%
66) 1,2-Dichlorobenzene-d4	12.192	152	62200	51.719	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.440%
Target Compounds						
13) Acetone	2.629	43	4741	4.050	ug/L	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
Data File : VU049815.D
Acq On : 20 Jul 2022 20:24
Operator : SY/MD
Sample : N3792-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUN1


Quant Time: Jul 21 04:26:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 21 04:19:56 2022
Response via : Initial Calibration

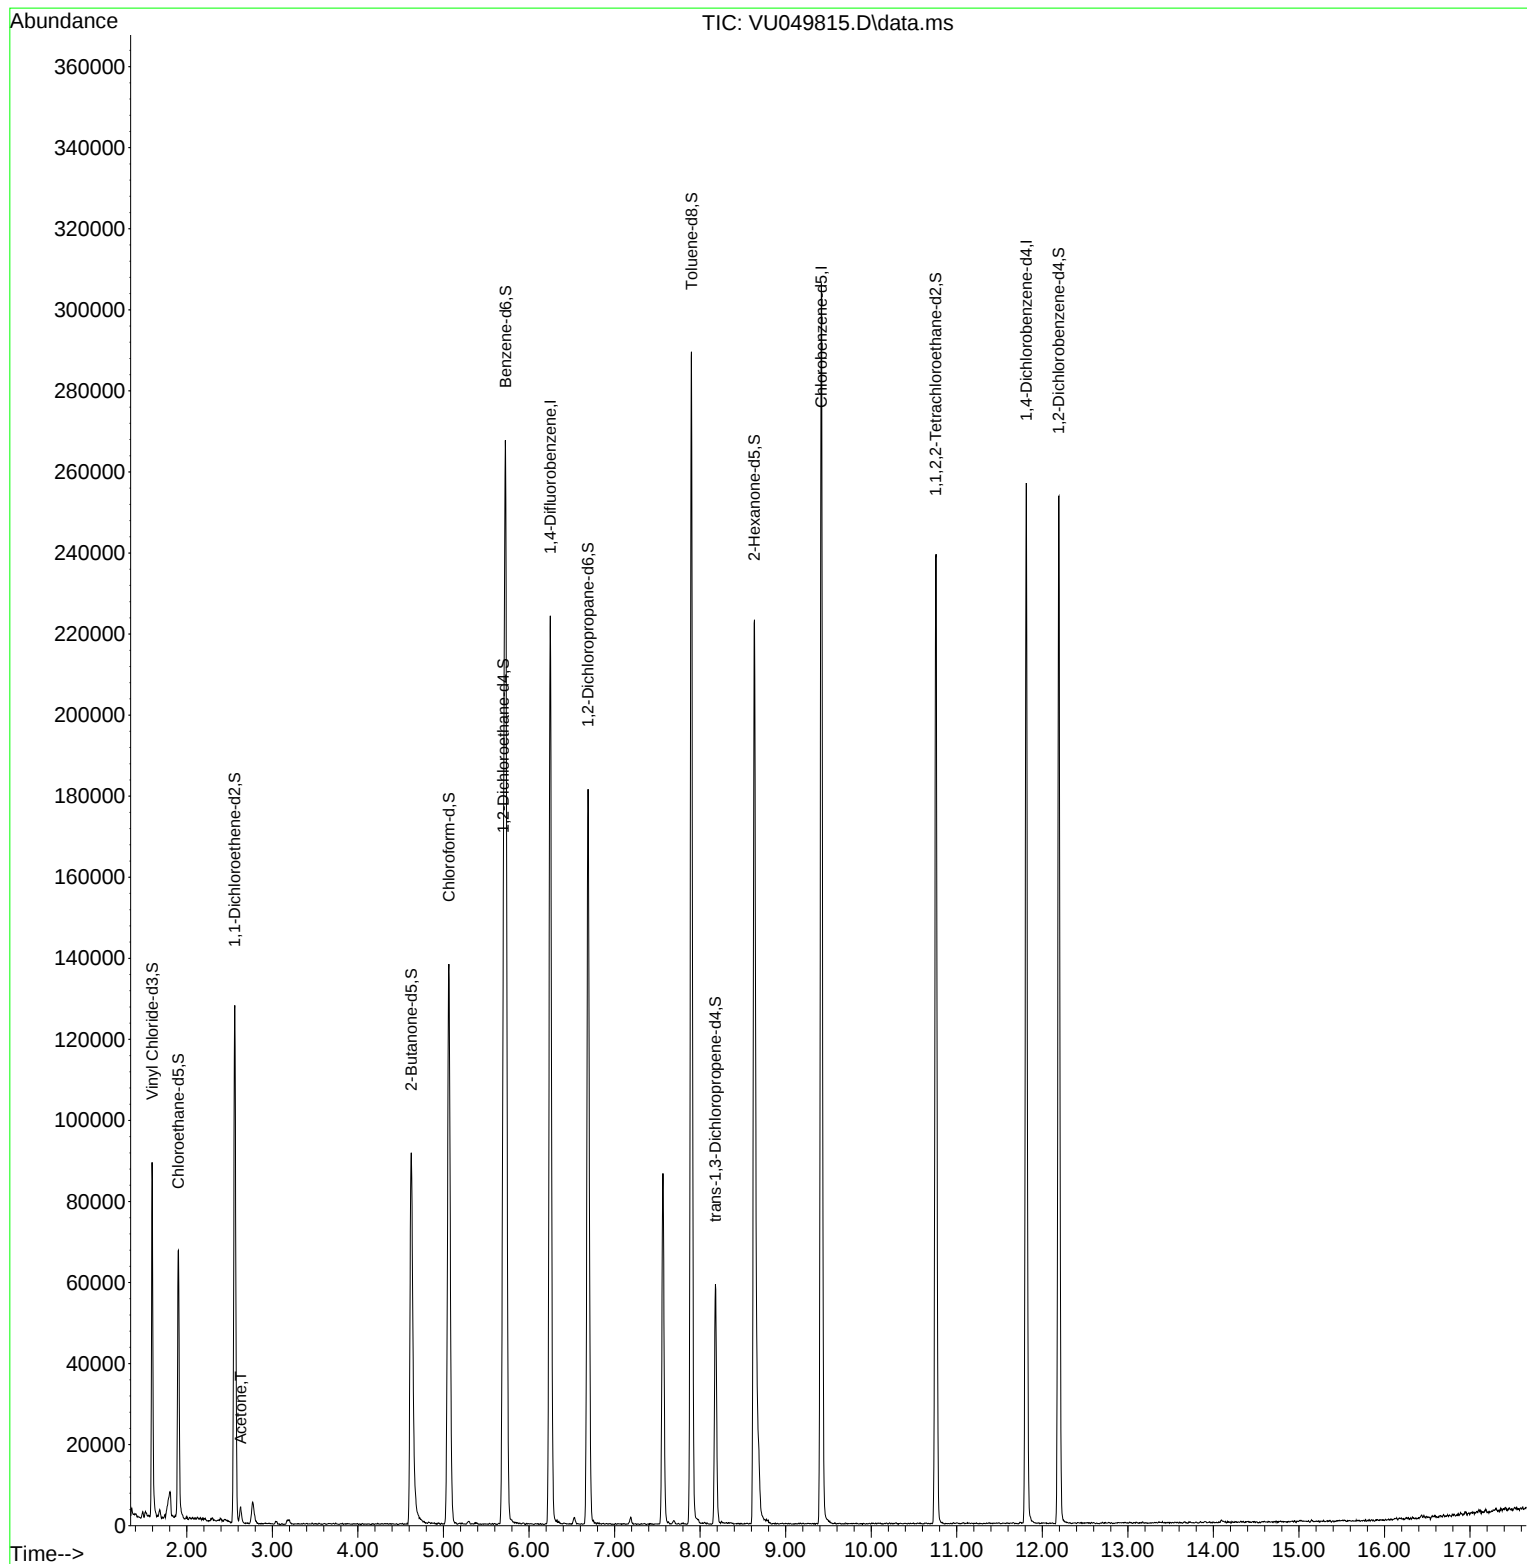

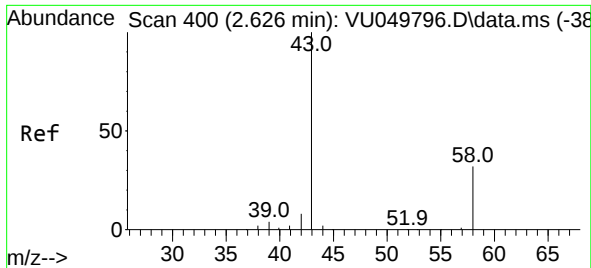

#13
 Acetone
 Concen: 4.050 ug/L
 RT: 2.629 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: VU049815.D
 Acq: 20 Jul 2022 20:24

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUN1

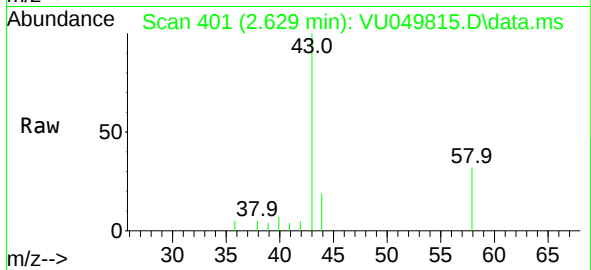

Tgt Ion: 43 Resp: 4741
 Ion Ratio Lower Upper
 43 100
 58 24.8 0.0 61.4

