

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
 Data File : VU049797.D
 Acq On : 20 Jul 2022 10:28
 Operator : SY/MD
 Sample : VU0720MBL01
 Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK162

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049797.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	50	rVB3	1741	1660	0.21%	0.029%
2	1.520	50	56	63	rBV2	2196	2906	0.37%	0.050%
3	1.597	72	80	96	rBV	99862	117327	14.74%	2.021%
4	1.903	166	175	193	rVB	78220	103595	13.02%	1.784%
5	2.318	302	304	308	rVB3	736	405	0.05%	0.007%
6	2.562	368	380	397	rVB	148241	237433	29.84%	4.089%
7	2.629	397	401	402	rBV	367	227	0.03%	0.004%
8	2.694	418	421	425	rBV	222	166	0.02%	0.003%
9	2.752	435	439	440	rBV2	293	170	0.02%	0.003%
10	2.787	446	450	463	rVB3	641	1121	0.14%	0.019%
11	3.047	521	531	543	rVB4	1685	2746	0.35%	0.047%
12	3.096	543	546	550	rBV	197	161	0.02%	0.003%
13	3.211	580	582	585	rBV	206	150	0.02%	0.003%
14	3.273	597	601	604	rBV2	170	193	0.02%	0.003%
15	3.536	679	683	687	rVV	243	199	0.03%	0.003%
16	3.572	691	694	699	rVV2	197	198	0.02%	0.003%
17	3.613	702	707	710	rBV2	182	215	0.03%	0.004%
18	3.674	720	726	731	rVB	220	263	0.03%	0.005%
19	3.777	752	758	765	rVB2	285	533	0.07%	0.009%
20	3.826	769	773	776	rBV	159	168	0.02%	0.003%
21	4.080	848	852	854	rBV	260	212	0.03%	0.004%
22	4.337	928	932	935	rBV	186	193	0.02%	0.003%
23	4.408	950	954	960	rBV2	172	228	0.03%	0.004%
24	4.623	1006	1021	1056	rBV	92542	235920	29.65%	4.063%
25	4.986	1131	1134	1137	rVB2	220	149	0.02%	0.003%
26	5.063	1140	1158	1185	rBV	150255	328508	41.28%	5.657%
27	5.276	1220	1224	1225	rBV	520	375	0.05%	0.006%
28	5.292	1226	1229	1234	rVV3	881	806	0.10%	0.014%
29	5.372	1247	1254	1257	rBV3	494	524	0.07%	0.009%
30	5.517	1297	1299	1304	rBV2	215	150	0.02%	0.003%
31	5.616	1320	1330	1335	rVB2	186	320	0.04%	0.006%
32	5.655	1335	1342	1343	rBV	230	269	0.03%	0.005%
33	5.723	1343	1363	1391	rBV2	290578	795721	100.00%	13.703%
34	5.935	1425	1429	1430	rBV2	315	190	0.02%	0.003%
35	6.002	1447	1450	1455	rVB2	310	307	0.04%	0.005%
36	6.150	1493	1496	1503	rVB2	197	254	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
 Data File : VU049797.D
 Acq On : 20 Jul 2022 10:28
 Operator : SY/MD
 Sample : VU0720MBL01
 Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK162

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	6.247	1510	1526	1550	rBV	224387	431980	54.29%	7.439%
38	6.385	1567	1569	1574	rBV3	259	202	0.03%	0.003%
39	6.427	1579	1582	1588	rVB2	292	228	0.03%	0.004%
40	6.456	1588	1591	1598	rBV2	165	212	0.03%	0.004%
41	6.526	1606	1613	1616	rBV3	1780	2313	0.29%	0.040%
42	6.610	1634	1639	1645	rBV2	478	615	0.08%	0.011%
43	6.690	1649	1664	1684	rVV	197034	377649	47.46%	6.504%
44	6.800	1695	1698	1704	rBV3	665	659	0.08%	0.011%
45	6.864	1714	1718	1722	rBV2	175	184	0.02%	0.003%
46	7.034	1767	1771	1773	rBV	208	157	0.02%	0.003%
47	7.182	1811	1817	1828	rVB4	1412	2235	0.28%	0.038%
48	7.292	1842	1851	1854	rBV2	265	449	0.06%	0.008%
49	7.311	1854	1857	1861	rVB2	225	157	0.02%	0.003%
50	7.372	1874	1876	1882	rVB2	325	275	0.03%	0.005%
51	7.423	1887	1892	1895	rBV	204	205	0.03%	0.004%
52	7.565	1923	1936	1955	rBV	96988	170789	21.46%	2.941%
53	7.671	1965	1969	1971	rBV2	302	235	0.03%	0.004%
54	7.687	1971	1974	1982	rVB2	983	1022	0.13%	0.018%
55	7.793	1999	2007	2008	rBV3	836	795	0.10%	0.014%
56	7.896	2026	2039	2058	rBV	322191	556622	69.95%	9.586%
57	8.073	2091	2094	2097	rBV	210	178	0.02%	0.003%
58	8.179	2116	2127	2146	rBV	65791	112283	14.11%	1.934%
59	8.510	2224	2230	2236	rBV2	201	312	0.04%	0.005%
60	8.562	2242	2246	2251	rBV	285	199	0.03%	0.003%
61	8.636	2257	2269	2298	rBV2	236863	486484	61.14%	8.378%
62	8.890	2346	2348	2353	rBV2	218	185	0.02%	0.003%
63	8.915	2353	2356	2360	rVB	294	182	0.02%	0.003%
64	9.031	2388	2392	2396	rBV2	265	317	0.04%	0.005%
65	9.163	2429	2433	2443	rVB3	524	742	0.09%	0.013%
66	9.324	2480	2483	2492	rVB2	218	286	0.04%	0.005%
67	9.417	2498	2512	2537	rBV	309360	515546	64.79%	8.878%
68	9.562	2551	2557	2558	rBV2	660	561	0.07%	0.010%
69	9.697	2594	2599	2605	rVB3	683	868	0.11%	0.015%
70	10.092	2720	2722	2723	rVV	339	176	0.02%	0.003%
71	10.121	2727	2731	2736	rVB3	599	536	0.07%	0.009%
72	10.147	2736	2739	2742	rBV2	230	188	0.02%	0.003%
73	10.211	2756	2759	2761	rBV	243	155	0.02%	0.003%
74	10.279	2777	2780	2784	rVV2	322	228	0.03%	0.004%
75	10.446	2829	2832	2835	rVB2	320	217	0.03%	0.004%
76	10.484	2839	2844	2848	rBV3	447	549	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
 Data File : VU049797.D
 Acq On : 20 Jul 2022 10:28
 Operator : SY/MD
 Sample : VU0720MBL01
 Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK162

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	10.681	2901	2905	2913	rVB	293	376	0.05%	0.006%
78	10.755	2915	2928	2953	rVV	254140	409969	51.52%	7.060%
79	10.841	2953	2955	2960	rVB	250	177	0.02%	0.003%
80	10.967	2991	2994	2999	rBV2	221	159	0.02%	0.003%
81	11.082	3027	3030	3039	rVB	472	515	0.06%	0.009%
82	11.381	3120	3123	3126	rBV2	233	187	0.02%	0.003%
83	11.562	3175	3179	3182	rBV	203	174	0.02%	0.003%
84	11.748	3232	3237	3241	rBV2	698	789	0.10%	0.014%
85	11.812	3245	3257	3276	rBV	260163	418140	52.55%	7.201%
86	12.018	3318	3321	3325	rBV	314	250	0.03%	0.004%
87	12.192	3363	3375	3397	rBV	278116	446460	56.11%	7.689%
88	12.404	3438	3441	3444	rBV2	378	283	0.04%	0.005%
89	13.224	3689	3696	3703	rBV5	1434	1766	0.22%	0.030%
90	13.475	3772	3774	3777	rBV	232	148	0.02%	0.003%
91	13.761	3861	3863	3866	rVB2	348	196	0.02%	0.003%
92	13.848	3882	3890	3898	rBV3	3030	4628	0.58%	0.080%
93	14.089	3957	3965	3973	rBV2	8914	13401	1.68%	0.231%
94	14.217	4002	4005	4007	rBV2	406	261	0.03%	0.004%
95	14.269	4019	4021	4024	rVB2	384	216	0.03%	0.004%
96	14.333	4033	4041	4050	rBV6	3955	6089	0.77%	0.105%
97	14.751	4168	4171	4174	rBV2	232	178	0.02%	0.003%
98	14.854	4200	4203	4209	rBV2	363	326	0.04%	0.006%
99	15.918	4531	4534	4539	rBV3	544	577	0.07%	0.010%
100	16.352	4667	4669	4672	rBV	613	390	0.05%	0.007%




Sum of corrected areas: 5806792

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
Data File : VU049797.D
Acq On : 20 Jul 2022 10:28
Operator : SY/MD
Sample : VU0720MBL01
Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK162

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

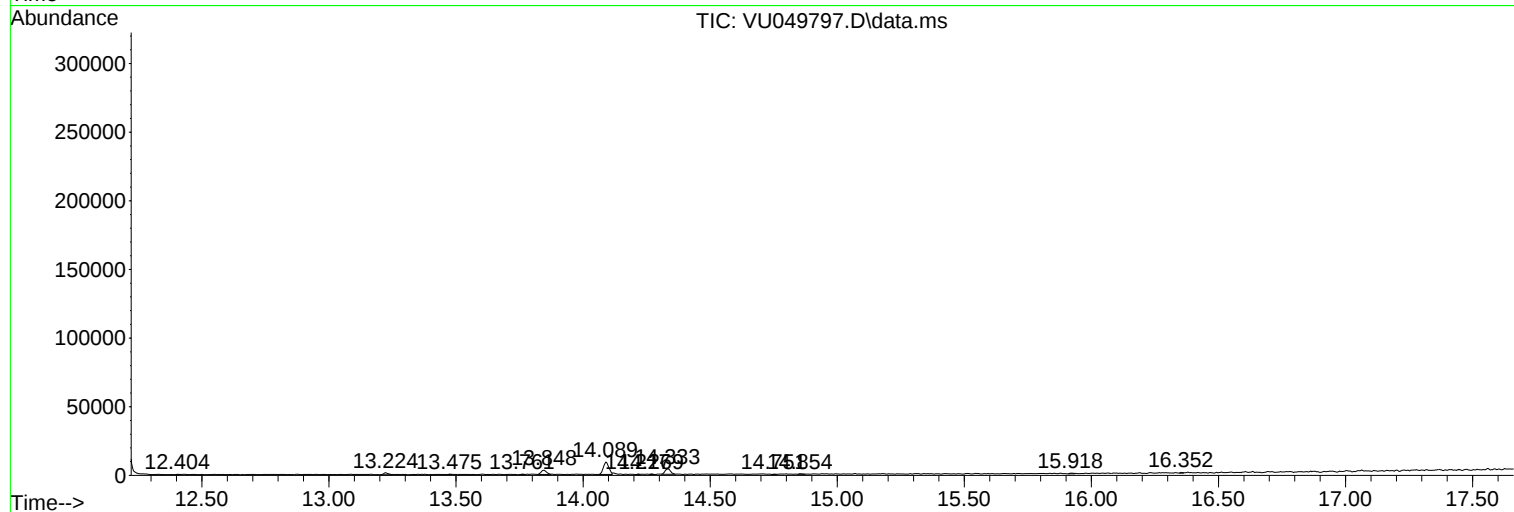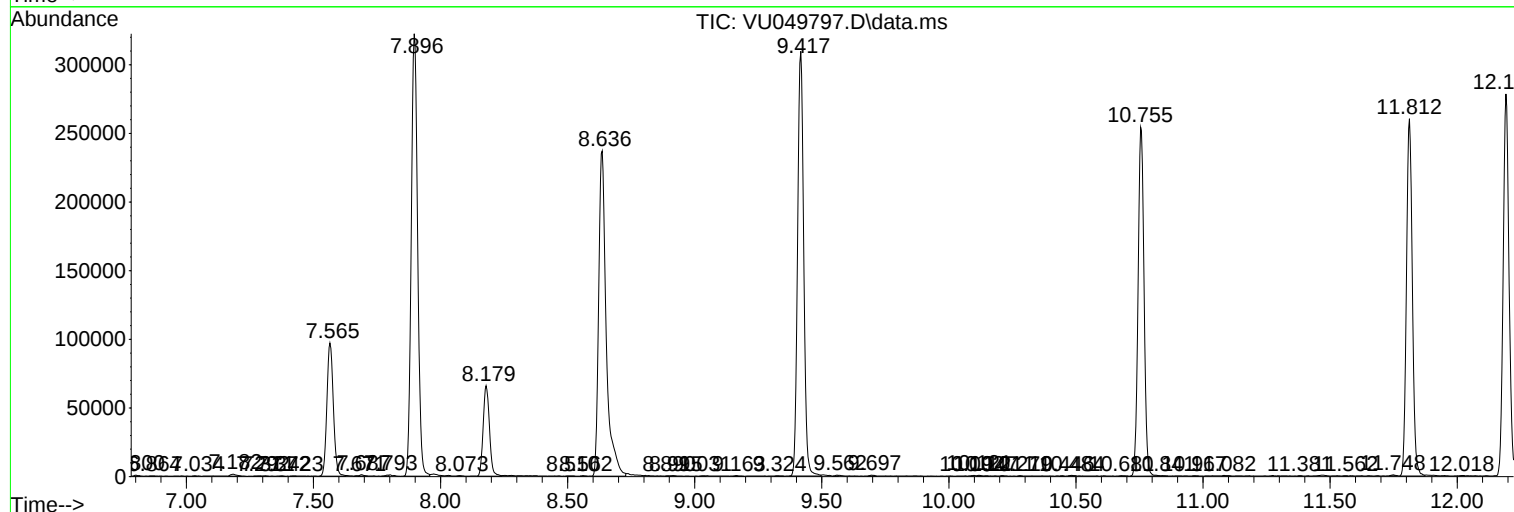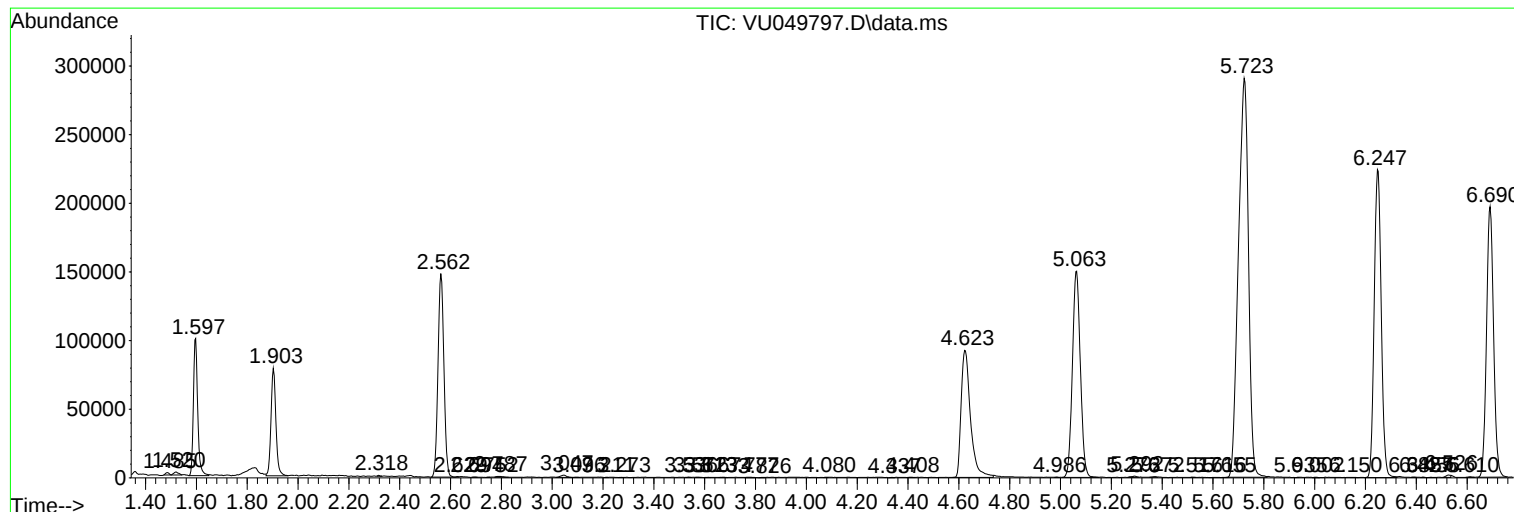

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
Data File : VU049797.D
Acq On : 20 Jul 2022 10:28
Operator : SY/MD
Sample : VU0720MBL01
Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK162

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
Data File : VU049797.D
Acq On : 20 Jul 2022 10:28
Operator : SY/MD
Sample : VU0720MBL01
Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK162

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------