

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
 Data File : VU049798.D
 Acq On : 20 Jul 2022 11:02
 Operator : SY/MD
 Sample : VU0720WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK163

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049798.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	42	45	50	rBV3	1128	1025	0.13%	0.018%
2	1.597	72	80	99	rBV	99989	115812	14.79%	1.997%
3	1.803	131	144	145	rBV7	3884	6138	0.78%	0.106%
4	1.906	167	176	190	rVB	75436	101007	12.90%	1.742%
5	2.388	323	326	331	rBV3	604	578	0.07%	0.010%
6	2.562	368	380	398	rBV	148722	237137	30.28%	4.089%
7	2.703	422	424	429	rVB	288	206	0.03%	0.004%
8	2.787	448	450	454	rVB2	315	192	0.02%	0.003%
9	2.848	461	469	475	rBV2	269	513	0.07%	0.009%
10	2.900	480	485	490	rVV2	325	326	0.04%	0.006%
11	3.047	521	531	538	rVB3	1323	2274	0.29%	0.039%
12	3.160	560	566	568	rBV2	352	347	0.04%	0.006%
13	3.173	568	570	575	rBV4	612	503	0.06%	0.009%
14	3.276	599	602	608	rBV2	186	235	0.03%	0.004%
15	3.417	640	646	655	rVB2	318	667	0.09%	0.012%
16	3.469	656	662	671	rBV2	394	847	0.11%	0.015%
17	3.739	742	746	749	rVV	268	220	0.03%	0.004%
18	3.877	784	789	795	rBV2	211	325	0.04%	0.006%
19	4.150	868	874	880	rVB	349	482	0.06%	0.008%
20	4.179	880	883	886	rBV2	237	238	0.03%	0.004%
21	4.237	897	901	908	rBV2	252	354	0.05%	0.006%
22	4.475	972	975	982	rBV2	156	170	0.02%	0.003%
23	4.626	1008	1022	1055	rBV	90384	227859	29.10%	3.929%
24	4.848	1089	1091	1095	rVB2	337	217	0.03%	0.004%
25	4.935	1114	1118	1121	rBV3	242	203	0.03%	0.004%
26	5.063	1138	1158	1181	rBV	145321	315509	40.29%	5.440%
27	5.288	1221	1228	1229	rBV2	694	673	0.09%	0.012%
28	5.375	1251	1255	1259	rBV3	414	452	0.06%	0.008%
29	5.420	1264	1269	1272	rBV	232	242	0.03%	0.004%
30	5.533	1301	1304	1309	rBV	211	174	0.02%	0.003%
31	5.584	1317	1320	1325	rBV2	171	175	0.02%	0.003%
32	5.726	1343	1364	1392	rBV2	286714	783030	100.00%	13.501%
33	5.835	1396	1398	1402	rVV4	340	299	0.04%	0.005%
34	5.858	1402	1405	1409	rVB2	351	228	0.03%	0.004%
35	5.932	1425	1428	1431	rBV	233	207	0.03%	0.004%
36	6.086	1473	1476	1480	rVB2	222	209	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
 Data File : VU049798.D
 Acq On : 20 Jul 2022 11:02
 Operator : SY/MD
 Sample : VU0720WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK163

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	6.112	1480	1484	1488	rBV2	310	283	0.04%	0.005%
38	6.195	1506	1510	1513	rVB	205	168	0.02%	0.003%
39	6.250	1513	1527	1543	rBV	225585	425239	54.31%	7.332%
40	6.375	1563	1566	1571	rVB2	353	274	0.03%	0.005%
41	6.488	1597	1601	1606	rVV2	264	198	0.03%	0.003%
42	6.530	1606	1614	1626	rVB5	1811	3111	0.40%	0.054%
43	6.616	1637	1641	1649	rBV2	187	246	0.03%	0.004%
44	6.690	1650	1664	1686	rBV	191540	370257	47.29%	6.384%
45	6.806	1693	1700	1702	rBV4	437	437	0.06%	0.008%
46	7.182	1809	1817	1818	rBV3	1042	947	0.12%	0.016%
47	7.565	1924	1936	1958	rBV	96974	167820	21.43%	2.893%
48	7.690	1969	1975	1983	rVB3	730	1087	0.14%	0.019%
49	7.800	2003	2009	2015	rBV3	397	602	0.08%	0.010%
50	7.899	2026	2040	2056	rBV	327180	557550	71.20%	9.613%
51	8.179	2114	2127	2150	rBV	66557	113806	14.53%	1.962%
52	8.349	2175	2180	2186	rBV2	363	513	0.07%	0.009%
53	8.517	2225	2232	2237	rBV2	222	321	0.04%	0.006%
54	8.565	2245	2247	2253	rVB2	199	179	0.02%	0.003%
55	8.636	2256	2269	2306	rBV2	232458	472801	60.38%	8.152%
56	8.854	2333	2337	2340	rBV3	298	187	0.02%	0.003%
57	9.009	2379	2385	2388	rBV	355	391	0.05%	0.007%
58	9.089	2405	2410	2417	rVB2	265	312	0.04%	0.005%
59	9.156	2428	2431	2434	rVV	281	178	0.02%	0.003%
60	9.375	2495	2499	2500	rBV2	330	204	0.03%	0.004%
61	9.417	2500	2512	2532	rVV	315680	524037	66.92%	9.035%
62	9.549	2551	2553	2556	rBV	315	217	0.03%	0.004%
63	9.568	2556	2559	2565	rVB3	465	440	0.06%	0.008%
64	10.076	2713	2717	2721	rBV	194	229	0.03%	0.004%
65	10.218	2754	2761	2763	rBV	236	292	0.04%	0.005%
66	10.317	2790	2792	2798	rVB	301	252	0.03%	0.004%
67	10.484	2841	2844	2848	rVB2	263	229	0.03%	0.004%
68	10.619	2883	2886	2890	rBV	298	279	0.04%	0.005%
69	10.709	2906	2914	2916	rBV2	352	486	0.06%	0.008%
70	10.758	2916	2929	2951	rVV	253213	409069	52.24%	7.053%
71	10.841	2951	2955	2958	rVB3	305	289	0.04%	0.005%
72	10.864	2958	2962	2964	rBV	220	194	0.02%	0.003%
73	10.935	2980	2984	2986	rBV2	276	250	0.03%	0.004%
74	11.012	3005	3008	3014	rBV2	189	192	0.02%	0.003%
75	11.044	3014	3018	3023	rBV2	252	366	0.05%	0.006%
76	11.205	3063	3068	3074	rBV2	245	346	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
 Data File : VU049798.D
 Acq On : 20 Jul 2022 11:02
 Operator : SY/MD
 Sample : VU0720WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK163

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	11.468	3147	3150	3154	rVV2	248	220	0.03%	0.004%
78	11.562	3174	3179	3181	rBV	196	203	0.03%	0.004%
79	11.745	3233	3236	3242	rVB2	433	404	0.05%	0.007%
80	11.812	3245	3257	3280	rBV	283229	452989	57.85%	7.810%
81	11.951	3298	3300	3305	rVB4	317	224	0.03%	0.004%
82	11.996	3310	3314	3320	rBV2	243	215	0.03%	0.004%
83	12.192	3363	3375	3401	rBV	289776	478134	61.06%	8.244%
84	12.417	3442	3445	3450	rBV	282	215	0.03%	0.004%
85	12.549	3481	3486	3487	rBV2	271	199	0.03%	0.003%
86	12.616	3504	3507	3512	rBV2	377	291	0.04%	0.005%
87	12.770	3551	3555	3560	rBV2	326	354	0.05%	0.006%
88	12.957	3609	3613	3616	rVB2	305	214	0.03%	0.004%
89	12.986	3618	3622	3625	rBV2	459	343	0.04%	0.006%
90	13.147	3668	3672	3675	rBV	261	257	0.03%	0.004%
91	13.176	3678	3681	3686	rBV2	364	296	0.04%	0.005%
92	13.230	3694	3698	3704	rVB2	478	459	0.06%	0.008%
93	13.359	3735	3738	3743	rBV2	380	326	0.04%	0.006%
94	13.803	3872	3876	3880	rVV2	361	342	0.04%	0.006%
95	13.844	3881	3889	3899	rVV7	1252	2165	0.28%	0.037%
96	14.092	3957	3966	3977	rBV2	3132	5293	0.68%	0.091%
97	14.266	4019	4020	4024	rBV2	293	216	0.03%	0.004%
98	14.333	4035	4041	4050	rVB5	1760	2480	0.32%	0.043%
99	14.719	4157	4161	4165	rBV3	381	399	0.05%	0.007%
100	15.124	4284	4287	4289	rBV2	458	338	0.04%	0.006%




Sum of corrected areas: 5799927

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
Data File : VU049798.D
Acq On : 20 Jul 2022 11:02
Operator : SY/MD
Sample : VU0720WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK163

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

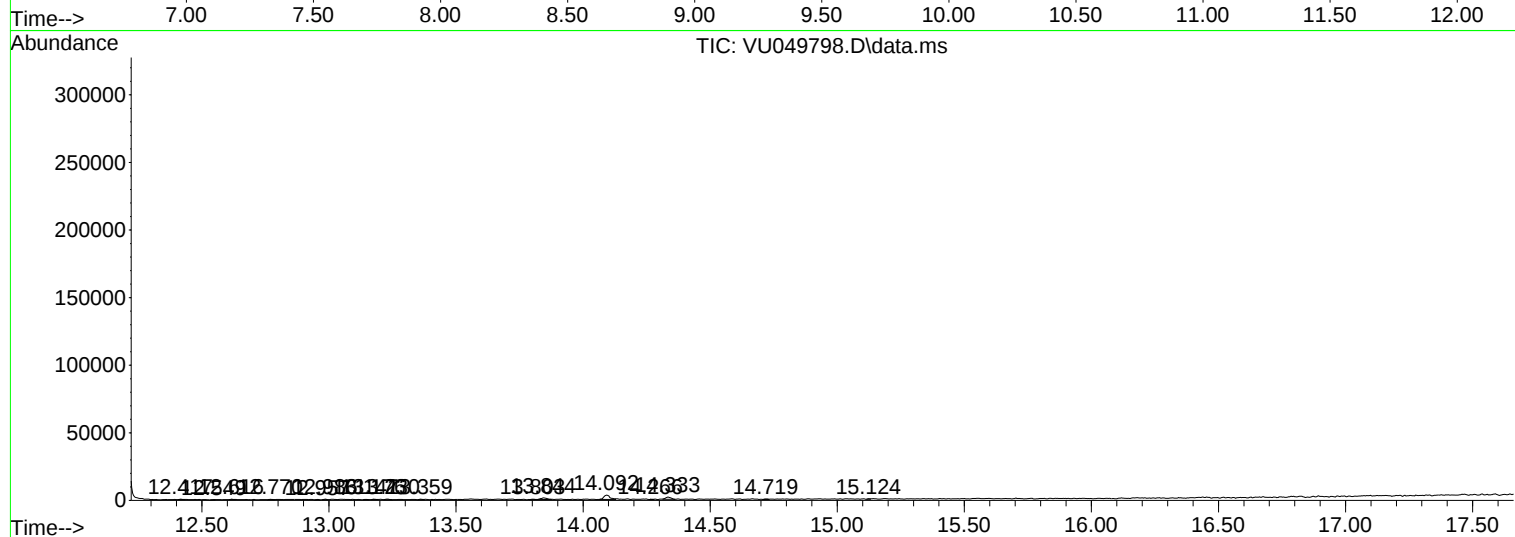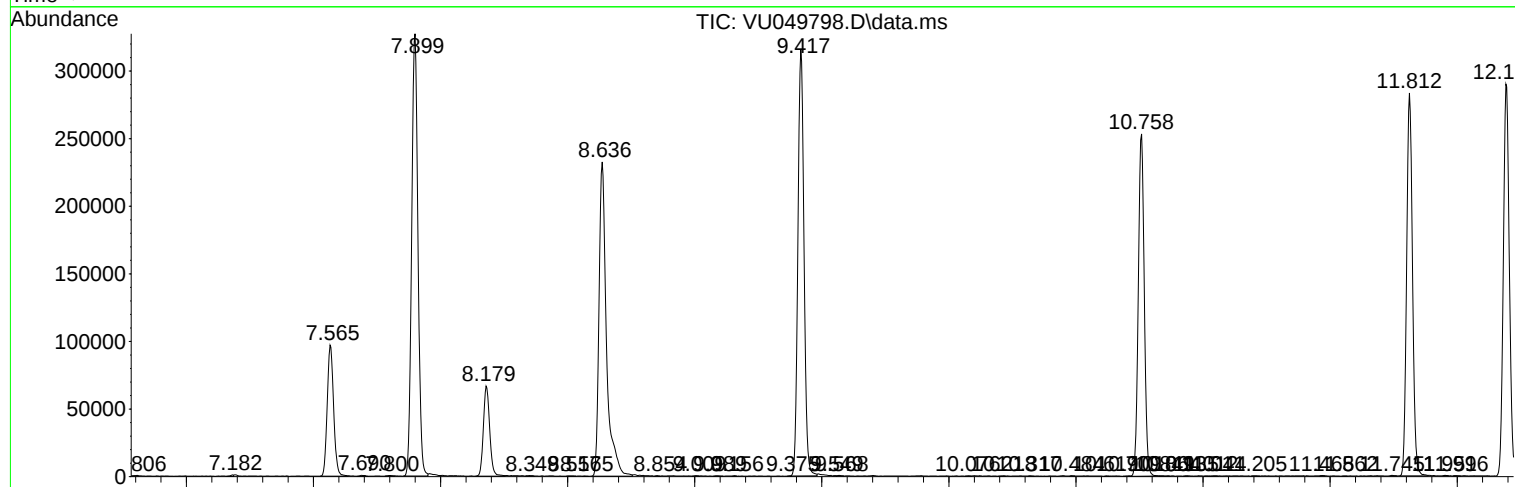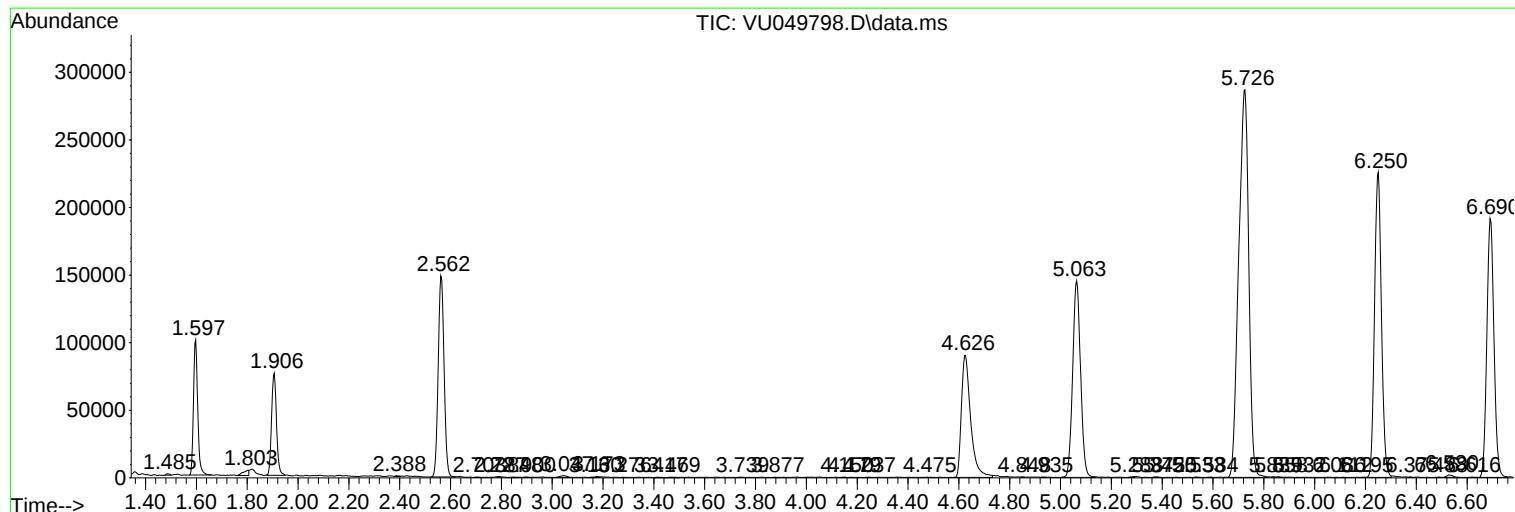

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
Data File : VU049798.D
Acq On : 20 Jul 2022 11:02
Operator : SY/MD
Sample : VU0720WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK163

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
Data File : VU049798.D
Acq On : 20 Jul 2022 11:02
Operator : SY/MD
Sample : VU0720WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK163

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc