

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
 Data File : VU049803.D
 Acq On : 20 Jul 2022 14:43
 Operator : SY/MD
 Sample : N3766-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ZD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049803.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	71	79	95	rBV	86628	103908	14.02%	1.834%
2	1.681	102	106	113	rVB2	2371	2671	0.36%	0.047%
3	1.903	165	175	192	rBV	68878	93429	12.61%	1.649%
4	2.443	341	343	344	rBV	334	168	0.02%	0.003%
5	2.562	368	380	393	rBV	135188	215275	29.04%	3.800%
6	2.629	393	401	415	rVB2	11514	20238	2.73%	0.357%
7	2.784	435	449	456	rBV4	2000	4536	0.61%	0.080%
8	3.044	524	530	534	rBV4	603	696	0.09%	0.012%
9	3.182	563	573	589	rBV2	2107	4370	0.59%	0.077%
10	3.533	679	682	685	rBV2	250	207	0.03%	0.004%
11	3.581	691	697	700	rBV2	336	380	0.05%	0.007%
12	4.060	839	846	852	rBV2	212	324	0.04%	0.006%
13	4.234	898	900	909	rVB2	390	438	0.06%	0.008%
14	4.272	909	912	915	rBV	340	276	0.04%	0.005%
15	4.439	961	964	967	rBV2	288	237	0.03%	0.004%
16	4.520	983	989	992	rBV2	316	390	0.05%	0.007%
17	4.623	1007	1021	1044	rBV	85193	207768	28.03%	3.667%
18	4.880	1099	1101	1106	rVB4	308	214	0.03%	0.004%
19	4.993	1132	1136	1140	rVB	283	215	0.03%	0.004%
20	5.063	1140	1158	1182	rBV	140225	299790	40.45%	5.291%
21	5.298	1220	1231	1238	rVB3	800	1618	0.22%	0.029%
22	5.343	1242	1245	1250	rVB	269	174	0.02%	0.003%
23	5.375	1250	1255	1261	rBV4	438	551	0.07%	0.010%
24	5.433	1271	1273	1276	rVV2	267	184	0.02%	0.003%
25	5.459	1278	1281	1283	rVV	216	172	0.02%	0.003%
26	5.472	1283	1285	1292	rVV2	278	354	0.05%	0.006%
27	5.549	1306	1309	1312	rVB2	268	176	0.02%	0.003%
28	5.571	1312	1316	1319	rBV	214	170	0.02%	0.003%
29	5.726	1343	1364	1389	rBV2	270250	741189	100.00%	13.082%
30	5.944	1429	1432	1436	rVB2	229	173	0.02%	0.003%
31	5.970	1437	1440	1443	rBV2	232	182	0.02%	0.003%
32	6.131	1484	1490	1497	rBV2	315	364	0.05%	0.006%
33	6.163	1497	1500	1503	rVB3	368	302	0.04%	0.005%
34	6.182	1503	1506	1509	rBV2	276	241	0.03%	0.004%
35	6.250	1513	1527	1545	rBV	230473	434657	58.64%	7.672%
36	6.404	1571	1575	1576	rBV2	246	182	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
 Data File : VU049803.D
 Acq On : 20 Jul 2022 14:43
 Operator : SY/MD
 Sample : N3766-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ZD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	6.529	1607	1614	1615	rBV2	1406	1491	0.20%	0.026%
38	6.568	1622	1626	1629	rVB2	331	241	0.03%	0.004%
39	6.690	1650	1664	1688	rBV	183797	355466	47.96%	6.274%
40	6.771	1688	1689	1693	rVB3	298	161	0.02%	0.003%
41	6.890	1720	1726	1732	rVB3	1331	1508	0.20%	0.027%
42	7.054	1771	1777	1783	rVV	368	413	0.06%	0.007%
43	7.127	1797	1800	1804	rBV3	407	393	0.05%	0.007%
44	7.189	1817	1819	1826	rVB3	1313	1216	0.16%	0.021%
45	7.427	1886	1893	1898	rBV2	270	452	0.06%	0.008%
46	7.565	1923	1936	1954	rBV2	90371	158757	21.42%	2.802%
47	7.687	1969	1974	1977	rBV2	907	835	0.11%	0.015%
48	7.761	1994	1997	1999	rBV	243	176	0.02%	0.003%
49	7.790	2003	2006	2007	rBV	261	178	0.02%	0.003%
50	7.899	2026	2040	2060	rBV	305233	529789	71.48%	9.351%
51	8.179	2116	2127	2144	rBV	63608	106301	14.34%	1.876%
52	8.398	2191	2195	2197	rBV3	376	189	0.03%	0.003%
53	8.465	2205	2216	2219	rBV4	1002	1151	0.16%	0.020%
54	8.635	2257	2269	2299	rBV2	225764	441047	59.51%	7.784%
55	8.790	2308	2317	2328	rVV4	12961	22157	2.99%	0.391%
56	8.832	2328	2330	2332	rVV	637	385	0.05%	0.007%
57	8.844	2332	2334	2340	rVB3	889	659	0.09%	0.012%
58	8.899	2347	2351	2356	rBV2	243	311	0.04%	0.005%
59	9.063	2398	2402	2404	rBV	247	160	0.02%	0.003%
60	9.417	2500	2512	2533	rBV	324857	537769	72.55%	9.492%
61	9.597	2564	2568	2570	rVB2	312	190	0.03%	0.003%
62	9.693	2595	2598	2601	rBV	241	191	0.03%	0.003%
63	9.777	2620	2624	2625	rBV	513	319	0.04%	0.006%
64	10.015	2695	2698	2700	rBV2	408	258	0.03%	0.005%
65	10.179	2746	2749	2755	rBV2	300	276	0.04%	0.005%
66	10.243	2762	2769	2778	rVB3	911	1635	0.22%	0.029%
67	10.298	2782	2786	2788	rBV	315	241	0.03%	0.004%
68	10.349	2796	2802	2807	rVB3	1136	1050	0.14%	0.019%
69	10.430	2819	2827	2832	rBV2	327	577	0.08%	0.010%
70	10.568	2862	2870	2878	rVV5	1554	2425	0.33%	0.043%
71	10.616	2881	2885	2890	rBV	329	345	0.05%	0.006%
72	10.758	2917	2929	2949	rVV	245244	392219	52.92%	6.923%
73	10.893	2967	2971	2979	rVB4	947	1177	0.16%	0.021%
74	11.044	3014	3018	3021	rBV2	202	208	0.03%	0.004%
75	11.089	3029	3032	3034	rBV2	277	213	0.03%	0.004%
76	11.362	3115	3117	3124	rVB4	434	464	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
 Data File : VU049803.D
 Acq On : 20 Jul 2022 14:43
 Operator : SY/MD
 Sample : N3766-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ZD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	11.478	3145	3153	3168	rVB4	3712	7141	0.96%	0.126%
78	11.693	3214	3220	3225	rBV5	1422	1371	0.18%	0.024%
79	11.812	3245	3257	3275	rBV	296055	468588	63.22%	8.271%
80	11.967	3302	3305	3310	rVV2	252	277	0.04%	0.005%
81	12.069	3326	3337	3350	rBV3	7758	15698	2.12%	0.277%
82	12.195	3363	3376	3395	rBV	291479	463397	62.52%	8.179%
83	12.262	3395	3397	3402	rVB4	740	505	0.07%	0.009%
84	12.574	3491	3494	3497	rVB3	312	198	0.03%	0.003%
85	12.597	3497	3501	3504	rBV3	463	354	0.05%	0.006%
86	12.770	3548	3555	3563	rVB3	1046	1697	0.23%	0.030%
87	12.819	3568	3570	3574	rVB2	346	195	0.03%	0.003%
88	12.848	3574	3579	3584	rBV3	481	497	0.07%	0.009%
89	12.893	3585	3593	3600	rVV5	2138	2561	0.35%	0.045%
90	12.960	3610	3614	3620	rBV2	308	335	0.05%	0.006%
91	13.349	3732	3735	3738	rBV2	269	212	0.03%	0.004%
92	14.098	3962	3968	3974	rBV2	704	855	0.12%	0.015%
93	14.169	3988	3990	3995	rVB2	391	222	0.03%	0.004%
94	14.336	4039	4042	4048	rBV3	512	465	0.06%	0.008%
95	14.507	4093	4095	4098	rVB2	426	216	0.03%	0.004%
96	14.526	4098	4101	4104	rBV2	463	401	0.05%	0.007%
97	14.786	4179	4182	4187	rBV	376	371	0.05%	0.007%
98	14.883	4209	4212	4214	rBV2	325	200	0.03%	0.004%
99	15.937	4538	4540	4544	rBV2	447	344	0.05%	0.006%
100	16.423	4689	4691	4694	rBV2	683	438	0.06%	0.008%




Sum of corrected areas: 5665750

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
Data File : VU049803.D
Acq On : 20 Jul 2022 14:43
Operator : SY/MD
Sample : N3766-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ZD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

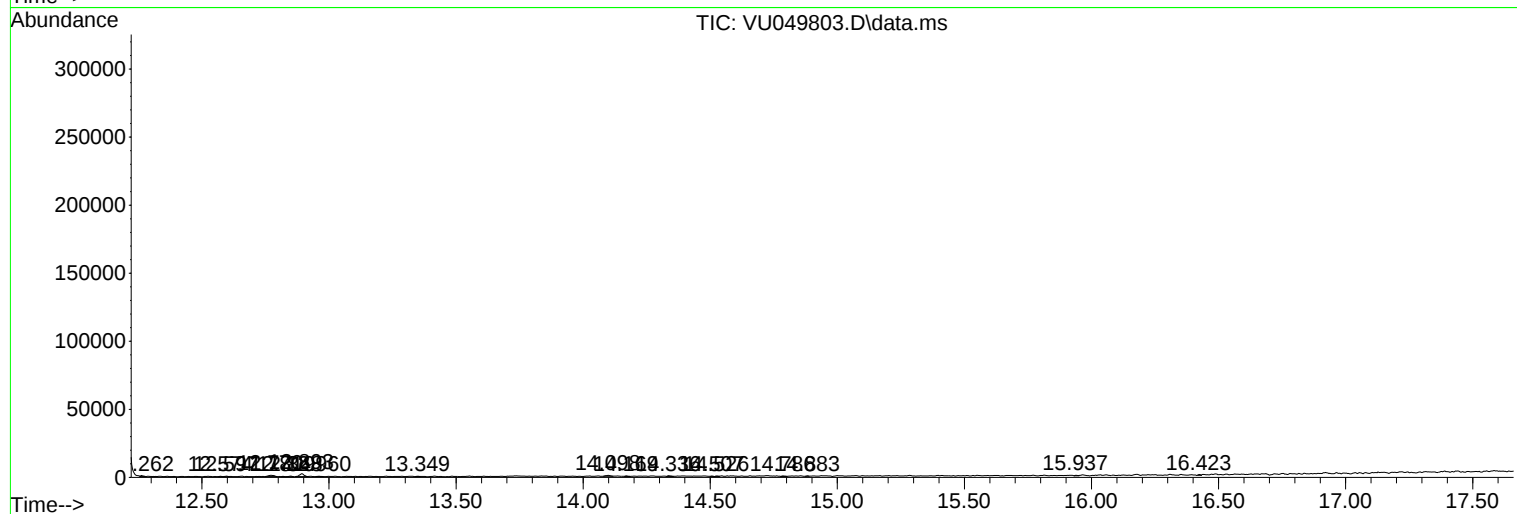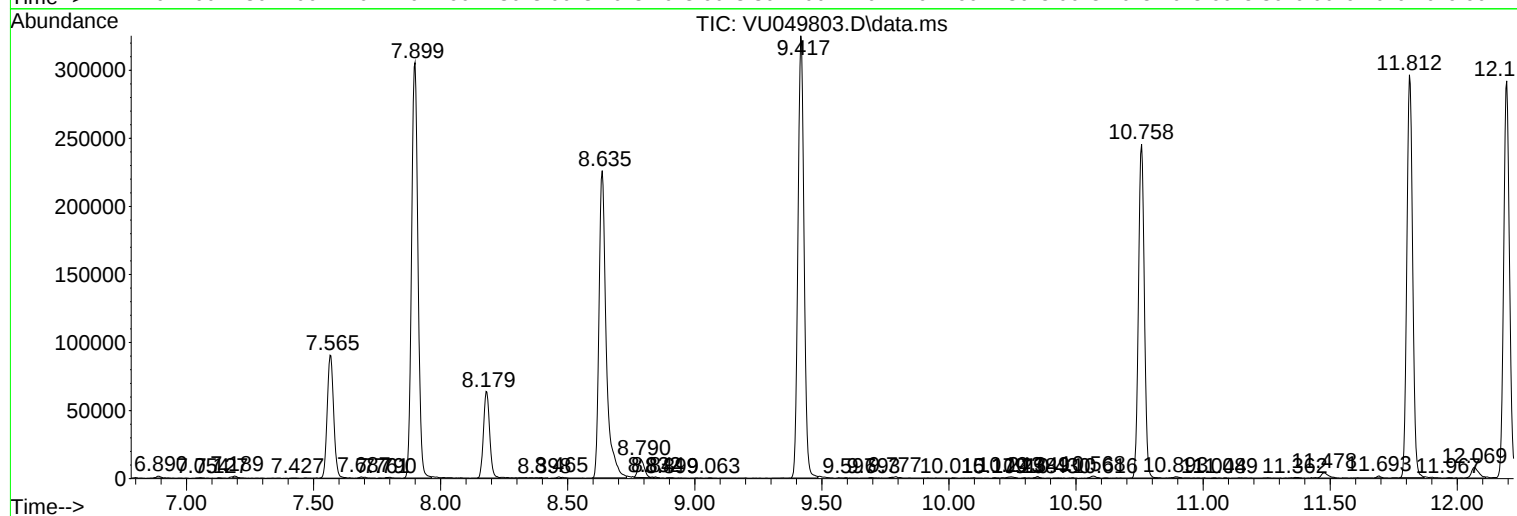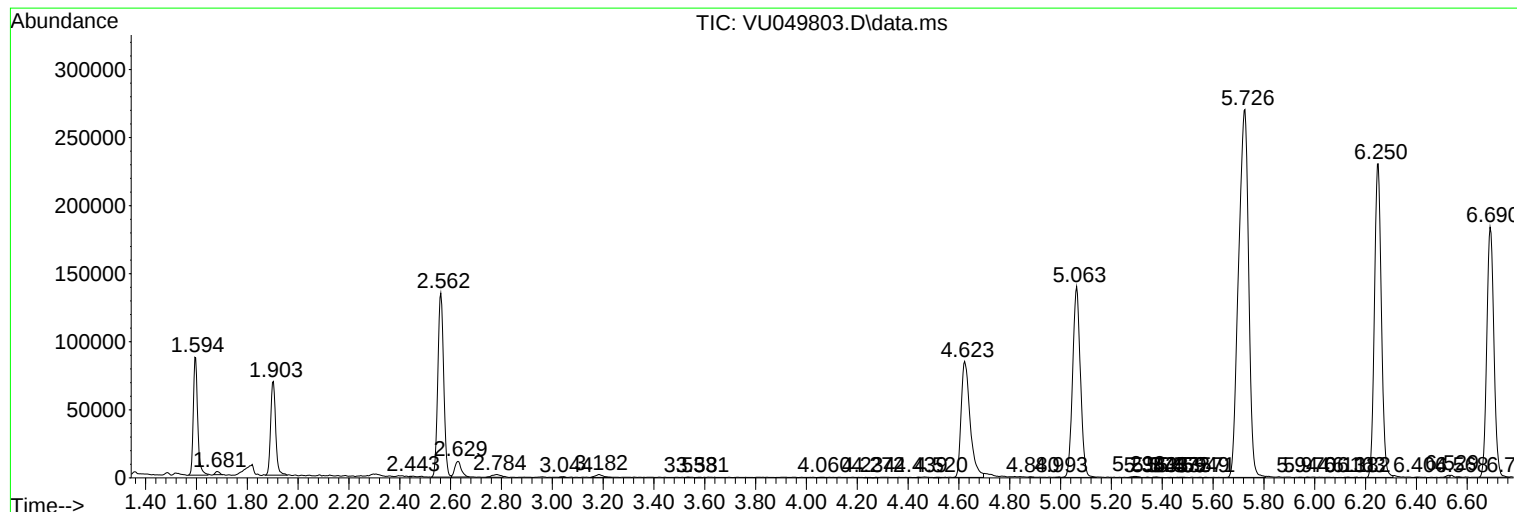

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
Data File : VU049803.D
Acq On : 20 Jul 2022 14:43
Operator : SY/MD
Sample : N3766-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ZD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
Data File : VU049803.D
Acq On : 20 Jul 2022 14:43
Operator : SY/MD
Sample : N3766-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ZD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------