

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
 Data File : VU049813.D
 Acq On : 20 Jul 2022 19:36
 Operator : SY/MD
 Sample : N3792-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049813.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	50	rBV2	1697	1518	0.20%	0.027%
2	1.594	72	79	100	rVB	90543	103489	13.93%	1.851%
3	1.681	100	106	116	rVB	4511	5530	0.74%	0.099%
4	1.797	130	142	149	rVB7	6646	13216	1.78%	0.236%
5	1.864	159	163	165	rBV3	809	813	0.11%	0.015%
6	1.903	166	175	193	rVB	69356	95427	12.85%	1.707%
7	2.240	278	280	287	rBV3	528	450	0.06%	0.008%
8	2.295	293	297	302	rVB3	680	570	0.08%	0.010%
9	2.453	344	346	353	rVB2	546	384	0.05%	0.007%
10	2.562	367	380	393	rBV	129483	210327	28.32%	3.762%
11	2.626	393	400	413	rVB	6276	9534	1.28%	0.171%
12	2.764	433	443	458	rBV2	5378	11190	1.51%	0.200%
13	2.957	497	503	512	rVB3	786	1115	0.15%	0.020%
14	3.041	524	529	539	rVB4	873	1098	0.15%	0.020%
15	3.125	552	555	559	rBV2	191	189	0.03%	0.003%
16	3.176	563	571	573	rBV2	1520	1782	0.24%	0.032%
17	3.276	597	602	606	rVB2	215	217	0.03%	0.004%
18	3.639	708	715	717	rBV2	143	187	0.03%	0.003%
19	3.797	758	764	767	rBV2	156	170	0.02%	0.003%
20	3.964	813	816	819	rVV	253	167	0.02%	0.003%
21	4.411	951	955	961	rBV2	202	274	0.04%	0.005%
22	4.440	961	964	969	rVB2	236	247	0.03%	0.004%
23	4.623	1007	1021	1047	rBV	96839	235614	31.73%	4.215%
24	4.880	1098	1101	1106	rVB	387	252	0.03%	0.005%
25	4.916	1106	1112	1116	rVB2	337	374	0.05%	0.007%
26	4.941	1116	1120	1122	rBV2	318	199	0.03%	0.004%
27	4.999	1135	1138	1141	rBV2	247	181	0.02%	0.003%
28	5.063	1141	1158	1180	rBV	139061	302662	40.75%	5.414%
29	5.231	1206	1210	1213	rBV3	280	187	0.03%	0.003%
30	5.285	1221	1227	1228	rBV	946	839	0.11%	0.015%
31	5.385	1255	1258	1265	rVB3	330	341	0.05%	0.006%
32	5.488	1284	1290	1292	rBV	246	176	0.02%	0.003%
33	5.723	1342	1363	1385	rBV2	271980	742658	100.00%	13.285%
34	5.835	1394	1398	1401	rVV2	337	278	0.04%	0.005%
35	5.864	1405	1407	1412	rVB2	378	229	0.03%	0.004%
36	5.973	1438	1441	1449	rVB2	278	224	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
 Data File : VU049813.D
 Acq On : 20 Jul 2022 19:36
 Operator : SY/MD
 Sample : N3792-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	6.144	1490	1494	1496	rBV	320	245	0.03%	0.004%
38	6.247	1513	1526	1548	rBV	231887	440001	59.25%	7.871%
39	6.404	1572	1575	1578	rBV3	276	227	0.03%	0.004%
40	6.449	1586	1589	1592	rBV2	314	184	0.02%	0.003%
41	6.465	1592	1594	1601	rVB2	342	262	0.04%	0.005%
42	6.530	1607	1614	1621	rBV5	1704	2627	0.35%	0.047%
43	6.690	1650	1664	1684	rVV	183532	354119	47.68%	6.335%
44	6.774	1688	1690	1692	rVV2	459	271	0.04%	0.005%
45	6.806	1696	1700	1706	rVB2	439	425	0.06%	0.008%
46	7.186	1810	1818	1830	rBV5	1590	2786	0.38%	0.050%
47	7.375	1872	1877	1880	rBV	172	176	0.02%	0.003%
48	7.475	1901	1908	1913	rBV2	135	207	0.03%	0.004%
49	7.565	1923	1936	1956	rBV	89297	156511	21.07%	2.800%
50	7.677	1968	1971	1973	rBV2	727	531	0.07%	0.009%
51	7.787	2000	2005	2006	rBV2	324	293	0.04%	0.005%
52	7.899	2026	2040	2056	rBV	290727	505005	68.00%	9.034%
53	8.179	2116	2127	2144	rBV	61387	102768	13.84%	1.838%
54	8.263	2151	2153	2158	rVB2	313	175	0.02%	0.003%
55	8.372	2184	2187	2191	rVV2	329	271	0.04%	0.005%
56	8.472	2214	2218	2223	rVB3	350	446	0.06%	0.008%
57	8.575	2247	2250	2252	rVB	388	227	0.03%	0.004%
58	8.632	2252	2268	2305	rBV2	235915	487899	65.70%	8.728%
59	8.848	2332	2335	2339	rBV2	335	236	0.03%	0.004%
60	8.906	2349	2353	2359	rBV2	315	258	0.03%	0.005%
61	9.012	2382	2386	2391	rBV	262	255	0.03%	0.005%
62	9.173	2431	2436	2438	rBV2	239	206	0.03%	0.004%
63	9.417	2499	2512	2538	rBV	313133	523202	70.45%	9.359%
64	9.565	2555	2558	2559	rBV	338	207	0.03%	0.004%
65	9.803	2628	2632	2635	rBV2	210	173	0.02%	0.003%
66	10.066	2709	2714	2717	rBV2	266	272	0.04%	0.005%
67	10.176	2744	2748	2750	rBV	257	217	0.03%	0.004%
68	10.224	2761	2763	2769	rVB2	220	185	0.02%	0.003%
69	10.266	2773	2776	2780	rBV2	205	222	0.03%	0.004%
70	10.353	2799	2803	2806	rBV	178	172	0.02%	0.003%
71	10.488	2841	2845	2853	rVB3	330	436	0.06%	0.008%
72	10.755	2916	2928	2950	rVV	248804	401168	54.02%	7.176%
73	10.893	2967	2971	2974	rBV2	335	305	0.04%	0.005%
74	11.211	3067	3070	3076	rVB	269	190	0.03%	0.003%
75	11.308	3097	3100	3107	rVB2	342	286	0.04%	0.005%
76	11.343	3107	3111	3114	rBV	254	219	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
 Data File : VU049813.D
 Acq On : 20 Jul 2022 19:36
 Operator : SY/MD
 Sample : N3792-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBUM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	11.404	3127	3130	3137	rVB2	245	266	0.04%	0.005%
78	11.449	3137	3144	3146	rBV2	230	279	0.04%	0.005%
79	11.677	3212	3215	3219	rBV	235	194	0.03%	0.003%
80	11.745	3231	3236	3240	rBV3	591	504	0.07%	0.009%
81	11.812	3242	3257	3276	rBV	271100	431225	58.07%	7.714%
82	12.127	3352	3355	3360	rBV2	314	222	0.03%	0.004%
83	12.195	3363	3376	3393	rBV	257857	422222	56.85%	7.553%
84	12.320	3412	3415	3417	rBV2	371	181	0.02%	0.003%
85	12.475	3460	3463	3466	rBV	284	202	0.03%	0.004%
86	12.767	3551	3554	3555	rBV	244	165	0.02%	0.003%
87	12.893	3591	3593	3597	rBV2	270	171	0.02%	0.003%
88	13.385	3744	3746	3752	rVB2	382	266	0.04%	0.005%
89	13.443	3762	3764	3768	rBV	274	262	0.04%	0.005%
90	13.658	3828	3831	3834	rBV2	231	170	0.02%	0.003%
91	13.844	3886	3889	3890	rBV3	498	278	0.04%	0.005%
92	14.092	3959	3966	3975	rBV3	2485	3662	0.49%	0.066%
93	14.150	3982	3984	3987	rBV3	328	228	0.03%	0.004%
94	14.336	4037	4042	4048	rVB3	1265	1441	0.19%	0.026%
95	14.420	4065	4068	4070	rBV2	344	213	0.03%	0.004%
96	14.459	4078	4080	4083	rBV	324	277	0.04%	0.005%
97	14.529	4099	4102	4105	rBV	367	221	0.03%	0.004%
98	15.844	4509	4511	4514	rBV3	422	304	0.04%	0.005%
99	16.002	4557	4560	4569	rBV3	652	693	0.09%	0.012%
100	16.523	4719	4722	4727	rBV4	703	562	0.08%	0.010%




Sum of corrected areas: 5590181

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
Data File : VU049813.D
Acq On : 20 Jul 2022 19:36
Operator : SY/MD
Sample : N3792-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

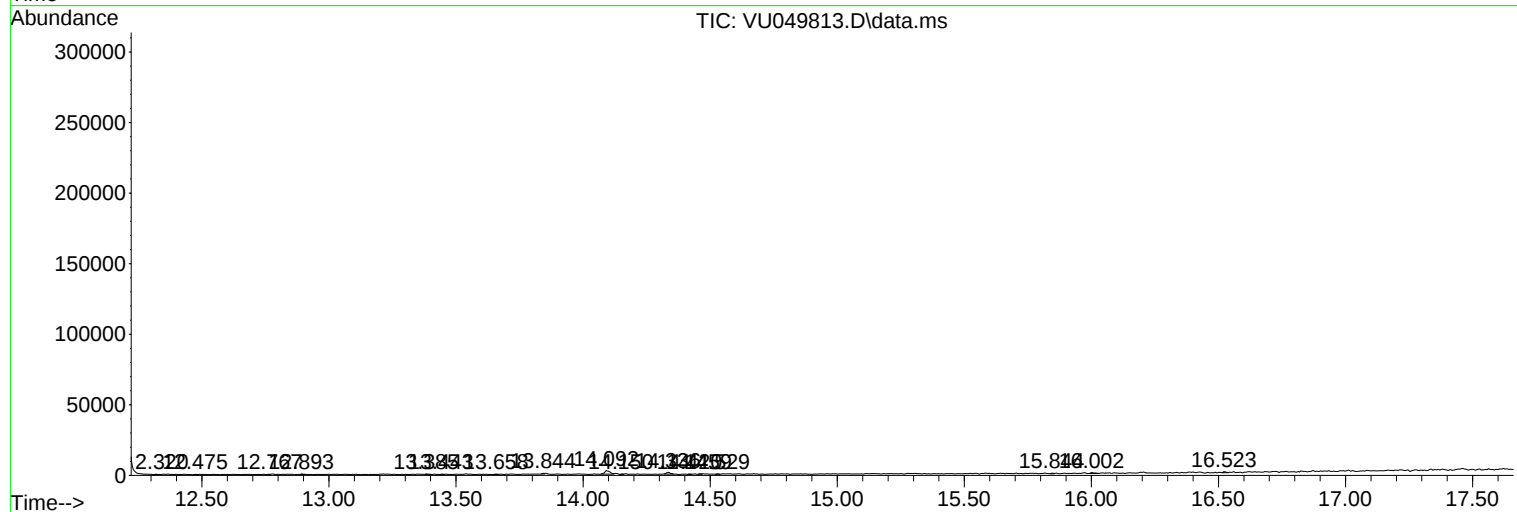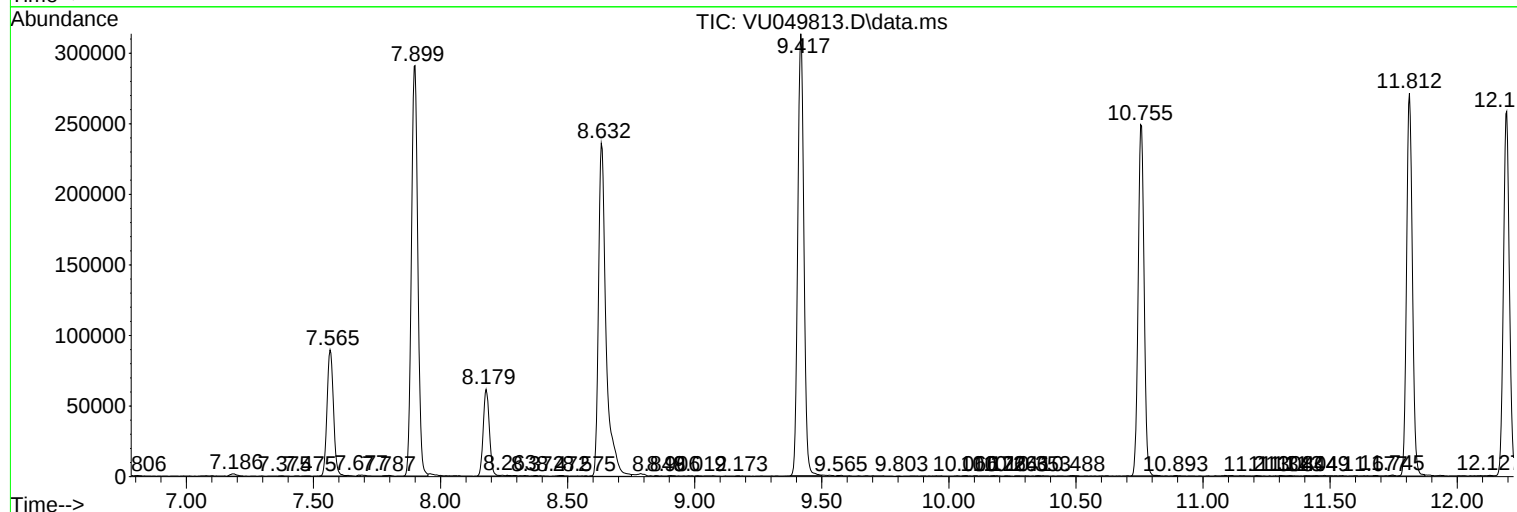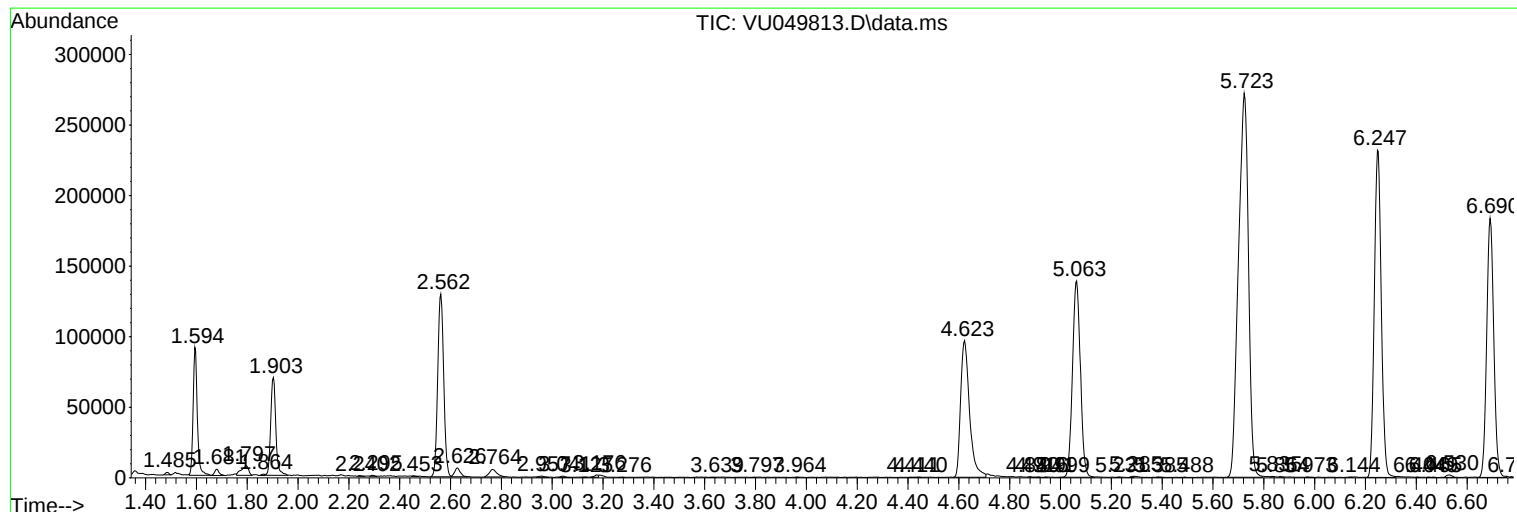

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
Data File : VU049813.D
Acq On : 20 Jul 2022 19:36
Operator : SY/MD
Sample : N3792-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
Data File : VU049813.D
Acq On : 20 Jul 2022 19:36
Operator : SY/MD
Sample : N3792-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBUM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc