
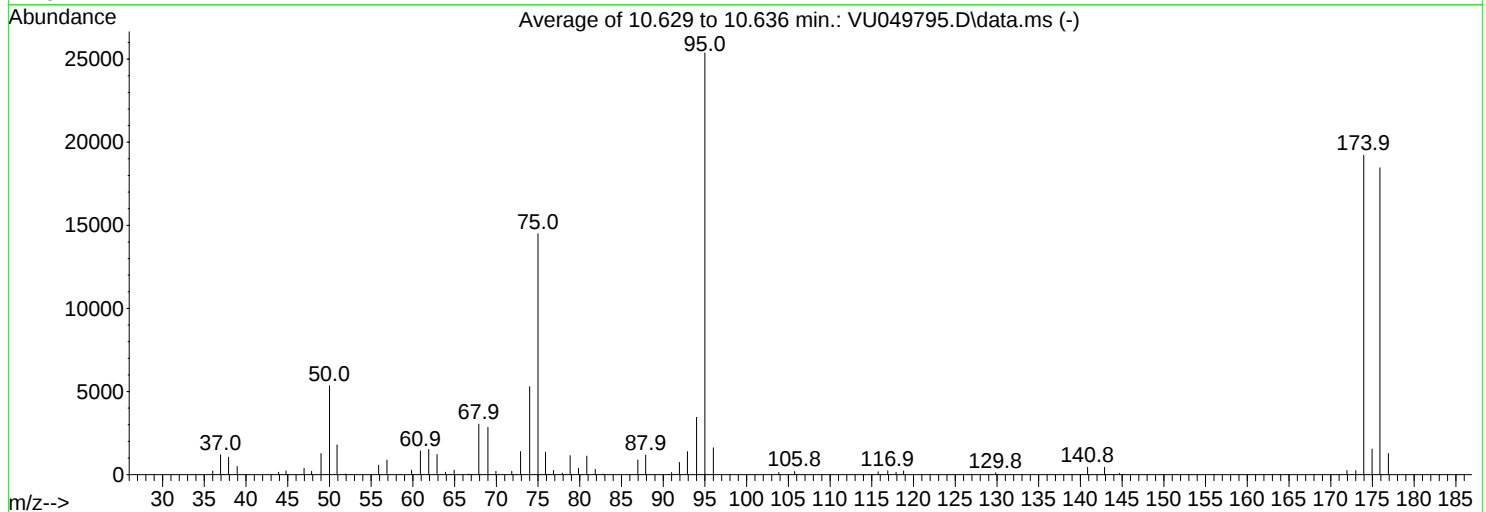


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072022\
Data File : VU049795.D
Acq On : 20 Jul 2022 09:00
Operator : SY/MD
Sample : BFB108
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB108

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Title : VOC Analysis
Last Update : Thu Jul 21 04:19:56 2022

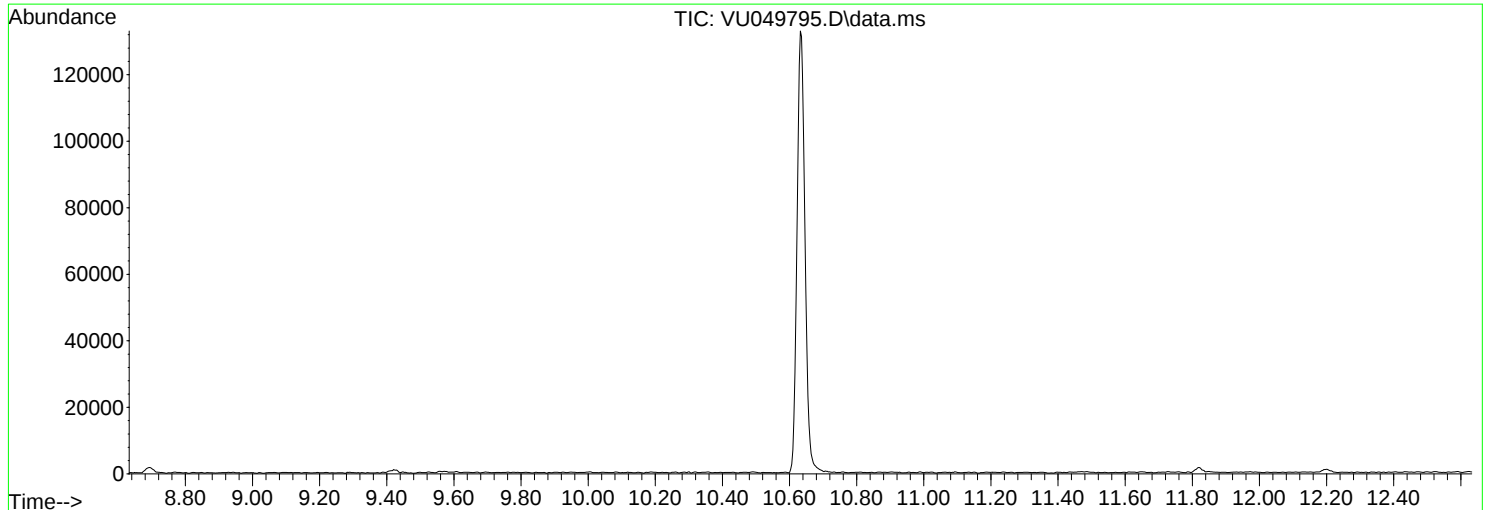

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	5349	PASS
75	95	30	80	57.1	14493	PASS
95	95	100	100	100.0	25376	PASS
96	95	5	9	6.4	1620	PASS
173	174	0.00	2	1.3	244	PASS
174	95	50	120	75.7	19211	PASS
175	174	5	9	8.0	1540	PASS
176	174	95	101	96.1	18459	PASS
177	176	5	9	6.9	1274	PASS

Scan 2878 (10.594 min): VU049795.D\data.ms
BFB108

m/z	Abundance
39.80	174.0
44.00	239.0

Instrument :
MSVOA_U
ClientSampleId :
BFB108

m/z	Abundance
36.00	222.0
36.90	1194.0
37.90	977.0
39.00	473.0
39.80	183.0
43.90	365.0
44.80	191.0
46.90	454.0
47.90	206.0
49.00	1272.0
50.00	5162.0
50.90	1629.0
55.90	583.0
56.90	840.0
59.80	267.0
60.90	1379.0
61.90	1539.0
62.90	1166.0
63.90	168.0
64.90	251.0
67.90	2947.0
69.00	2869.0
69.90	199.0
71.80	194.0
72.90	1306.0
74.00	4877.0
75.00	13799.0
75.90	1234.0
76.80	218.0
78.80	1091.0
79.80	396.0
80.80	1013.0
81.90	273.0
87.00	865.0
87.90	962.0
91.00	111.0
92.00	764.0
92.90	1504.0
94.00	3455.0
95.00	24096.0
96.00	1594.0
103.90	154.0
105.70	184.0
115.70	154.0
116.90	210.0
117.90	172.0
118.80	164.0
129.80	196.0
140.80	383.0
142.90	452.0
172.00	255.0
173.00	365.0
173.90	17776.0
174.90	1520.0
175.90	17424.0
176.90	1211.0

Instrument :
MSVOA_U
ClientSampleId :
BFB108

m/z	Abundance
36.00	232.0
36.90	1206.0
37.90	1075.0
38.90	487.0
39.80	161.0
43.90	368.0
44.80	224.0
46.90	394.0
47.90	211.0
49.00	1329.0
50.00	5499.0
50.90	1853.0
55.90	578.0
56.90	918.0
59.90	270.0
60.90	1484.0
61.90	1552.0
62.90	1249.0
63.90	145.0
65.00	278.0
67.90	3142.0
69.00	2957.0
70.00	221.0
71.90	212.0
72.90	1410.0
74.00	5501.0
75.00	14909.0
75.90	1397.0
76.90	252.0
77.90	134.0
78.80	1167.0
79.80	396.0
80.80	1137.0
81.80	323.0
82.80	105.0
87.00	905.0
87.90	1254.0
91.00	134.0
92.00	742.0
92.90	1429.0
94.00	3491.0
95.00	26064.0
96.00	1674.0
103.90	144.0
105.80	205.0
115.80	178.0
116.90	239.0
117.90	145.0
118.80	218.0
129.90	159.0
140.80	461.0
142.90	457.0
144.70	122.0
172.00	253.0
173.00	368.0
173.90	19744.0
175.00	1590.0
175.90	19040.0
176.90	1303.0

Instrument :
MSVOA_U
ClientSampleId :
BFB108

m/z	Abundance
36.00	203.0
37.00	1176.0
37.90	1111.0
38.90	514.0
39.80	152.0
43.90	403.0
44.80	243.0
47.00	310.0
47.80	186.0
49.00	1207.0
50.00	5386.0
50.90	1881.0
51.90	111.0
55.90	537.0
56.90	862.0
59.90	277.0
60.90	1399.0
61.90	1464.0
62.90	1228.0
63.90	117.0
65.00	287.0
66.70	109.0
67.90	3027.0
69.00	2722.0
70.00	201.0
71.90	190.0
72.90	1435.0
74.00	5506.0
75.00	14770.0
75.90	1430.0
76.90	296.0
77.90	153.0
78.90	1167.0
79.90	357.0
80.90	1190.0
81.80	354.0
86.90	891.0
87.90	1348.0
91.00	125.0
91.90	694.0
92.90	1213.0
94.00	3381.0
95.00	25968.0
96.00	1593.0
103.80	118.0
105.80	191.0
115.80	175.0
116.90	240.0
117.90	124.0
118.80	270.0
140.90	481.0
142.90	418.0
144.70	120.0
171.90	244.0
174.00	20112.0
174.90	1511.0
175.90	18912.0
176.90	1308.0

Instrument :
MSVOA_U
ClientSampleId :
BFB108