


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072023\
Data File : VU054825.D
Acq On : 20 Jul 2023 09:25
Operator : MD/SY
Sample : BFB031
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB031

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM072023.M
Title : TRACE VOA SOM01.0
Last Update : Fri Jul 21 01:10:23 2023

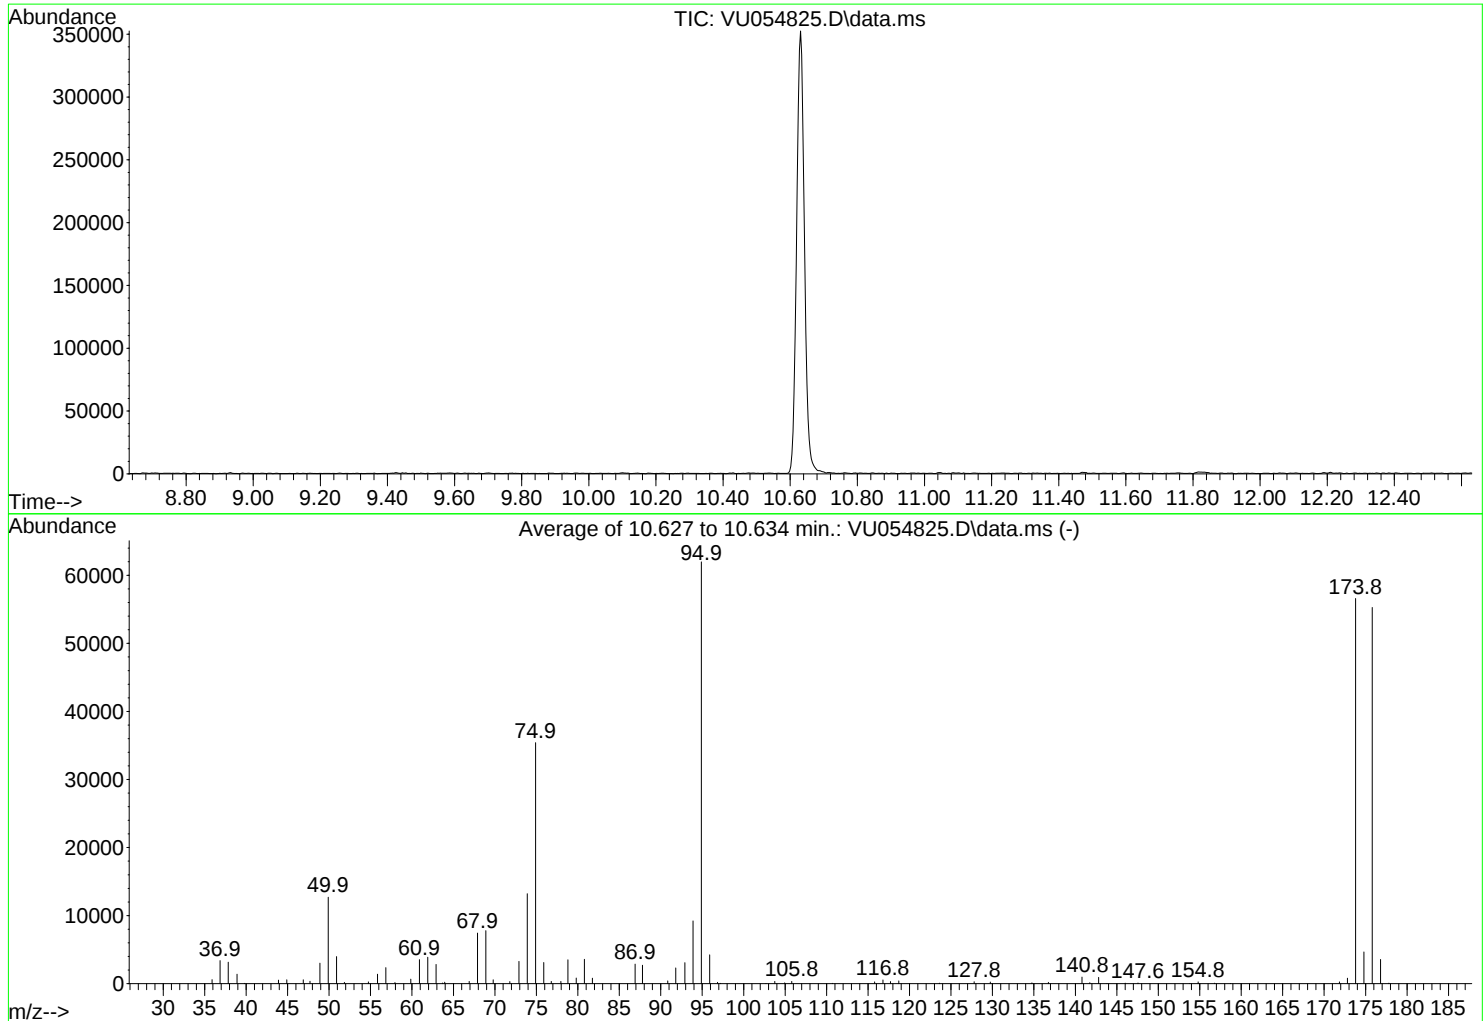

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.5	12704	PASS
75	95	30	80	57.1	35416	PASS
95	95	100	100	100.0	61981	PASS
96	95	5	9	6.8	4234	PASS
173	174	0.00	2	1.4	801	PASS
174	95	50	120	91.3	56603	PASS
175	174	5	9	8.2	4650	PASS
176	174	95	101	97.7	55275	PASS
177	176	5	9	6.4	3562	PASS

Scan 2892 (10.589 min): VU054825.D\data.ms
BFB031

m/z	Abundance
39.80	156.0
44.00	280.0

Instrument :
MSVOA_U
ClientSampleId :
BFB031

m/z	Abundance
35.90	513.0
36.90	3370.0
37.80	3388.0
38.90	1536.0
39.80	210.0
43.90	757.0
44.90	640.0
47.00	503.0
47.70	347.0
48.90	3129.0
49.90	12893.0
50.90	4140.0
51.80	161.0
54.80	288.0
55.90	1259.0
56.80	2358.0
57.90	128.0
59.80	807.0
60.90	3803.0
61.90	3815.0
62.90	2795.0
64.00	340.0
66.90	369.0
67.90	7292.0
68.90	8098.0
69.80	631.0
71.80	311.0
72.90	3234.0
73.90	13158.0
74.90	35216.0
75.90	2992.0
76.80	302.0
78.00	347.0
78.80	3291.0
79.80	809.0
80.80	3486.0
81.70	834.0
86.90	2838.0
87.80	2629.0
90.90	360.0
91.80	2203.0
92.90	3000.0
93.90	9262.0
94.90	61496.0
95.90	4205.0
96.80	144.0
97.20	115.0
103.80	378.0
105.00	113.0
105.80	382.0
115.80	248.0
116.80	594.0
117.70	341.0
118.70	419.0
123.60	106.0
127.70	300.0
129.80	234.0
134.80	120.0
136.70	137.0
140.80	979.0
141.70	152.0
142.80	913.0
143.80	111.0
146.00	102.0
147.60	141.0
154.80	208.0
171.80	320.0
172.80	735.0
173.80	55120.0
174.80	4369.0
175.80	53288.0
176.80	3612.0

Instrument :
MSVOA_U
ClientSampleId :
BFB031

m/z	Abundance
35.90	572.0
36.80	3537.0
37.80	3222.0
38.90	1431.0
39.80	219.0
43.90	800.0
44.90	550.0
46.90	543.0
47.70	362.0
48.90	3136.0
49.90	13145.0
50.90	4059.0
51.90	180.0
54.80	255.0
55.90	1420.0
56.80	2430.0
58.00	167.0
59.80	659.0
60.90	3650.0
61.90	4099.0
62.90	2926.0
63.90	320.0
66.90	366.0
67.90	7655.0
68.90	8094.0
69.80	576.0
71.80	321.0
72.90	3340.0
73.90	13640.0
74.90	36440.0
75.90	3259.0
76.80	351.0
78.00	368.0
78.80	3554.0
79.80	858.0
80.80	3628.0
81.80	823.0
86.90	2966.0
87.80	2743.0
90.90	397.0
91.80	2409.0
92.90	3201.0
93.90	9616.0
94.90	64096.0
95.90	4364.0
96.90	200.0
102.70	102.0
103.70	331.0
105.00	109.0
105.80	339.0
115.80	264.0
116.80	558.0
117.70	330.0
118.70	406.0
123.60	101.0
127.80	286.0
129.70	235.0
134.70	128.0
136.70	197.0
140.80	1022.0
141.80	139.0
142.80	949.0
146.00	118.0
147.50	122.0
154.80	255.0
156.80	112.0
158.70	101.0
171.80	268.0
172.80	868.0
173.80	58512.0
174.80	4909.0
175.80	57016.0
176.80	3691.0
177.80	107.0

Instrument :
MSVOA_U
ClientSampleId :
BFB031

m/z	Abundance
35.90	648.0
36.90	3249.0
37.90	2852.0
38.90	1199.0
39.80	183.0
43.90	823.0
44.90	489.0
46.80	618.0
47.70	373.0
48.90	2791.0
49.90	12074.0
50.90	3702.0
51.90	227.0
54.70	249.0
55.80	1458.0
56.90	2257.0
57.90	169.0
59.90	536.0
60.90	3133.0
61.90	3714.0
62.90	2754.0
63.70	270.0
66.90	258.0
67.90	7361.0
68.90	7174.0
69.80	506.0
71.80	319.0
72.90	3267.0
73.90	12832.0
74.90	34592.0
75.90	3057.0
76.80	350.0
77.90	297.0
78.80	3682.0
79.80	798.0
80.80	3617.0
81.80	742.0
86.90	2840.0
87.80	2734.0
90.80	426.0
91.80	2316.0
92.90	3040.0
93.90	8787.0
94.90	60352.0
95.90	4134.0
96.90	189.0
103.70	294.0
104.90	114.0
105.80	299.0
110.70	132.0
115.80	262.0
116.80	456.0
117.70	258.0
118.70	372.0
127.90	244.0
129.70	212.0
134.70	144.0
136.80	213.0
140.80	901.0
141.80	131.0
142.80	882.0
153.80	102.0
154.80	298.0
156.80	106.0
171.90	213.0
172.80	801.0
173.80	56176.0
174.80	4673.0
175.80	55520.0
176.80	3382.0
177.80	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB031