

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072118\
 Data File : VU025579.D
 Acq On : 21 Jul 2018 12:54
 Operator : MD/SY
 Sample : J4037-06ME
 Misc : 5.54g/5.0ml/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEY49ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.670	23	25	31	rVB3	387	298	0.03%	0.003%
2	0.703	31	35	37	rBV3	365	290	0.03%	0.003%
3	0.735	41	45	47	rBV2	298	235	0.02%	0.002%
4	0.802	63	66	70	rBV2	282	210	0.02%	0.002%
5	0.822	70	72	76	rVV	168	109	0.01%	0.001%
6	0.841	76	78	84	rVB3	254	224	0.02%	0.002%
7	0.870	84	87	89	rBV2	178	110	0.01%	0.001%
8	0.899	94	96	98	rBV2	297	129	0.01%	0.001%
9	0.928	102	105	107	rBV	250	116	0.01%	0.001%
10	0.950	110	112	115	rBV	200	91	0.01%	0.001%
11	0.986	121	123	124	rBV	113	27	0.00%	0.000%
12	1.005	127	129	133	rVB3	322	141	0.01%	0.001%
13	1.082	145	153	171	rBV	1055552	1123574	100.00%	11.814%
14	1.397	245	251	265	rVB	63407	76344	6.79%	0.803%
15	2.243	505	514	528	rVB	157331	237673	21.15%	2.499%
16	2.686	647	652	656	rBV4	1360	1535	0.14%	0.016%
17	2.831	684	697	713	rBV	11611	24601	2.19%	0.259%
18	2.937	725	730	733	rBV3	486	473	0.04%	0.005%
19	3.111	782	784	787	rVB3	156	77	0.01%	0.001%
20	3.137	787	792	795	rBV3	340	374	0.03%	0.004%
21	3.249	826	827	830	rBV2	290	154	0.01%	0.002%
22	3.275	830	835	836	rBV3	575	447	0.04%	0.005%
23	3.362	857	862	866	rBV3	451	538	0.05%	0.006%
24	3.410	871	877	879	rBV3	421	422	0.04%	0.004%
25	3.461	890	893	897	rBV2	378	223	0.02%	0.002%
26	3.522	910	912	915	rVB2	311	165	0.01%	0.002%
27	3.538	915	917	922	rVB2	182	138	0.01%	0.001%
28	3.561	922	924	926	rVB	165	54	0.00%	0.001%
29	3.667	955	957	960	rVB	258	129	0.01%	0.001%
30	3.754	982	984	985	rBV	176	62	0.01%	0.001%
31	3.818	998	1004	1008	rVB2	469	475	0.04%	0.005%
32	3.841	1008	1011	1014	rBV	386	229	0.02%	0.002%
33	3.889	1021	1026	1030	rBV4	394	429	0.04%	0.005%
34	3.940	1039	1042	1044	rVB	195	83	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072118\
 Data File : VU025579.D
 Acq On : 21 Jul 2018 12:54
 Operator : MD/SY
 Sample : J4037-06ME
 Misc : 5.54g/5.0ml/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEY49ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

35	3.998	1057	1060	1063	rBV2	195	130	0.01%	0.001%
36	4.053	1073	1077	1080	rBV	356	281	0.03%	0.003%
37	4.191	1105	1120	1162	rBV2	63592	207042	18.43%	2.177%
38	4.445	1197	1199	1201	rBV2	266	99	0.01%	0.001%
39	4.458	1201	1203	1205	rBV2	250	108	0.01%	0.001%
40	4.587	1240	1243	1245	rBV	286	187	0.02%	0.002%
41	4.648	1245	1262	1284	rVV	151840	362443	32.26%	3.811%
42	4.770	1296	1300	1301	rBV	509	283	0.03%	0.003%
43	4.809	1309	1312	1313	rBV2	356	196	0.02%	0.002%
44	4.866	1323	1330	1332	rBV3	726	639	0.06%	0.007%
45	4.960	1345	1359	1361	rBV5	2073	3553	0.32%	0.037%
46	5.046	1383	1386	1388	rBV	235	125	0.01%	0.001%
47	5.130	1410	1412	1414	rVB	193	78	0.01%	0.001%
48	5.227	1438	1442	1443	rBV2	418	230	0.02%	0.002%
49	5.336	1451	1476	1499	rBV2	293624	870496	77.48%	9.153%
50	5.564	1542	1547	1549	rBV2	294	278	0.02%	0.003%
51	5.612	1549	1562	1575	rVB6	2083	4881	0.43%	0.051%
52	5.821	1625	1627	1629	rVB	96	42	0.00%	0.000%
53	5.886	1629	1647	1672	rBV	377274	752304	66.96%	7.910%
54	6.082	1705	1708	1710	rBV2	240	154	0.01%	0.002%
55	6.136	1722	1725	1727	rVB2	202	106	0.01%	0.001%
56	6.178	1727	1738	1750	rBV8	4085	7471	0.66%	0.079%
57	6.246	1751	1759	1769	rBV4	1897	3702	0.33%	0.039%
58	6.333	1771	1786	1804	rBV	202451	410269	36.51%	4.314%
59	6.548	1851	1853	1854	rBV	198	93	0.01%	0.001%
60	6.612	1868	1873	1880	rBV2	240	248	0.02%	0.003%
61	6.760	1917	1919	1923	rVB2	165	98	0.01%	0.001%
62	6.812	1933	1935	1939	rVB2	349	247	0.02%	0.003%
63	6.847	1939	1946	1948	rBV3	1534	1771	0.16%	0.019%
64	6.992	1988	1991	1994	rVB3	484	312	0.03%	0.003%
65	7.059	2010	2012	2013	rBV	117	33	0.00%	0.000%
66	7.069	2013	2015	2017	rBV2	307	137	0.01%	0.001%
67	7.230	2052	2065	2086	rBV2	114004	212570	18.92%	2.235%
68	7.307	2086	2089	2093	rVB3	556	404	0.04%	0.004%
69	7.358	2101	2105	2109	rBV5	1174	1314	0.12%	0.014%
70	7.458	2133	2136	2138	rBV	507	331	0.03%	0.003%
71	7.567	2155	2170	2187	rBV	396915	700504	62.35%	7.365%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072118\
 Data File : VU025579.D
 Acq On : 21 Jul 2018 12:54
 Operator : MD/SY
 Sample : J4037-06ME
 Misc : 5.54g/5.0ml/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEY49ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
 Title : VOC Analysis

72	7.853	2247	2259	2275	rBV2	79694	146475	13.04%	1.540%
73	7.976	2294	2297	2300	rBV2	662	345	0.03%	0.004%
74	8.069	2323	2326	2328	rBV	220	161	0.01%	0.002%
75	8.185	2353	2362	2365	rBV3	11904	18295	1.63%	0.192%
76	8.230	2366	2376	2392	rVV	283758	482579	42.95%	5.074%
77	8.326	2394	2406	2427	rVB	270134	494138	43.98%	5.196%
78	8.898	2582	2584	2587	rBV	286	191	0.02%	0.002%
79	9.017	2617	2621	2625	rBV2	415	373	0.03%	0.004%
80	9.095	2632	2645	2670	rVB	533921	924130	82.25%	9.717%
81	9.268	2696	2699	2706	rBV3	559	466	0.04%	0.005%
82	9.371	2726	2731	2739	rBV4	793	976	0.09%	0.010%
83	9.474	2761	2763	2766	rBV	386	205	0.02%	0.002%
84	9.522	2776	2778	2779	rBV	359	183	0.02%	0.002%
85	9.779	2854	2858	2862	rBV4	769	828	0.07%	0.009%
86	9.886	2888	2891	2898	rVB3	379	338	0.03%	0.004%
87	10.439	3051	3063	3082	rBV	347174	549636	48.92%	5.779%
88	10.609	3109	3116	3128	rVB4	3566	6541	0.58%	0.069%
89	10.808	3175	3178	3180	rBV3	663	439	0.04%	0.005%
90	10.892	3201	3204	3205	rBV	397	188	0.02%	0.002%
91	11.487	3377	3389	3406	rBV	659350	1039301	92.50%	10.928%
92	11.866	3494	3507	3526	rBV	513230	830721	73.94%	8.735%
93	12.168	3598	3601	3604	rBV4	499	433	0.04%	0.005%
94	13.249	3933	3937	3939	rBV2	500	407	0.04%	0.004%


Sum of corrected areas: 9510687

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072118\
Data File : VU025579.D
Acq On : 21 Jul 2018 12:54
Operator : MD/SY
Sample : J4037-06ME
Misc : 5.54g/5.0ml/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEY49ME

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

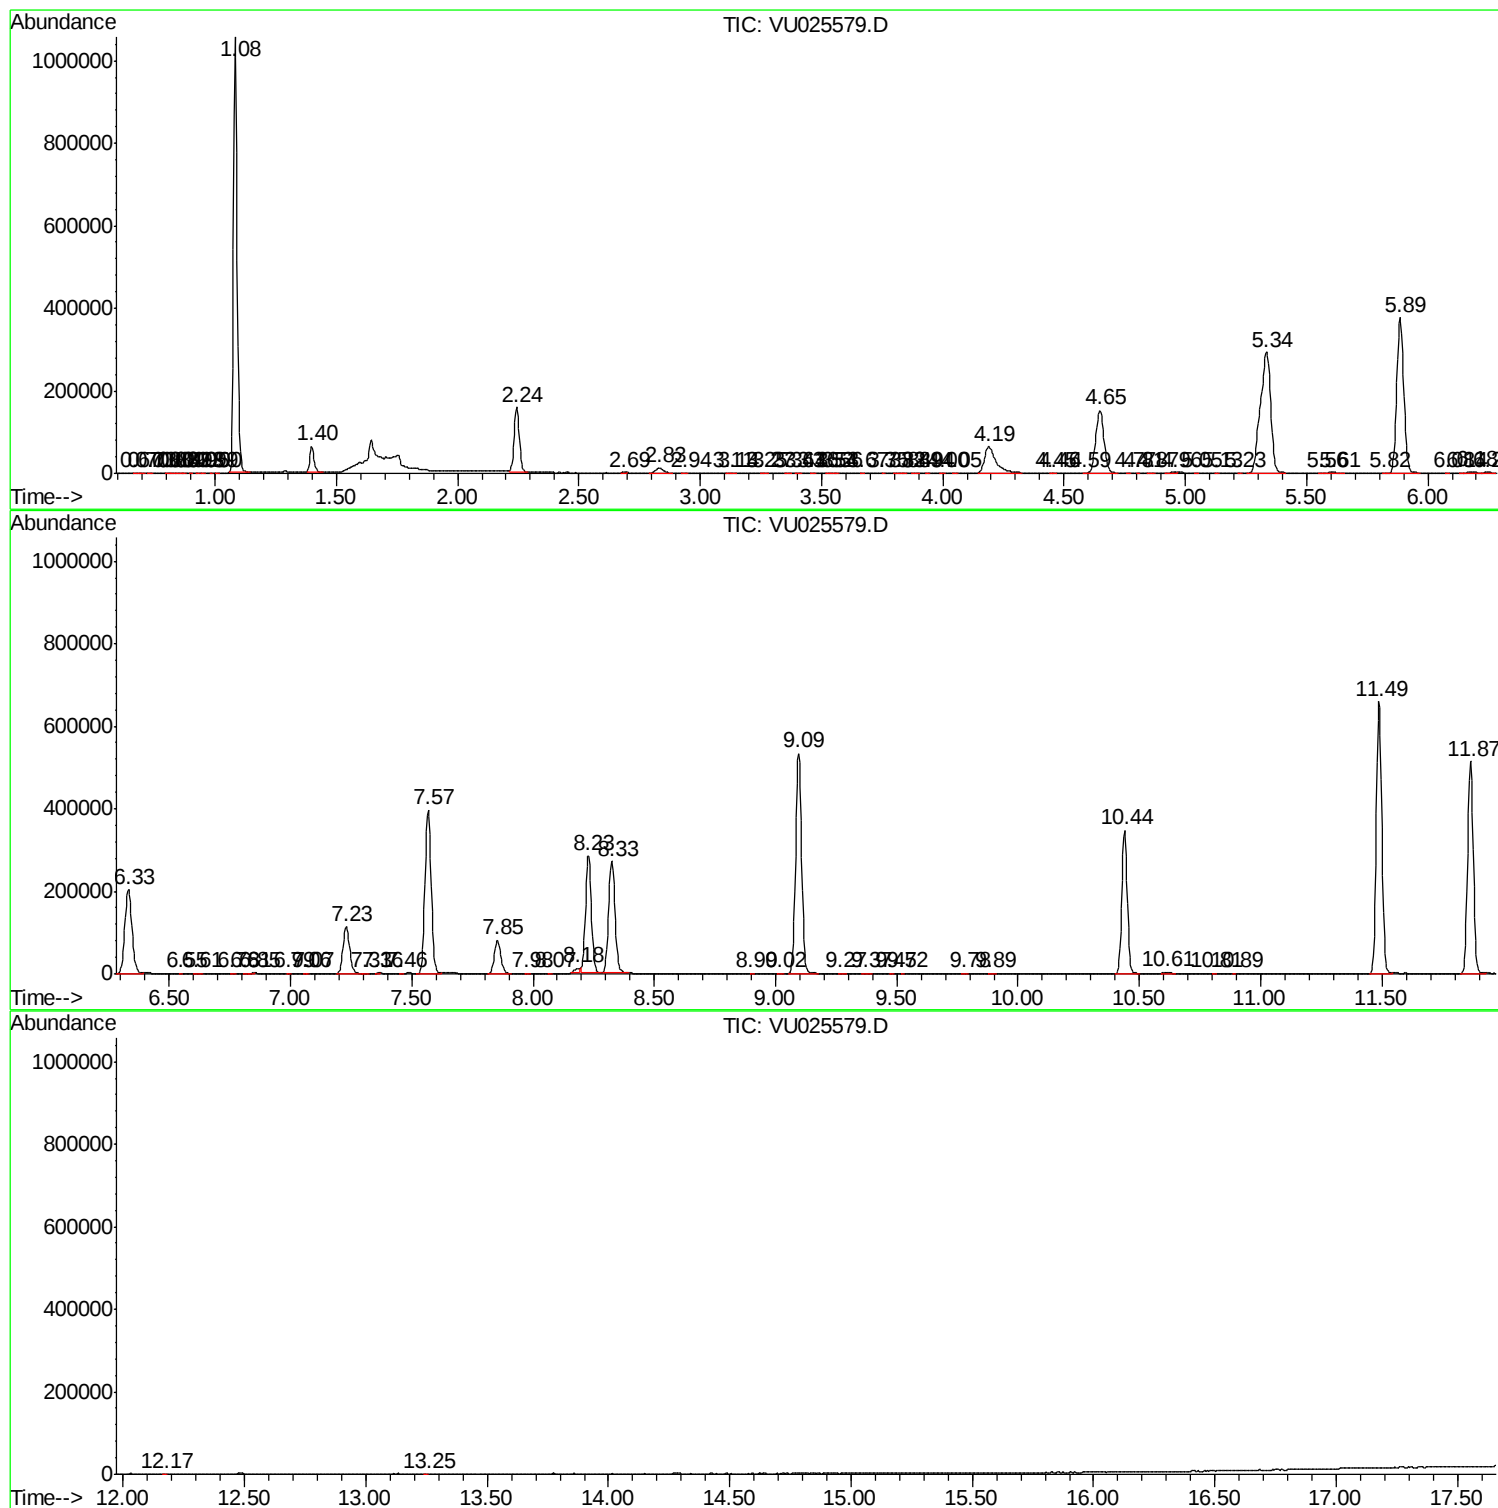

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072118\
Data File : VU025579.D
Acq On : 21 Jul 2018 12:54
Operator : MD/SY
Sample : J4037-06ME
Misc : 5.54g/5.0ml/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEY49ME

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU072118\
Data File : VU025579.D
Acq On : 21 Jul 2018 12:54
Operator : MD/SY
Sample : J4037-06ME
Misc : 5.54g/5.0ml/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEY49ME

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM072018WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc